

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081122\
 Data File : FB027891.D
 Signal(s) : FID2B.CH
 Acq On : 11 Aug 2022 10:37
 Operator : AJ/MA
 Sample : BSF0811S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0811S1

Integration File: Calibration.e
 Quant Time: Aug 12 05:20:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	246908	21.305 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	488837	27.021 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	530375	27.046 ng/ml
3) t n-Heptane	7.751	165570	8.594 ng/ml
4) t Benzene	7.889	207157	8.910 ng/ml
6) t Toluene	10.623	600224	27.372 ng/ml
7) t Ethylbenzene	13.059	186640	9.057 ng/ml
8) t m-Xylene	13.192	370095	18.086 ng/ml
9) t O-Xylene	13.919	359610	18.154 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	354303	18.169 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081122\
Data File : FB027891.D
Signal(s) : FID2B.CH
Acq On : 11 Aug 2022 10:37
Operator : AJ/MA
Sample : BSF0811S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0811S1

Integration File: Calibration.e
Quant Time: Aug 12 05:20:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

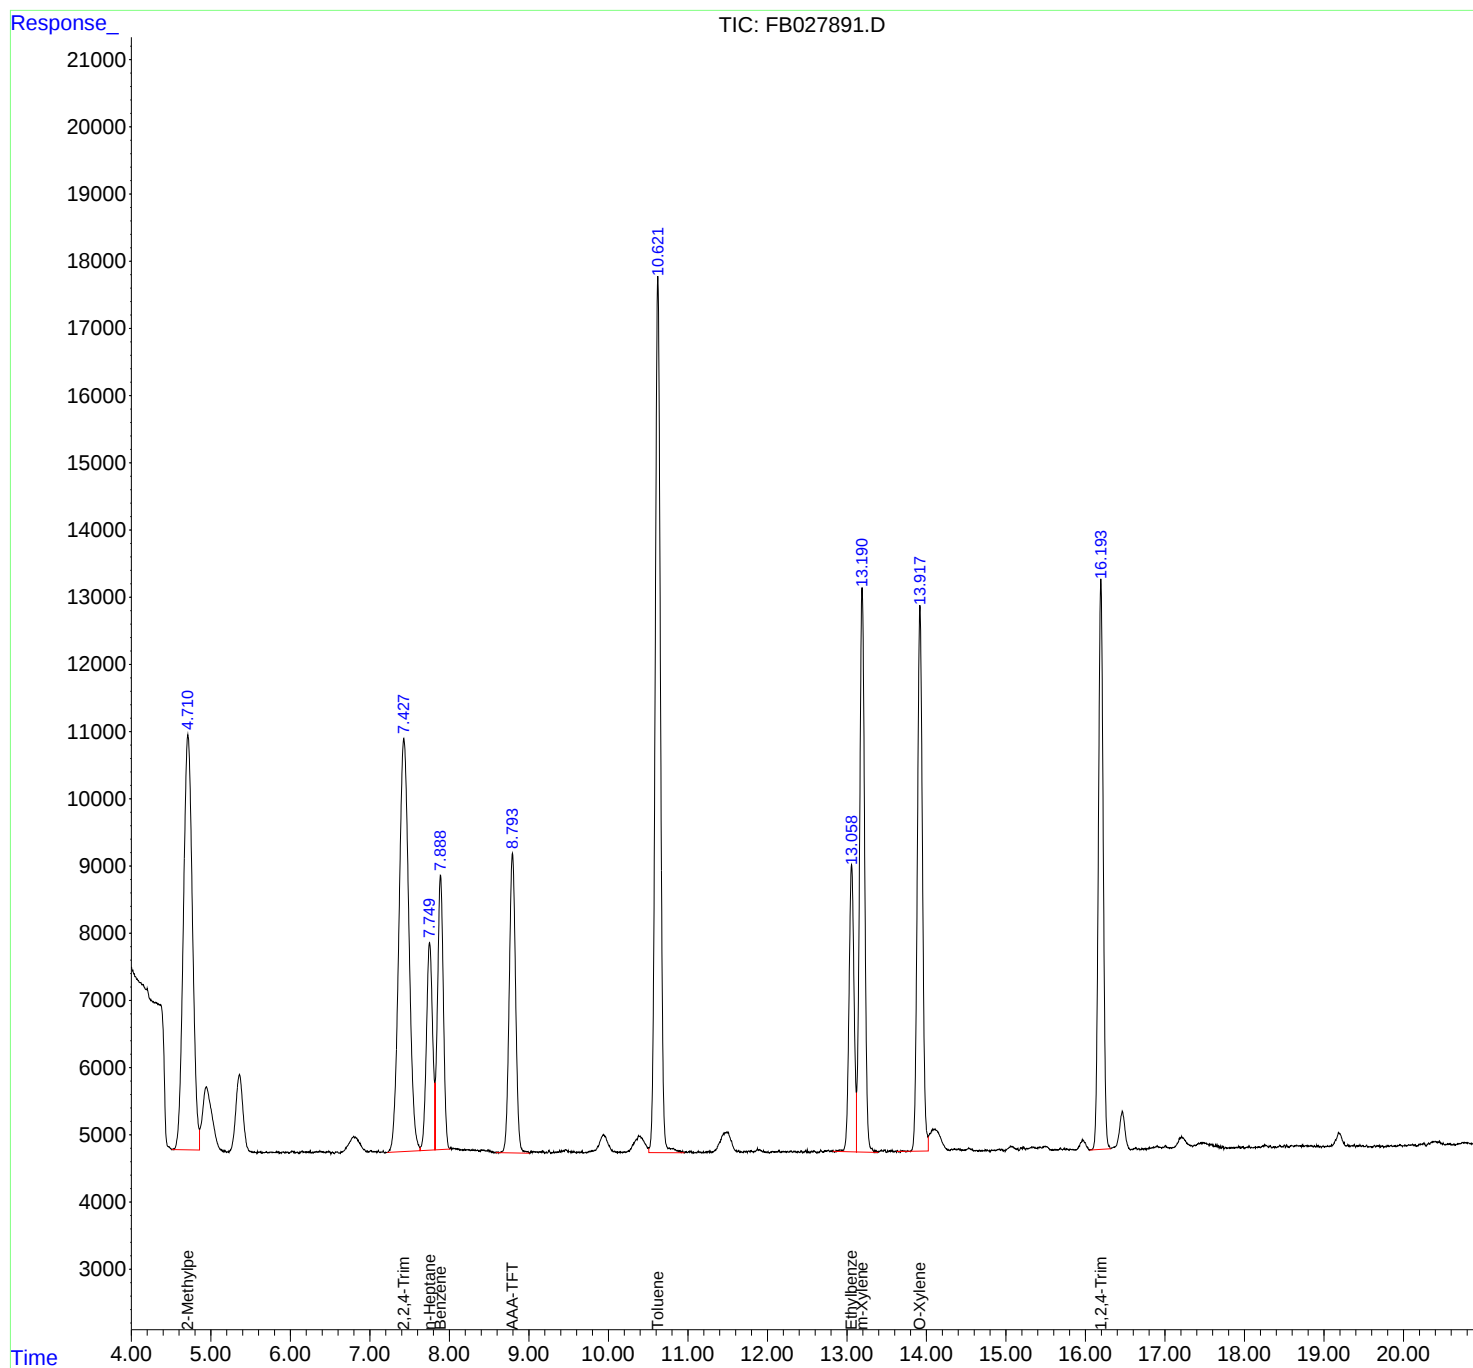


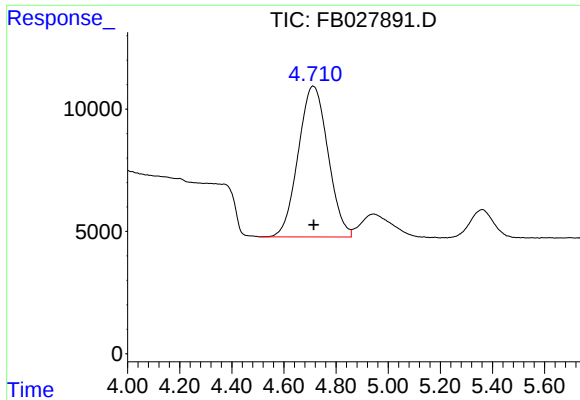

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: -0.003 min
Response: 488837
Conc: 27.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0811S1

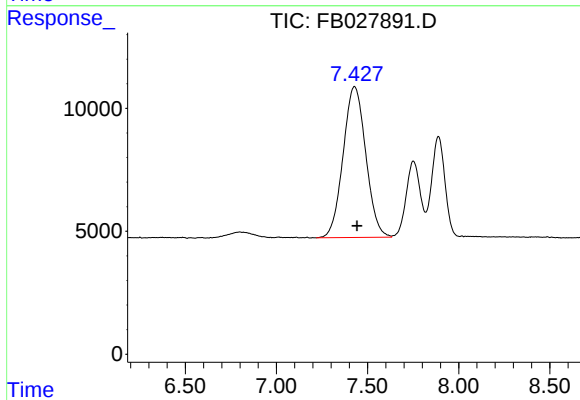


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.015 min
Response: 530375
Conc: 27.05 ng/ml

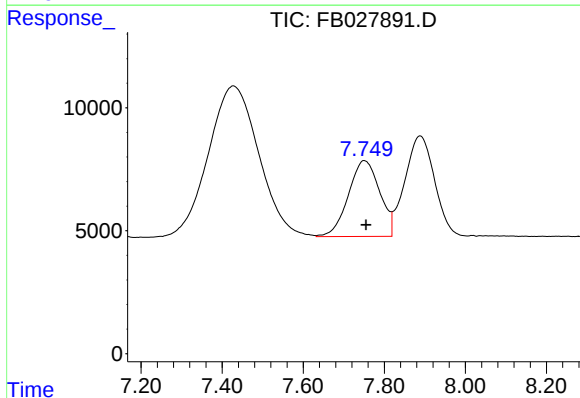


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.004 min
Response: 165570
Conc: 8.59 ng/ml

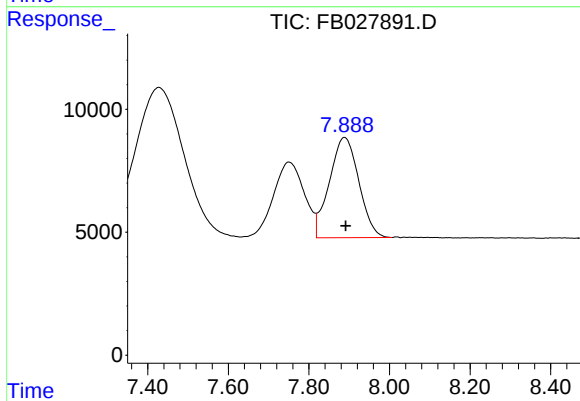

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 207157
Conc: 8.91 ng/ml

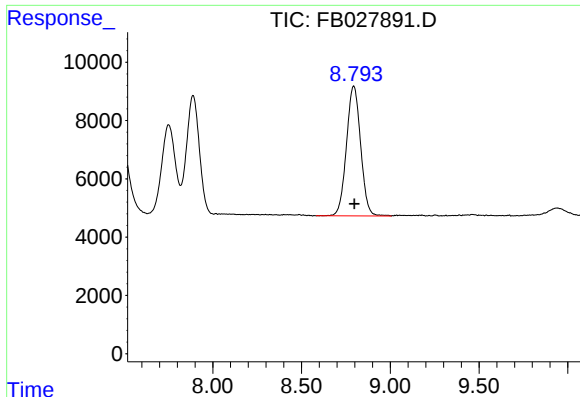

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.004 min
Response: 246908
Conc: 21.30 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0811S1

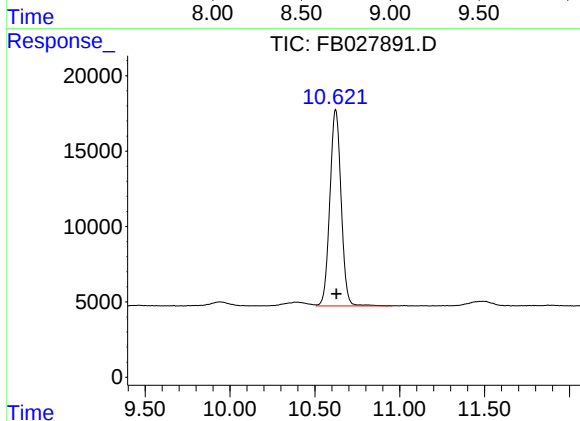


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.005 min
Response: 600224
Conc: 27.37 ng/ml

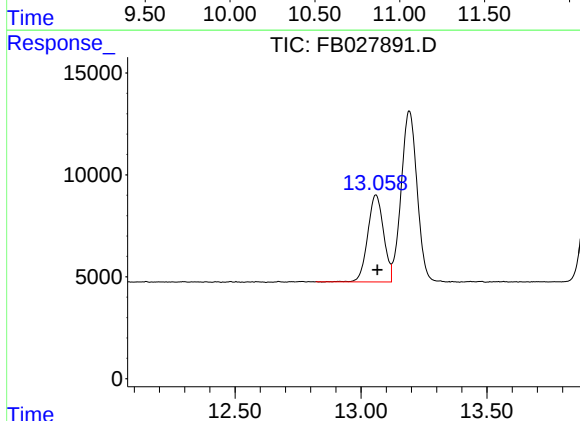


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: -0.005 min
Response: 186640
Conc: 9.06 ng/ml

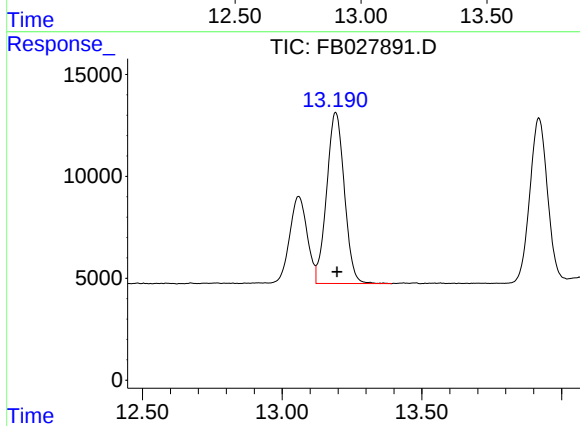

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.005 min
Response: 370095
Conc: 18.09 ng/ml

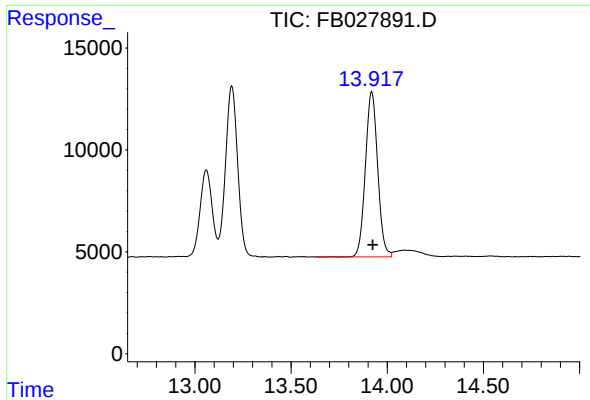

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.005 min
Response: 359610
Conc: 18.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0811S1

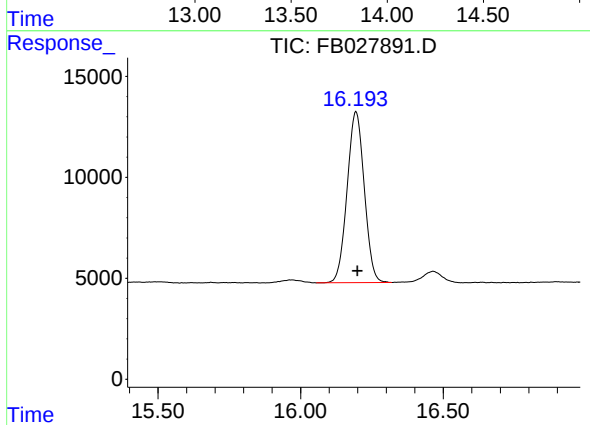

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.005 min
Response: 354303
Conc: 18.17 ng/ml