

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081122\
 Data File : FB027894.D
 Signal(s) : FID2B.CH
 Acq On : 11 Aug 2022 12:34
 Operator : AJ/MA
 Sample : N4130-01MS
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB02MS

Integration File: Calibration.e
 Quant Time: Aug 12 10:14:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	137828	11.893 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	386381	21.358 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	481635	24.561 ng/ml
3) t n-Heptane	7.751	142718	7.408 ng/ml
4) t Benzene	7.889	201238	8.655 ng/ml
6) t Toluene	10.623	558978	25.491 ng/ml
7) t Ethylbenzene	13.061	175233	8.504 ng/ml
8) t m-Xylene	13.194	348603	17.036 ng/ml
9) t O-Xylene	13.920	338854	17.106 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	339900	17.430 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081122\
Data File : FB027894.D
Signal(s) : FID2B.CH
Acq On : 11 Aug 2022 12:34
Operator : AJ/MA
Sample : N4130-01MS
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB02MS

Integration File: Calibration.e
Quant Time: Aug 12 10:14:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

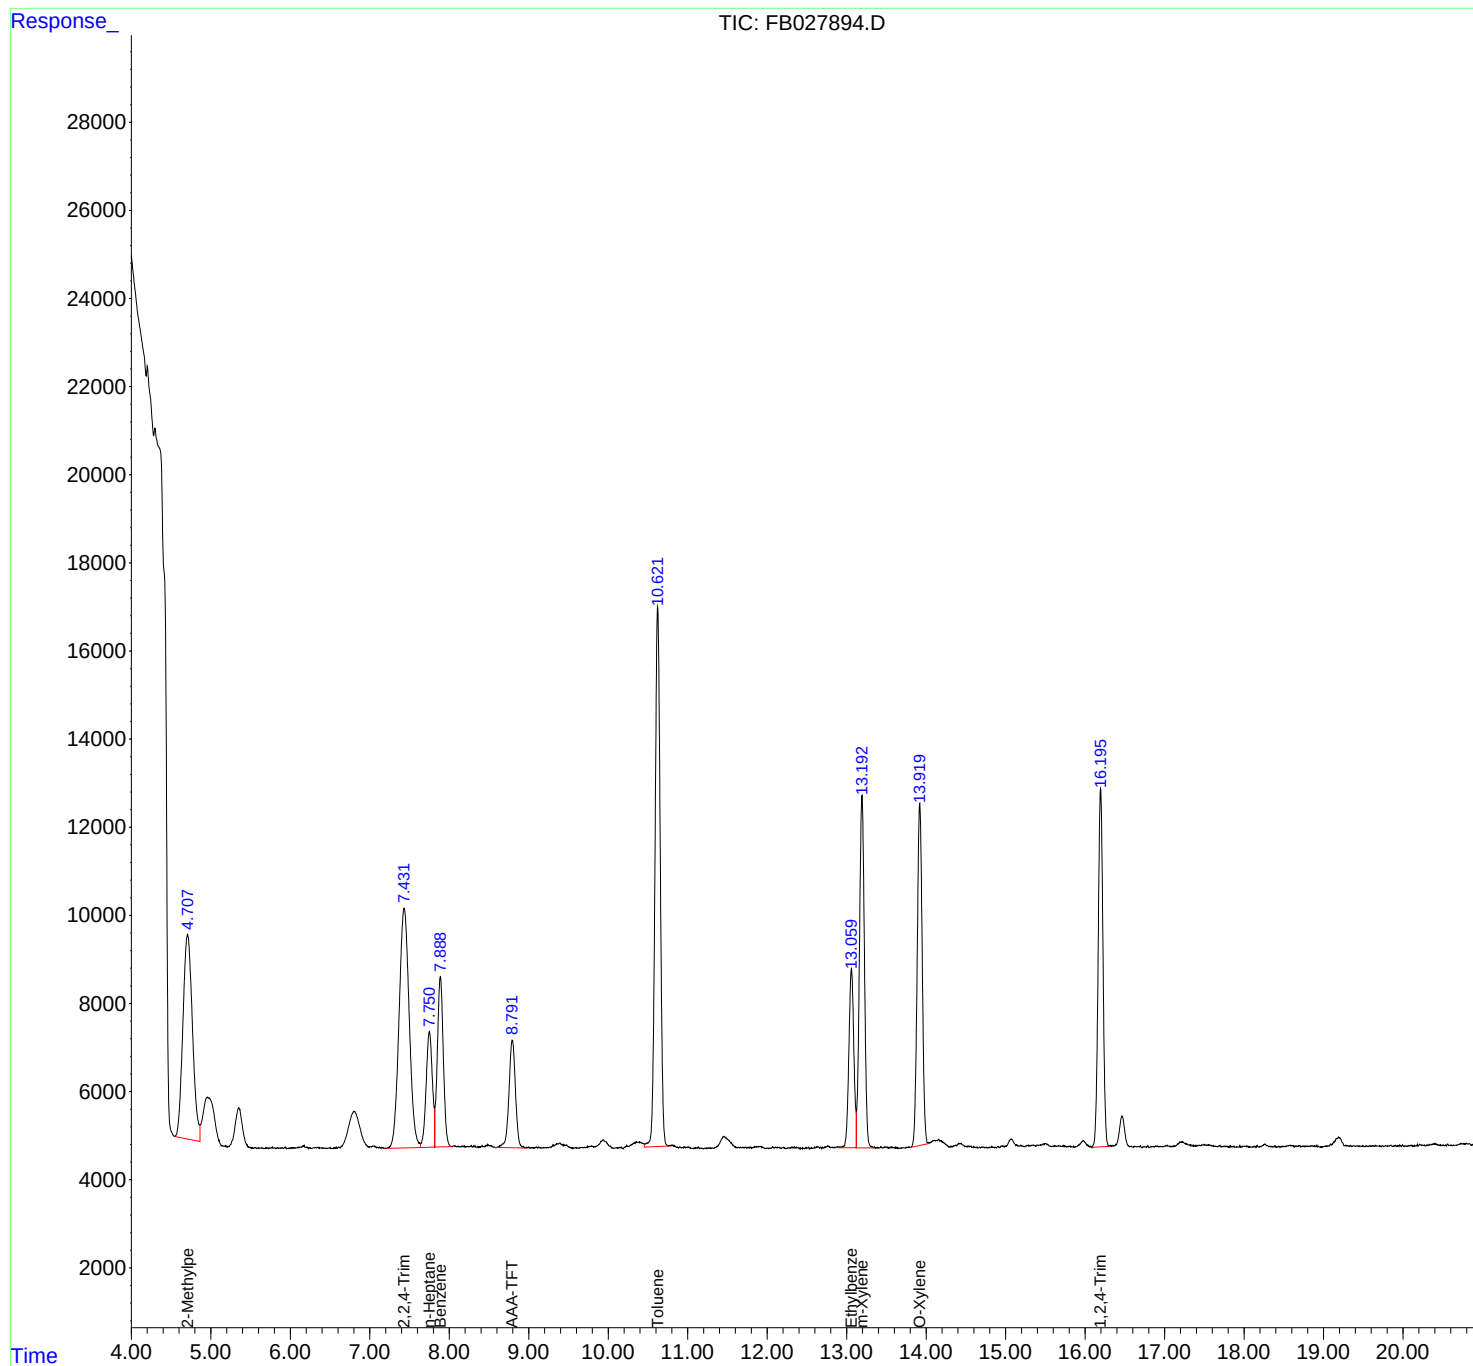


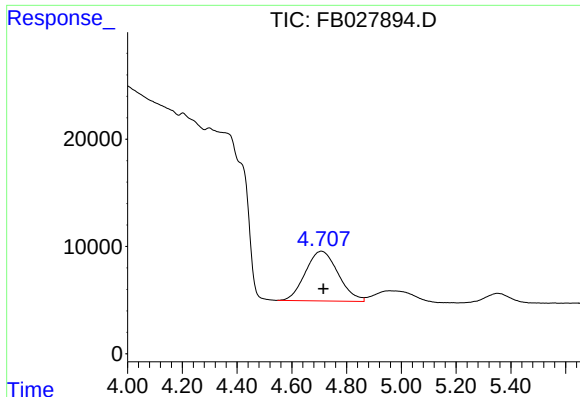

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.007 min
Response: 386381
Conc: 21.36 ng/ml

Instrument :
FID_B
ClientSampleId :
SB02MS

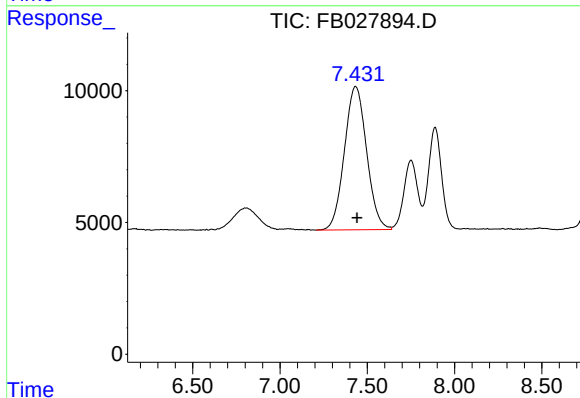


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: -0.010 min
Response: 481635
Conc: 24.56 ng/ml

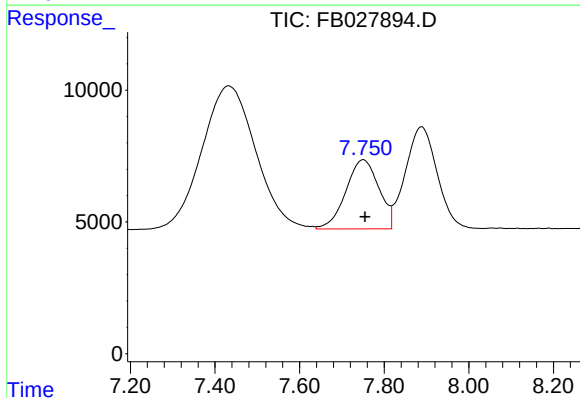


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.004 min
Response: 142718
Conc: 7.41 ng/ml

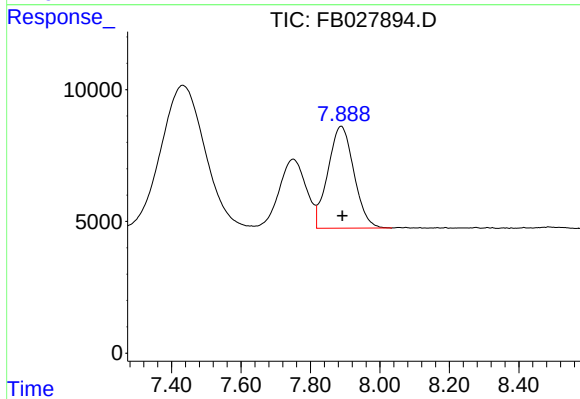

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 201238
Conc: 8.66 ng/ml

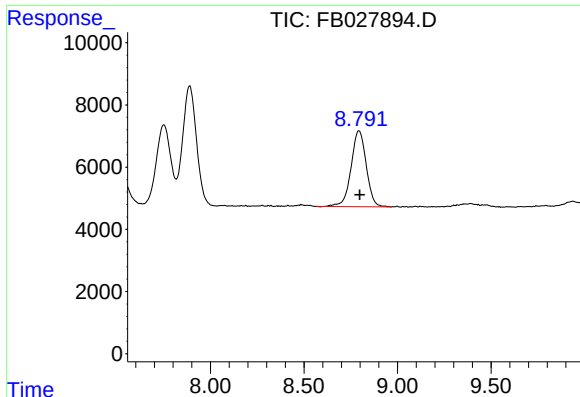

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.005 min
Response: 137828
Conc: 11.89 ng/ml

Instrument :
FID_B
ClientSampleId :
SB02MS

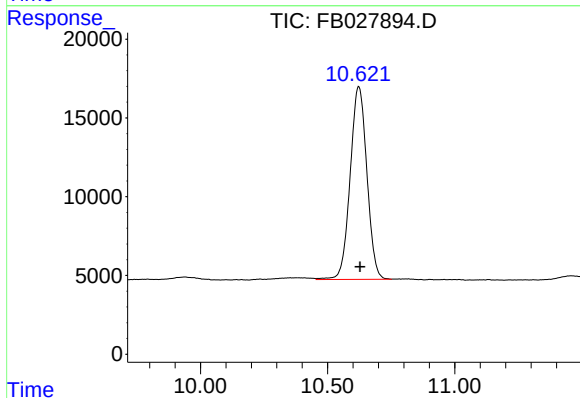


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.005 min
Response: 558978
Conc: 25.49 ng/ml

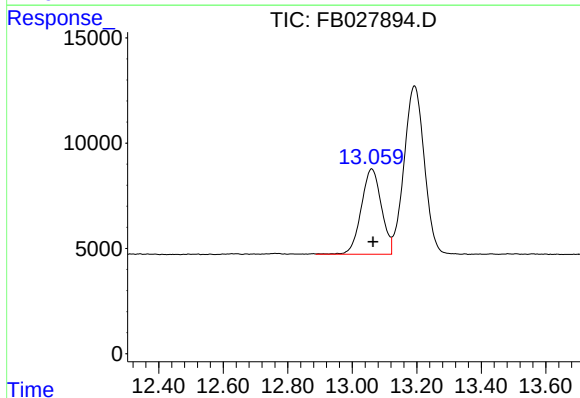


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.004 min
Response: 175233
Conc: 8.50 ng/ml

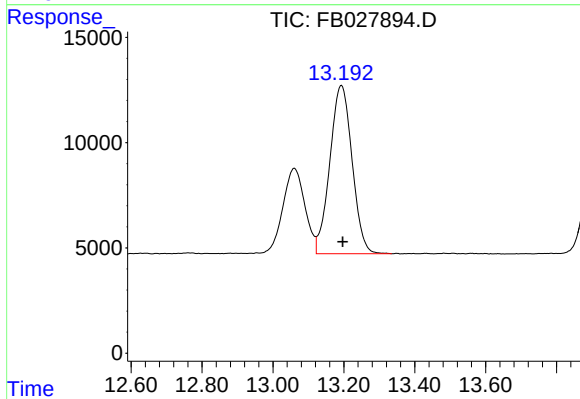

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.003 min
Response: 348603
Conc: 17.04 ng/ml

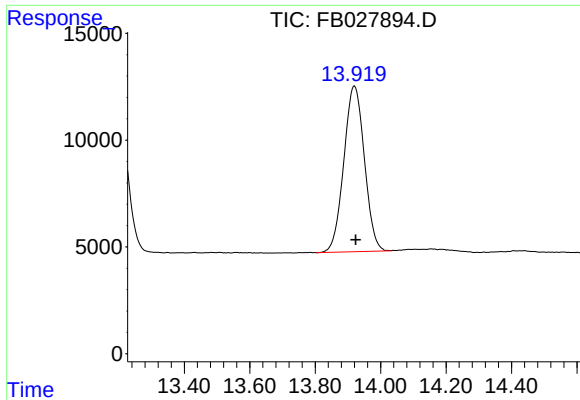

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 338854
Conc: 17.11 ng/ml

Instrument :
FID_B
ClientSampleId :
SB02MS

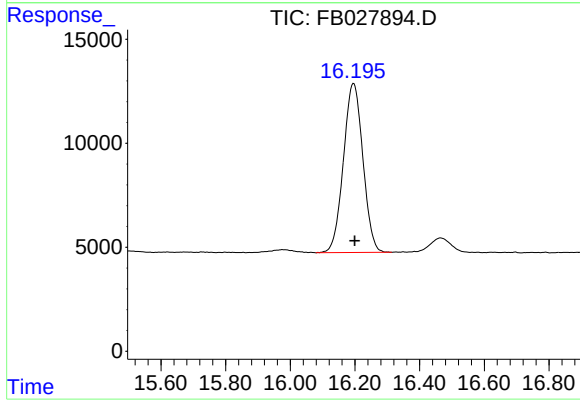

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.003 min
Response: 339900
Conc: 17.43 ng/ml