

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081123\
 Data File : FB030237.D
 Signal(s) : FID2B.CH
 Acq On : 11 Aug 2023 12:56
 Operator : YP/AJ
 Sample : 03971-03MS 50X
 Misc : 5.06G/5.00 ML MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 12 00:56:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	251402	20.454 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	373454	22.607 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	507411	27.344 ng/ml
3) t n-Heptane	7.749	169328	8.802 ng/ml
4) t Benzene	7.886	241512	10.266 ng/ml
6) t Toluene	10.620	695682	30.356 ng/ml
7) t Ethylbenzene	13.056	221862	10.337 ng/ml
8) t m-Xylene	13.189	425784	20.246 ng/ml
9) t O-Xylene	13.916	410309	19.992 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	364781	18.637 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081123\
Data File : FB030237.D
Signal(s) : FID2B.CH
Acq On : 11 Aug 2023 12:56
Operator : YP/AJ
Sample : 03971-03MS 50X
Misc : 5.06G/5.00 ML MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 12 00:56:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

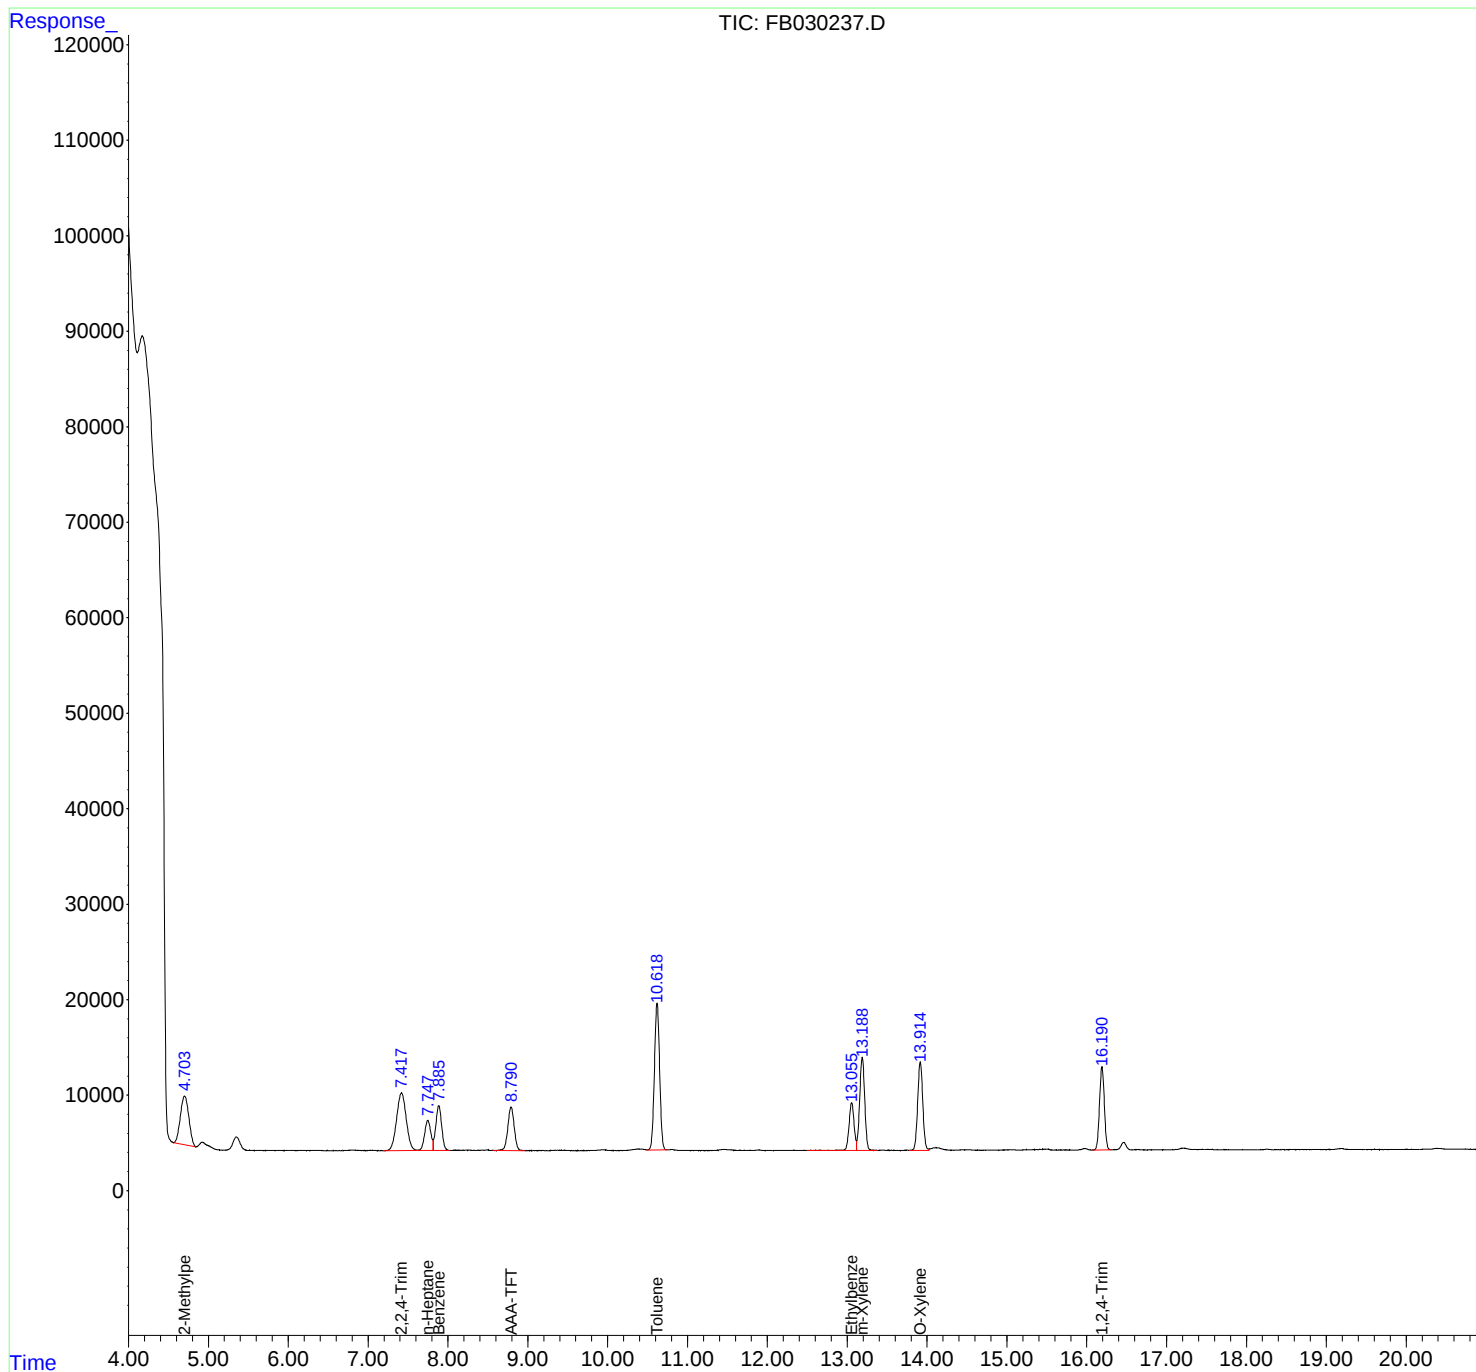

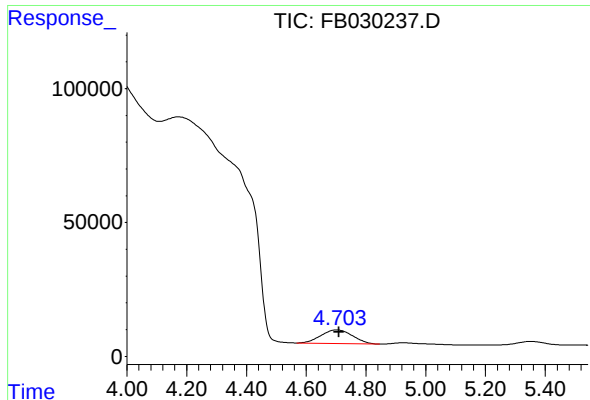


#1 2-Methylpentane

R.T.: 4.703 min
Delta R.T.: -0.007 min
Response: 373454
Conc: 22.61 ng/ml


Instrument : FID_B

ClientSampleId :

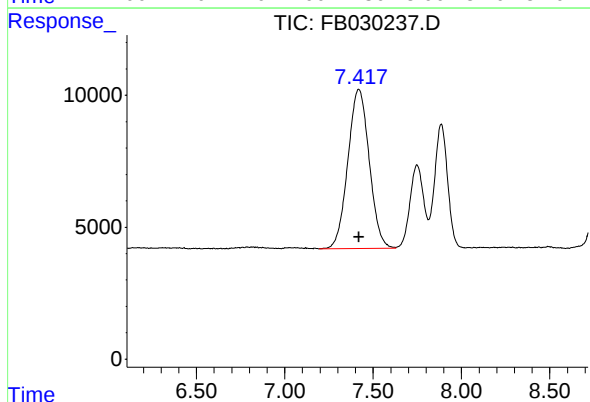


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.003 min
Response: 507411
Conc: 27.34 ng/ml

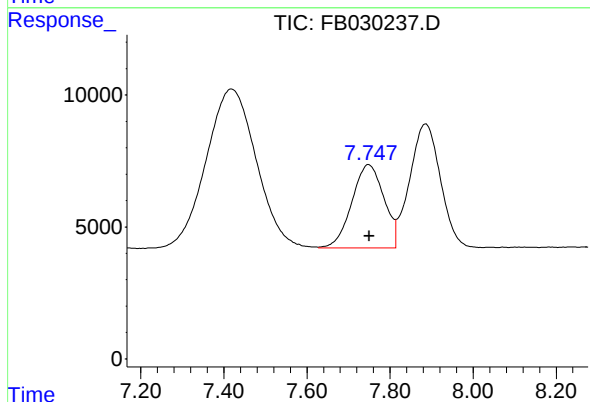


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 169328
Conc: 8.80 ng/ml

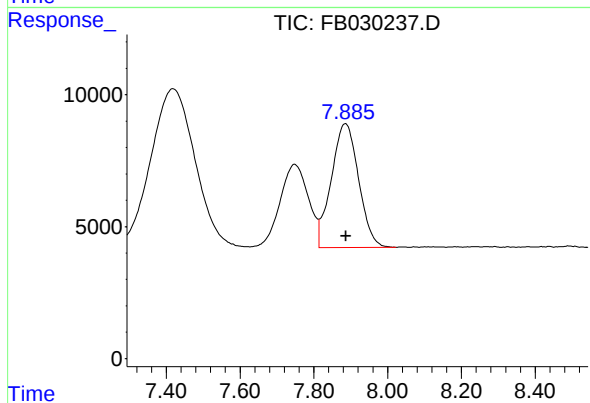

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 241512
Conc: 10.27 ng/ml

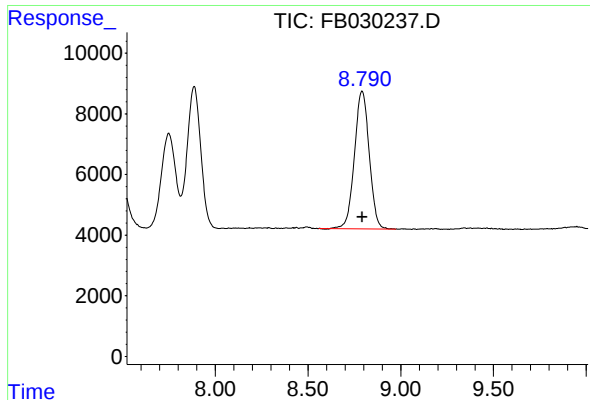

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.001 min
Response: 251402
Conc: 20.45 ng/ml

Instrument :
FID_B
ClientSampleId :

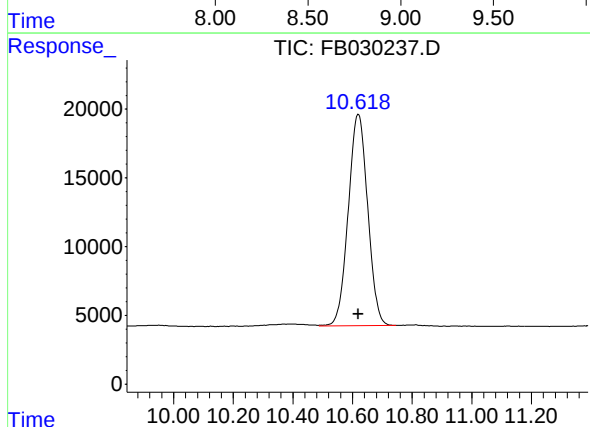


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 695682
Conc: 30.36 ng/ml

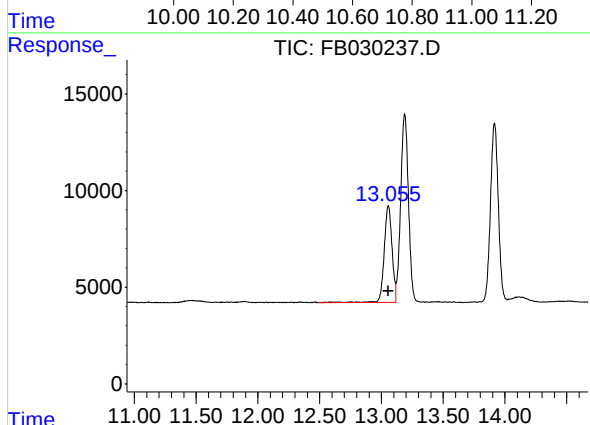


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 221862
Conc: 10.34 ng/ml

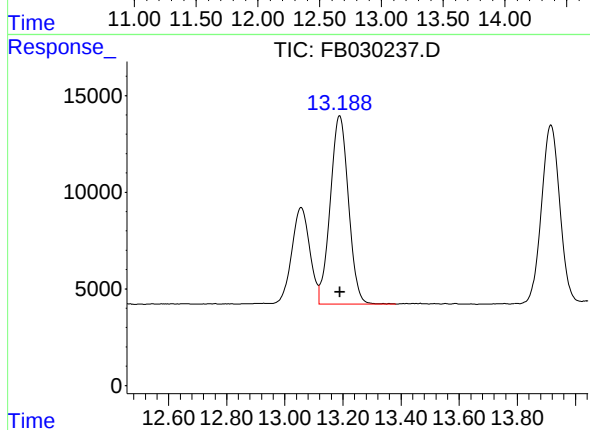

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 425784
Conc: 20.25 ng/ml

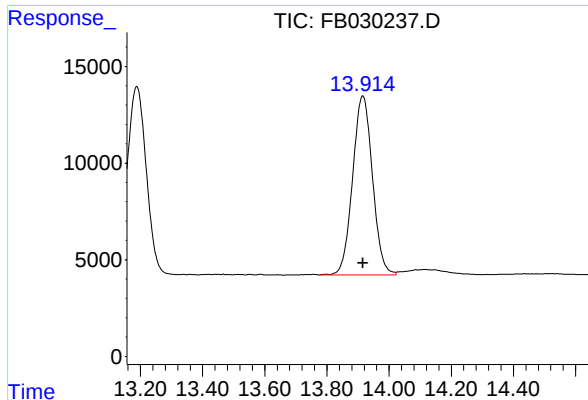

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 410309
Conc: 19.99 ng/ml

Instrument :
FID_B
ClientSampleId :

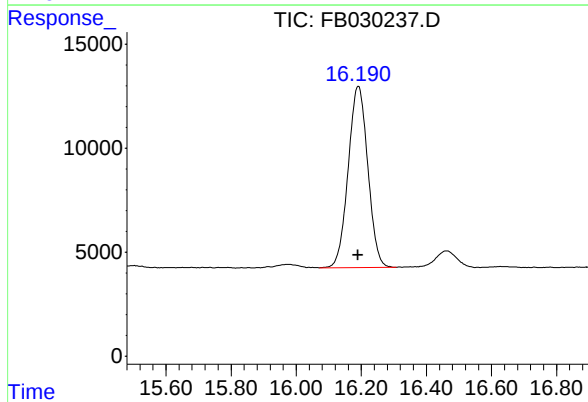

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.001 min
Response: 364781
Conc: 18.64 ng/ml