

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081123\
 Data File : FB030239.D
 Signal(s) : FID2B.CH
 Acq On : 11 Aug 2023 14:14
 Operator : YP/AJ
 Sample : BSF0811S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0811S2

Integration File: Calibration.e
 Quant Time: Aug 12 00:57:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	239923	19.520 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	396398	23.996 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	477660	25.741 ng/ml
3) t n-Heptane	7.752	151614	7.881 ng/ml
4) t Benzene	7.889	203590	8.654 ng/ml
6) t Toluene	10.621	599141	26.144 ng/ml
7) t Ethylbenzene	13.058	187702	8.746 ng/ml
8) t m-Xylene	13.190	373650	17.767 ng/ml
9) t O-Xylene	13.917	364702	17.770 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	347764	17.767 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081123\
Data File : FB030239.D
Signal(s) : FID2B.CH
Acq On : 11 Aug 2023 14:14
Operator : YP/AJ
Sample : BSF0811S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0811S2

Integration File: Calibration.e
Quant Time: Aug 12 00:57:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

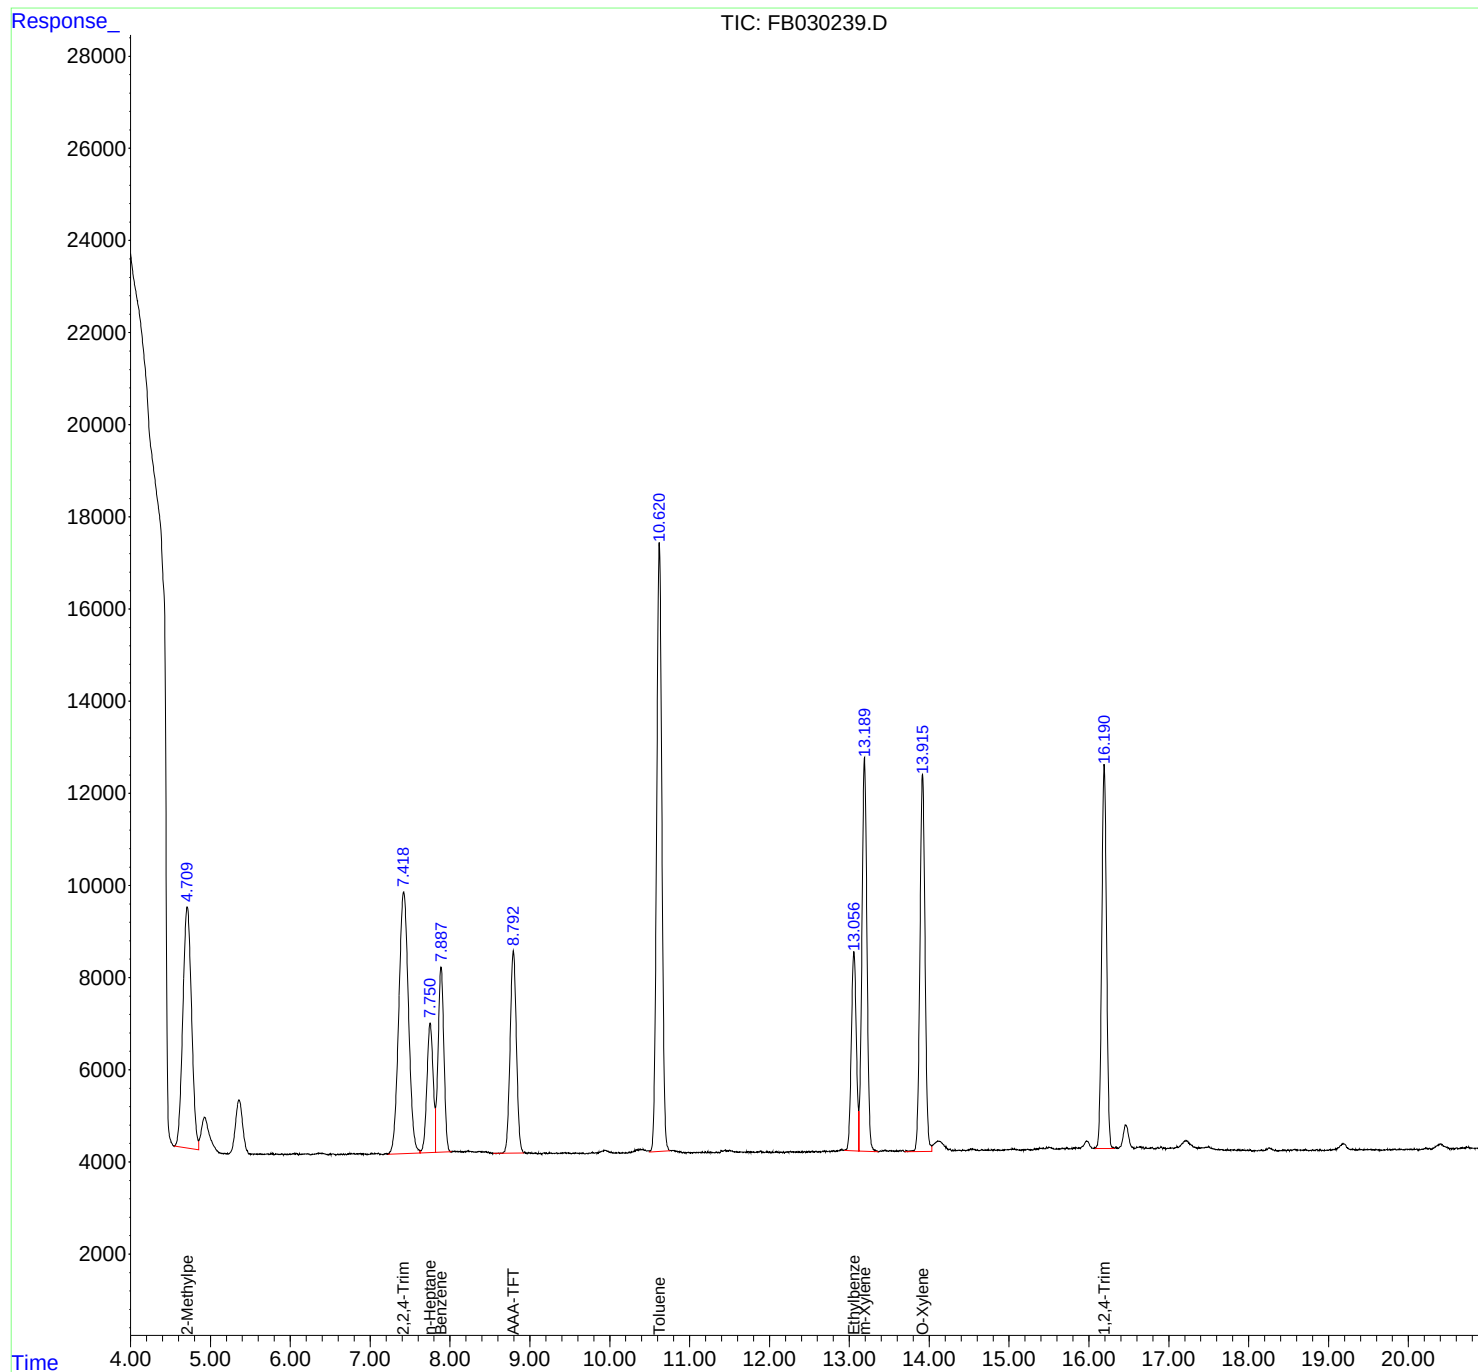


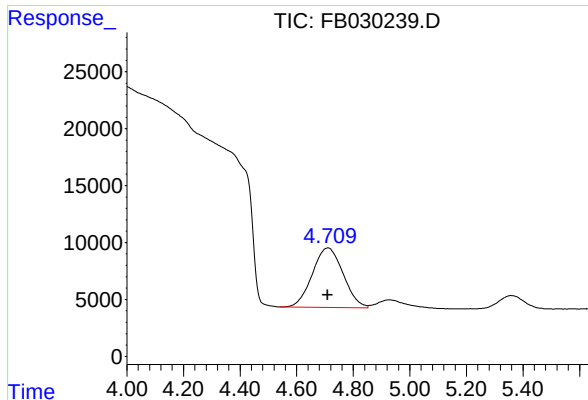

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 396398
Conc: 24.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0811S2

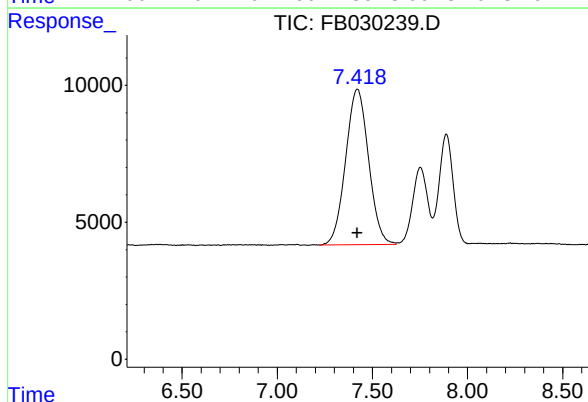


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.002 min
Response: 477660
Conc: 25.74 ng/ml

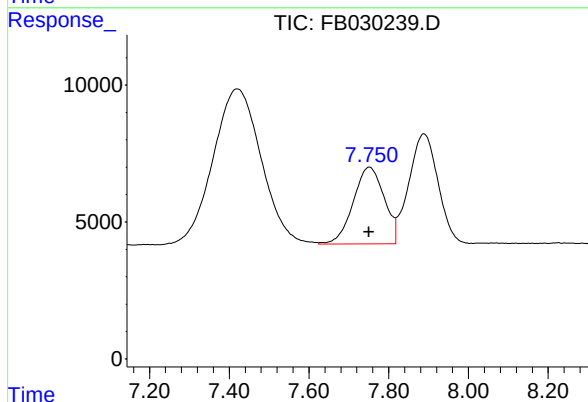


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.001 min
Response: 151614
Conc: 7.88 ng/ml

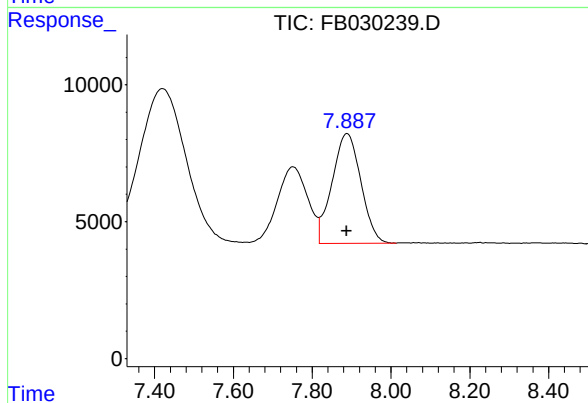

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 203590
Conc: 8.65 ng/ml

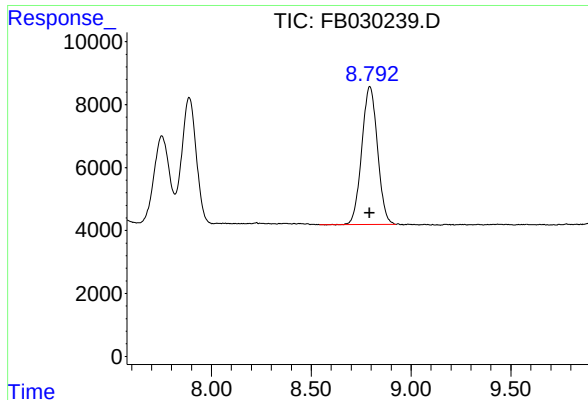

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 239923
Conc: 19.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0811S2

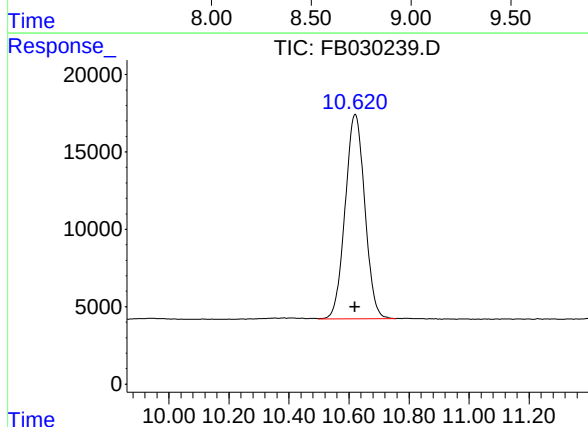


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 599141
Conc: 26.14 ng/ml

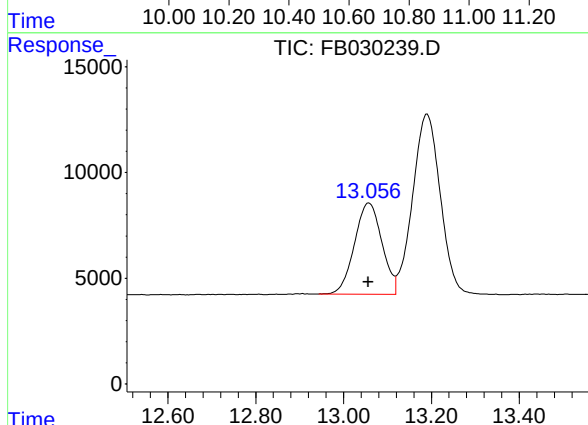


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.001 min
Response: 187702
Conc: 8.75 ng/ml

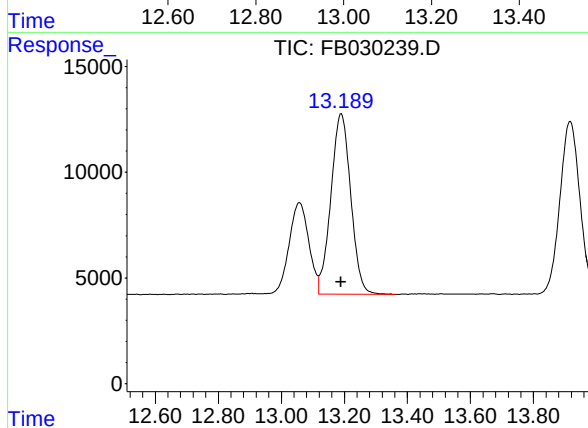

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.001 min
Response: 373650
Conc: 17.77 ng/ml

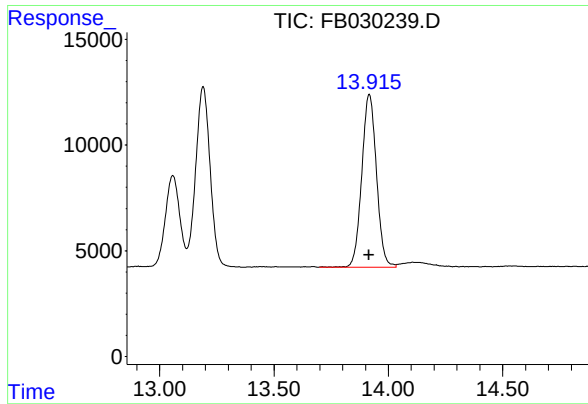

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.001 min
Response: 364702
Conc: 17.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0811S2

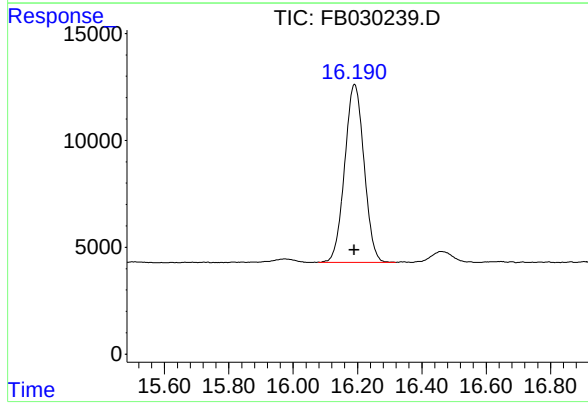

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.001 min
Response: 347764
Conc: 17.77 ng/ml