

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081219\
 Data File : FB021985.D
 Signal(s) : FID2B.CH
 Acq On : 12 Aug 2019 13:10
 Operator : DD/AJ
 Sample : K4090-05MSD
 Misc : 5.06/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 13 01:15:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	285559	20.925 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	817058	29.629 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	790929	29.921 ng/ml
3) t n-Heptane	7.948	231337	9.330 ng/ml
4) t Benzene	8.085	305381	10.453 ng/ml
6) t Toluene	10.831	610689	29.679 ng/ml
7) t Ethylbenzene	13.276	195685	9.406 ng/ml
8) t m-Xylene	13.409	416104	18.731 ng/ml
9) t O-Xylene	14.138	428206	18.615 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	445895	18.912 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081219\
Data File : FB021985.D
Signal(s) : FID2B.CH
Acq On : 12 Aug 2019 13:10
Operator : DD/AJ
Sample : K4090-05MSD
Misc : 5.06/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 13 01:15:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

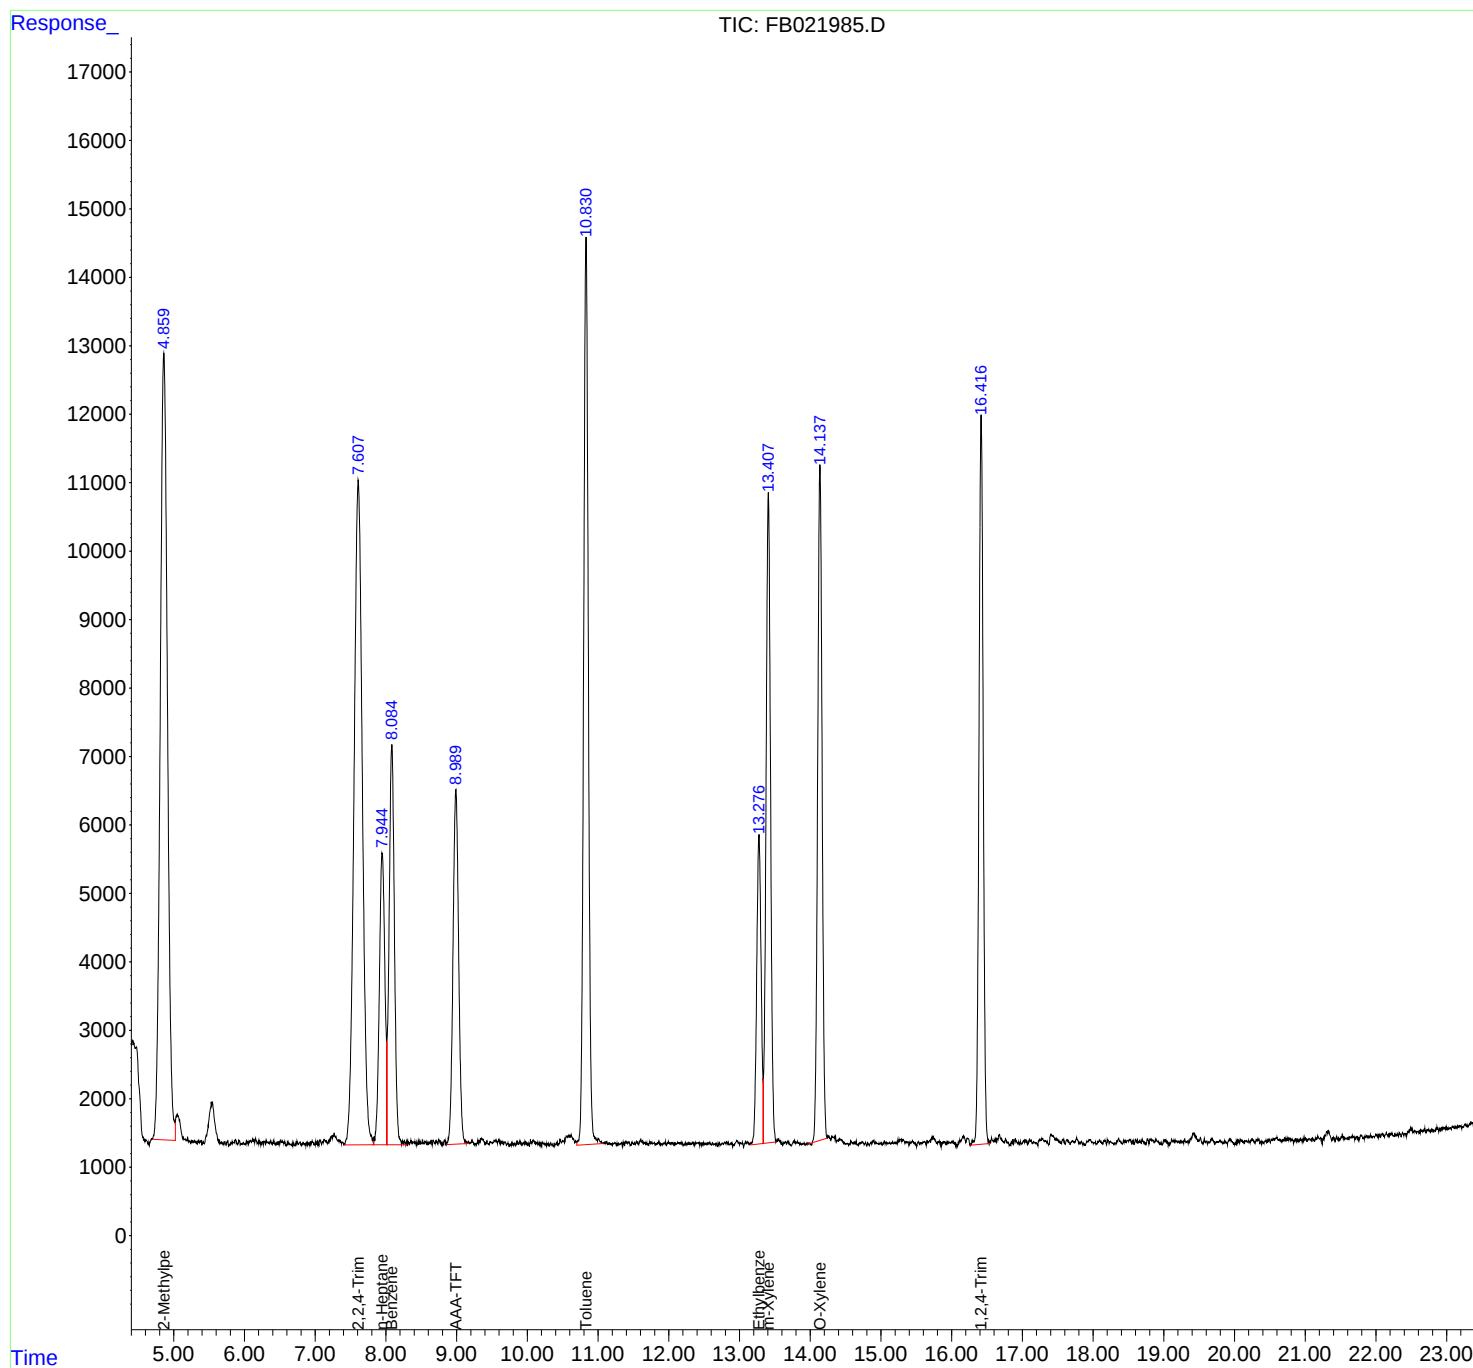

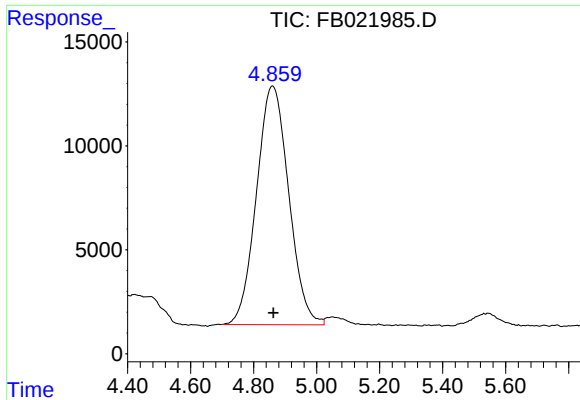


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: -0.002 min
Response: 817058
Conc: 29.63 ng/ml

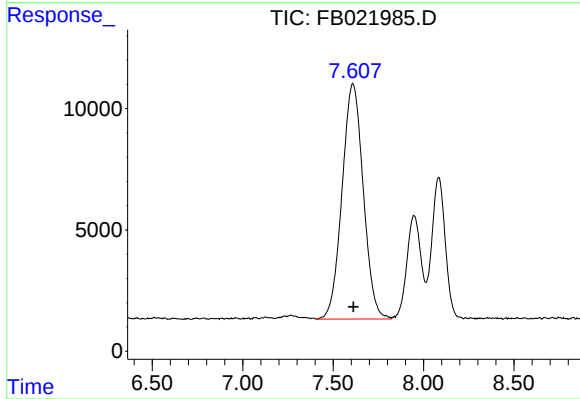


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 790929
Conc: 29.92 ng/ml

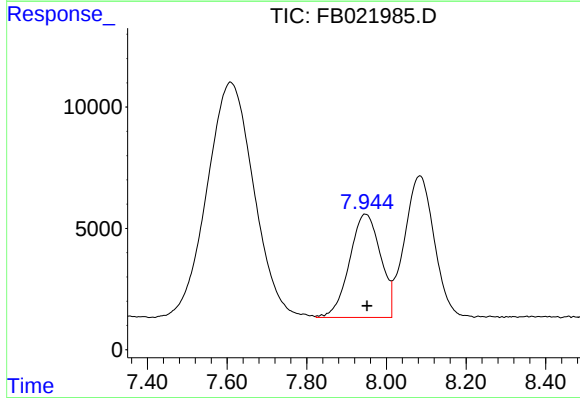


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 231337
Conc: 9.33 ng/ml

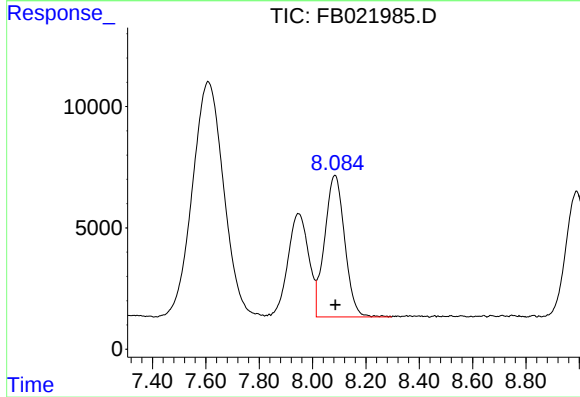


#4 Benzene

R.T.: 8.085 min
Delta R.T.: -0.001 min
Response: 305381
Conc: 10.45 ng/ml

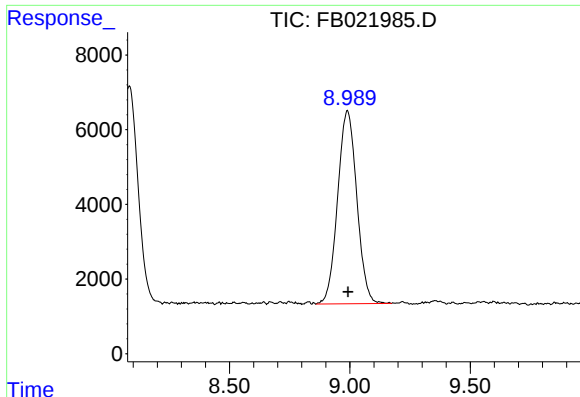


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.002 min
Response: 285559
Conc: 20.93 ng/ml

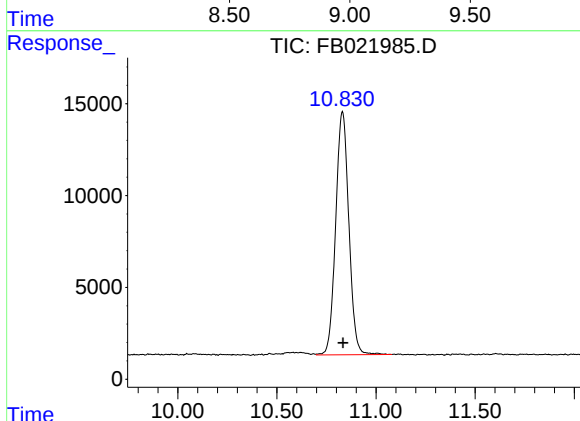


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.002 min
Response: 610689
Conc: 29.68 ng/ml

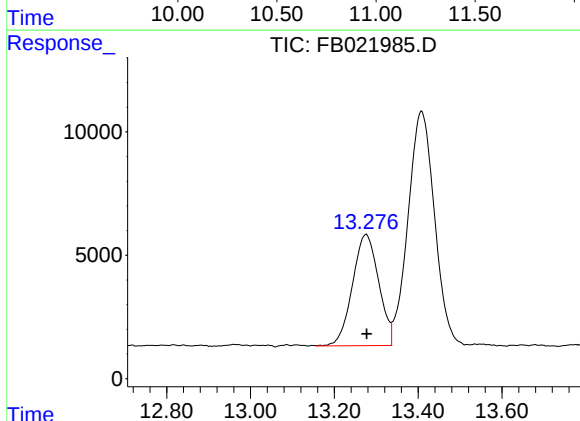


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.002 min
Response: 195685
Conc: 9.41 ng/ml

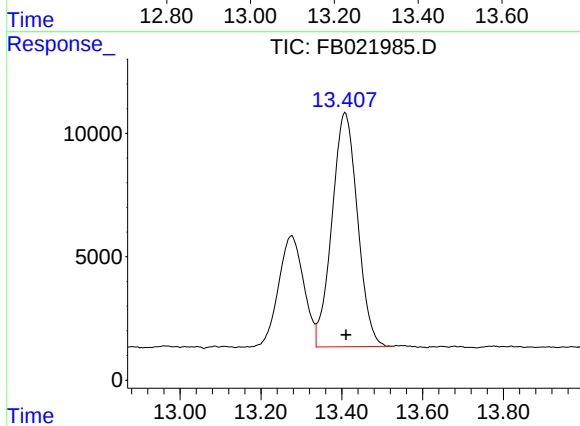


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.002 min
Response: 416104
Conc: 18.73 ng/ml

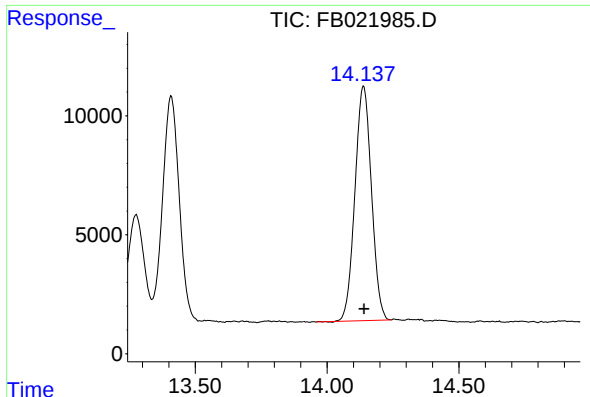

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.002 min
Response: 428206
Conc: 18.62 ng/ml

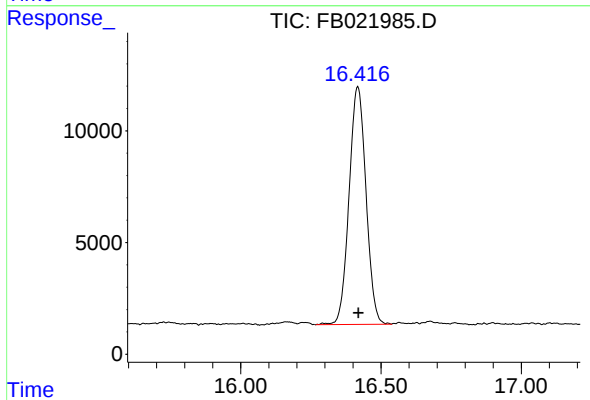

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: -0.002 min
Response: 445895
Conc: 18.91 ng/ml