

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081222\
 Data File : FB027946.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2022 8:14
 Operator : AJ/MA
 Sample : N4189-11MS 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 14 21:36:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	239500	20.665 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	399098	22.061 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	472250	24.082 ng/ml
3) t n-Heptane	7.743	128986	6.695 ng/ml
4) t Benzene	7.881	209317	9.002 ng/ml
6) t Toluene	10.615	569414	25.967 ng/ml
7) t Ethylbenzene	13.053	179876	8.729 ng/ml
8) t m-Xylene	13.186	351406	17.173 ng/ml
9) t O-Xylene	13.912	345817	17.457 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	332213	17.036 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081222\
Data File : FB027946.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2022 8:14
Operator : AJ/MA
Sample : N4189-11MS 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 14 21:36:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

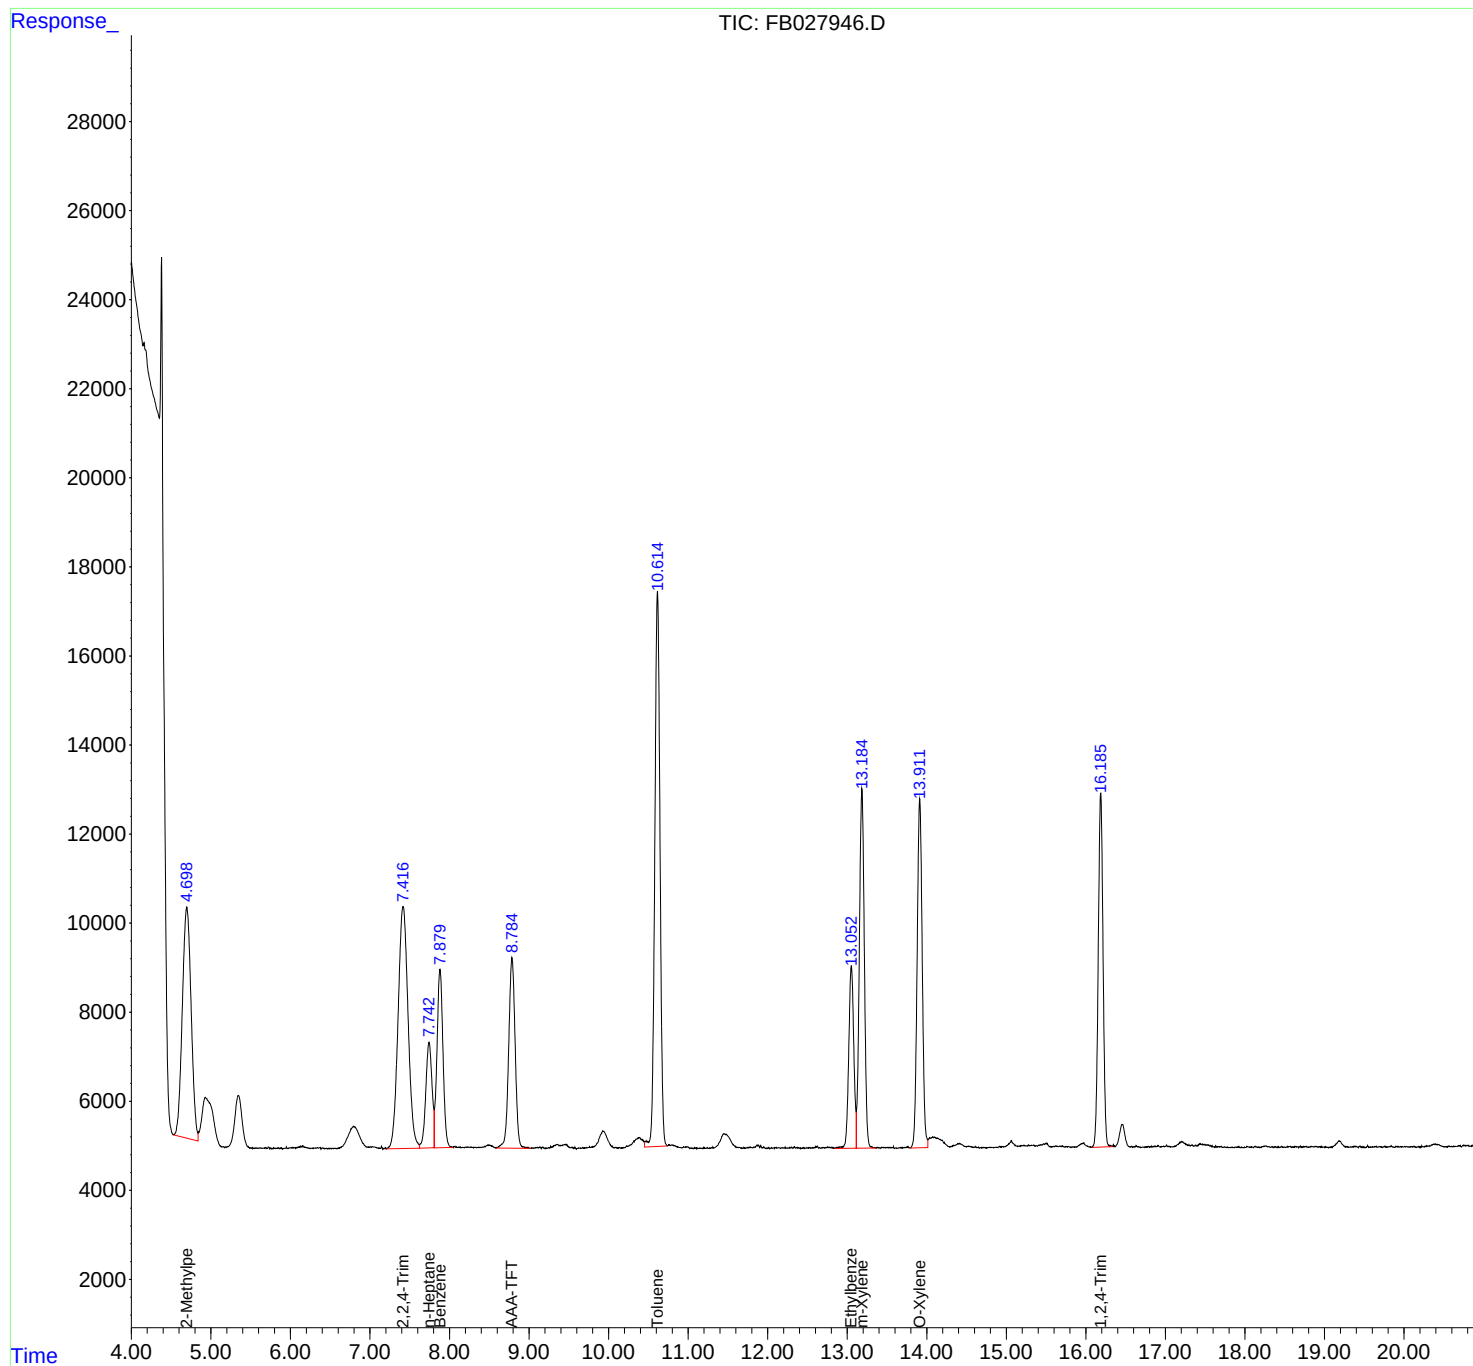


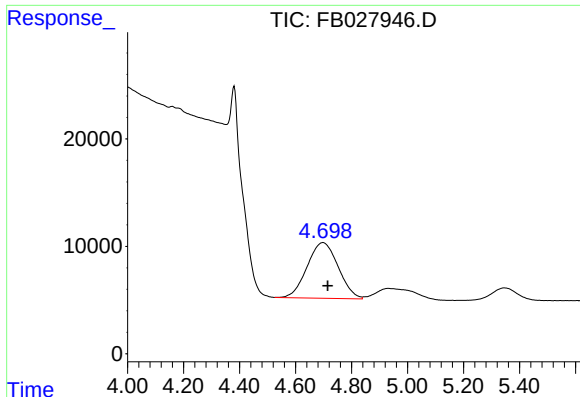

#1 2-Methylpentane


R.T.: 4.699 min
Delta R.T.: -0.016 min
Response: 399098
Conc: 22.06 ng/ml

Instrument :
FID_B
ClientSampleId :

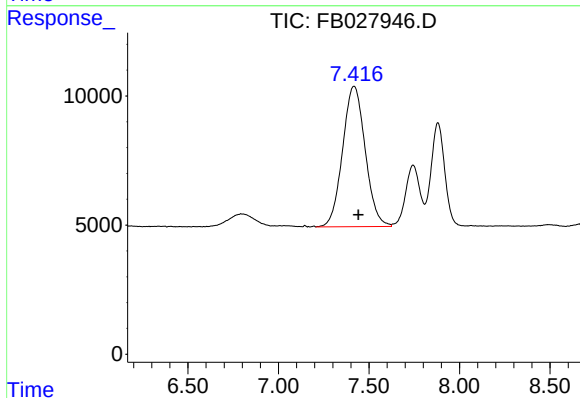


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.025 min
Response: 472250
Conc: 24.08 ng/ml

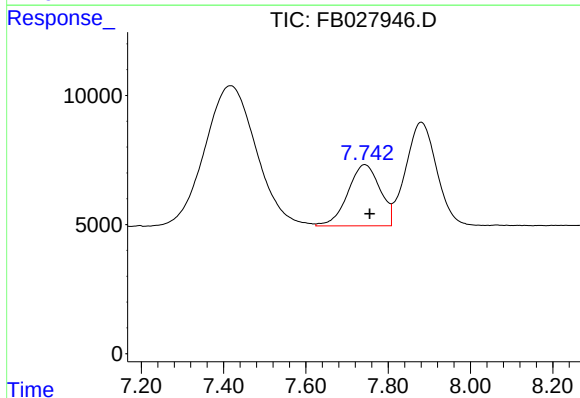


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.012 min
Response: 128986
Conc: 6.70 ng/ml

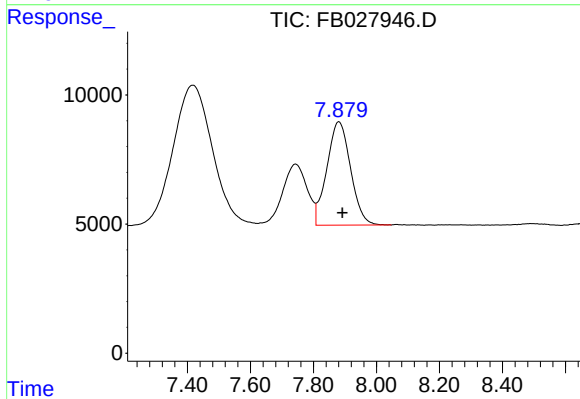

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.011 min
Response: 209317
Conc: 9.00 ng/ml

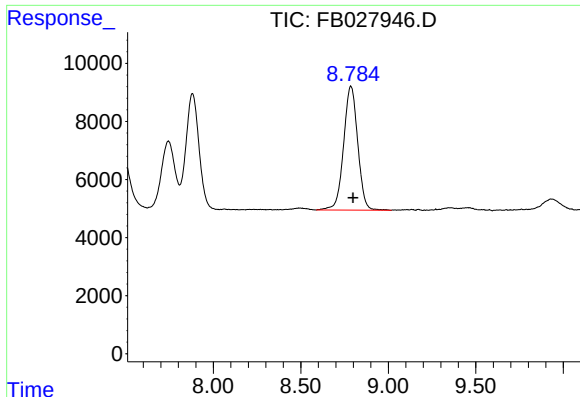

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.012 min
Response: 239500
Conc: 20.67 ng/ml

Instrument :
FID_B
ClientSampleId :

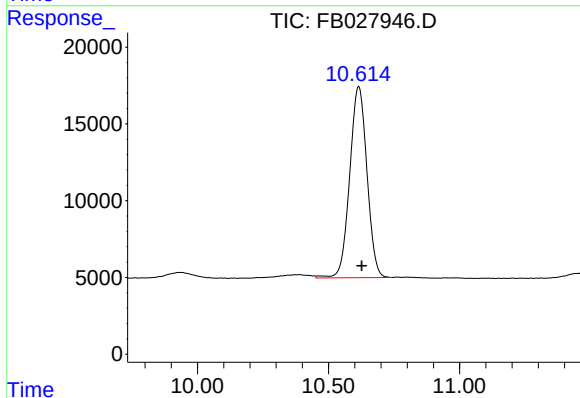


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.012 min
Response: 569414
Conc: 25.97 ng/ml

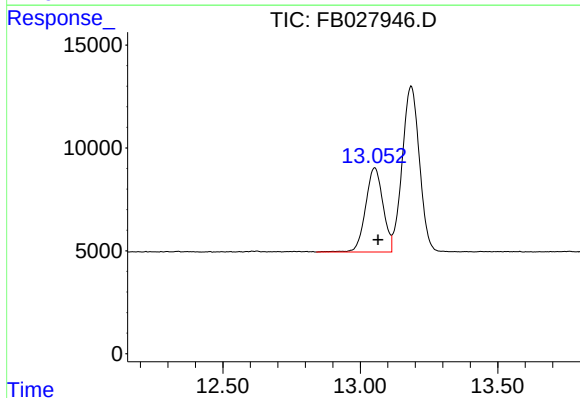


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.012 min
Response: 179876
Conc: 8.73 ng/ml

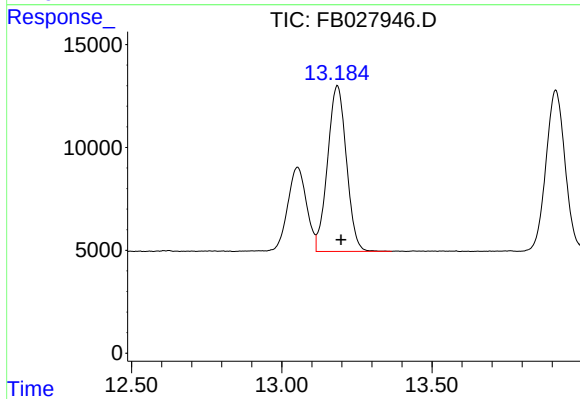

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.012 min
Response: 351406
Conc: 17.17 ng/ml

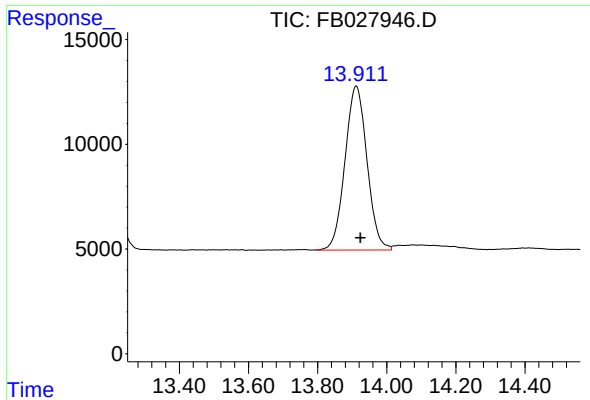

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.012 min
Response: 345817
Conc: 17.46 ng/ml

Instrument :
FID_B
ClientSampleId :

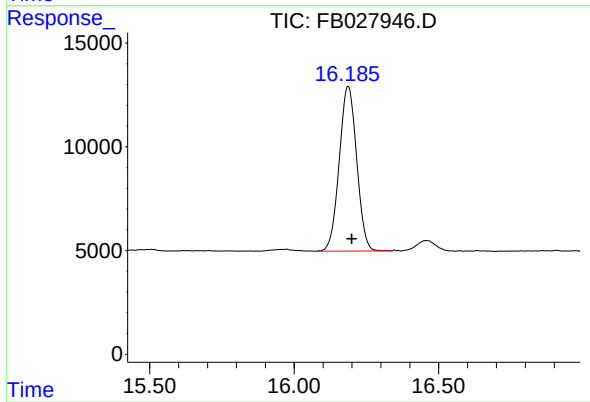

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.012 min
Response: 332213
Conc: 17.04 ng/ml