

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081319\
 Data File : FB022002.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2019 12:43
 Operator : DD/AJ
 Sample : K4089-01MS
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 13 13:05:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.991	267984	19.637 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.862	659716	23.923 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	615846	23.297 ng/ml
3) t	n-Heptane	7.949	185887	7.497 ng/ml
4) t	Benzene	8.085	293875	10.059 ng/ml
6) t	Toluene	10.832	623170	30.286 ng/ml
7) t	Ethylbenzene	13.278	205159	9.861 ng/ml
8) t	m-Xylene	13.410	428648	19.295 ng/ml
9) t	O-Xylene	14.139	436945	18.995 ng/ml
10) t	1,2,4-Trimethylbenzene	16.419	415708	17.632 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081319\
Data File : FB022002.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2019 12:43
Operator : DD/AJ
Sample : K4089-01MS
Misc : 5.05/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 13 13:05:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

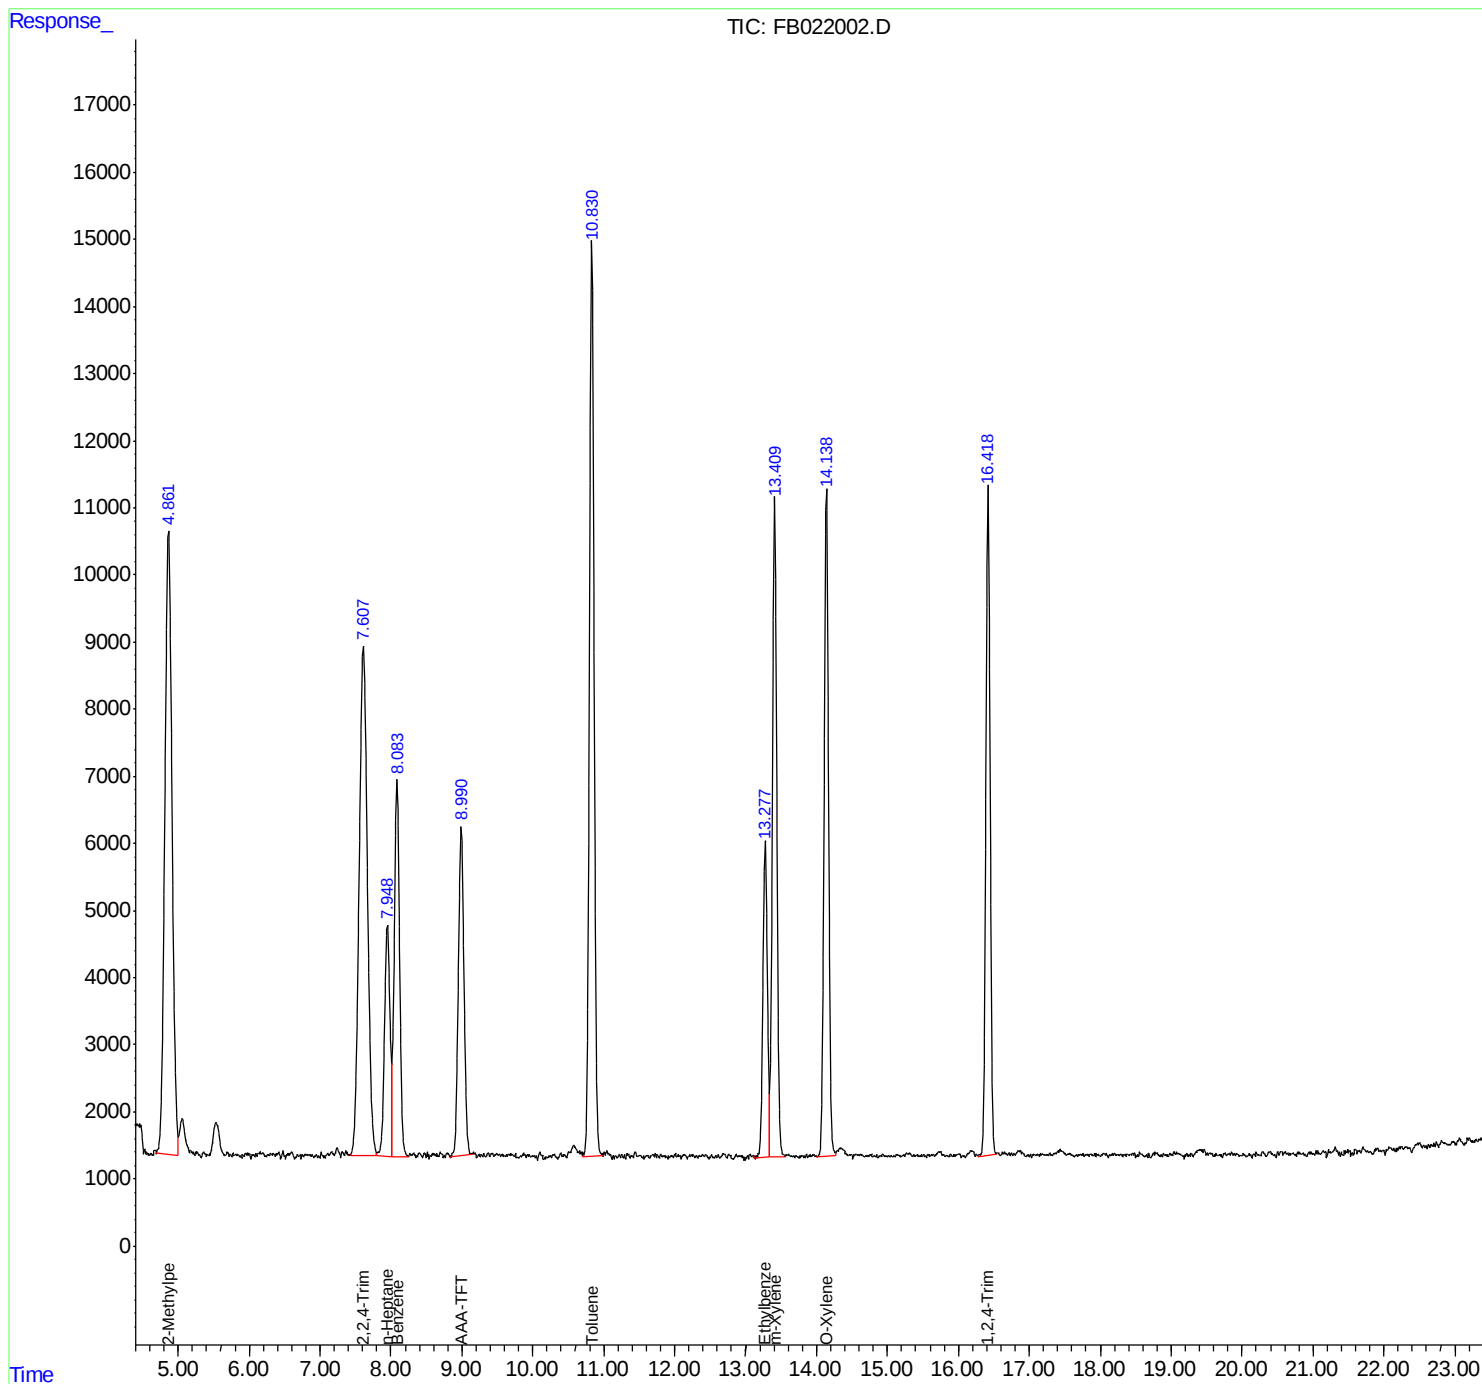

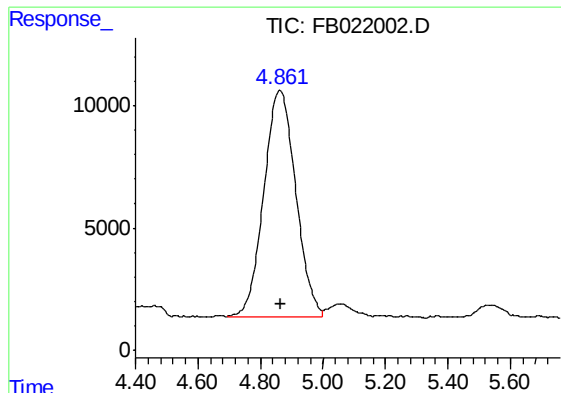


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 659716
Conc: 23.92 ng/ml

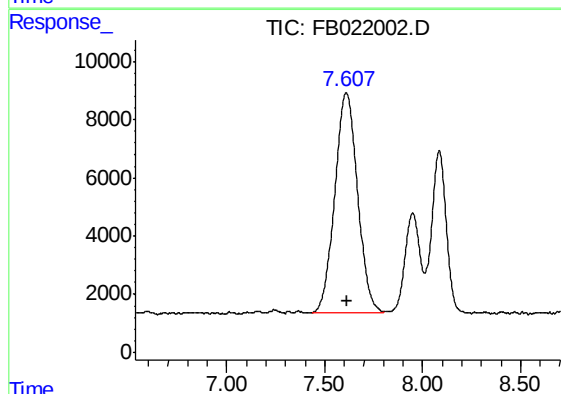


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 615846
Conc: 23.30 ng/ml

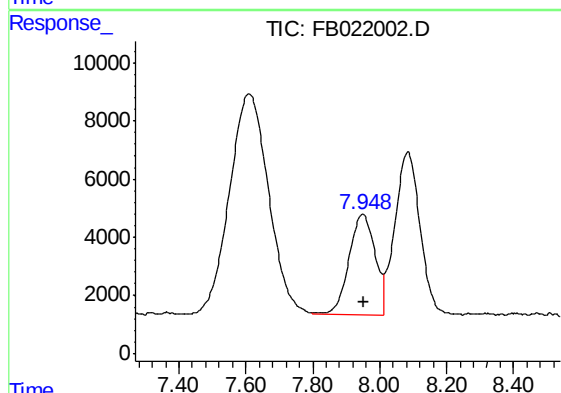


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 185887
Conc: 7.50 ng/ml

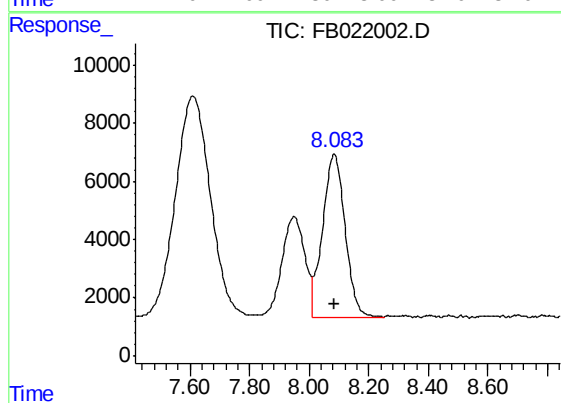


#4 Benzene

R.T.: 8.085 min
Delta R.T.: -0.001 min
Response: 293875
Conc: 10.06 ng/ml

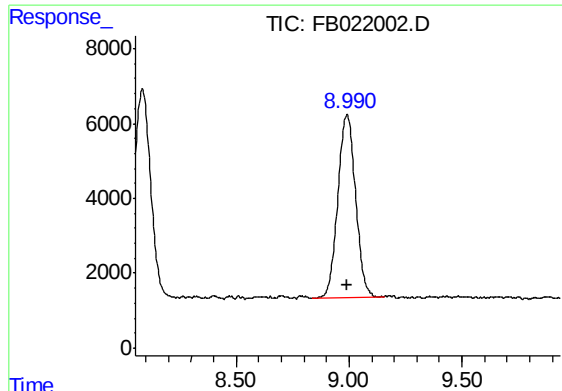


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 267984
Conc: 19.64 ng/ml

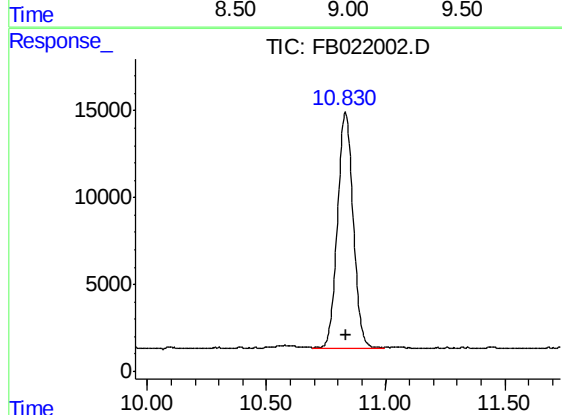


#6 Toluene

R.T.: 10.832 min
Delta R.T.: -0.002 min
Response: 623170
Conc: 30.29 ng/ml

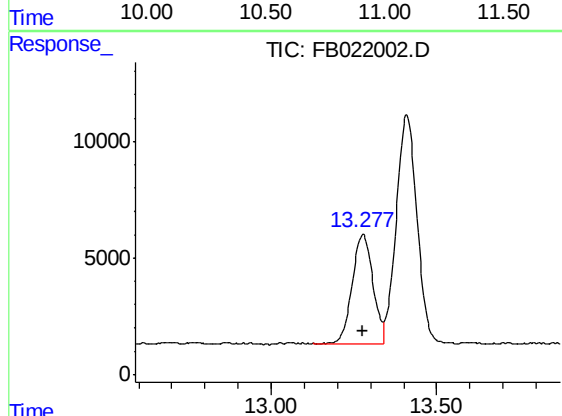


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: 0.000 min
Response: 205159
Conc: 9.86 ng/ml

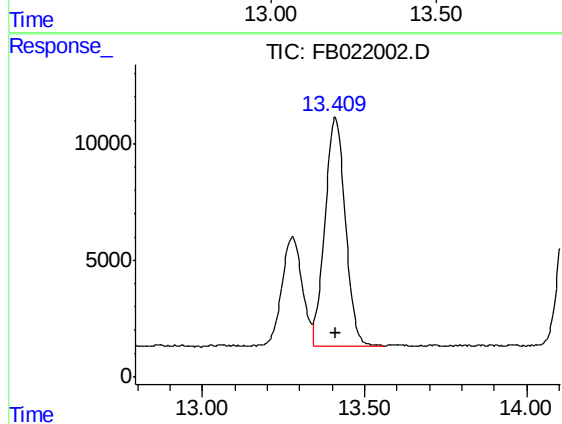


#8 m-Xylene

R.T.: 13.410 min
Delta R.T.: -0.001 min
Response: 428648
Conc: 19.30 ng/ml

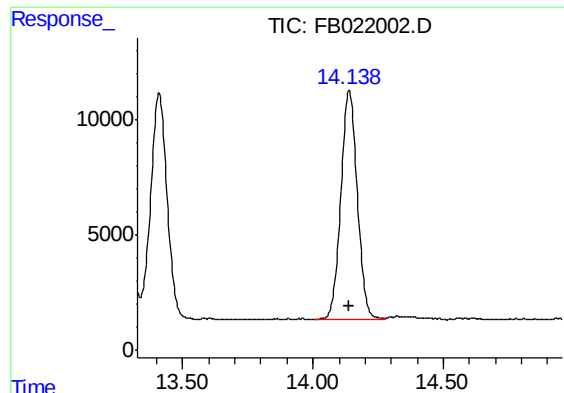

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: -0.001 min
Response: 436945
Conc: 19.00 ng/ml

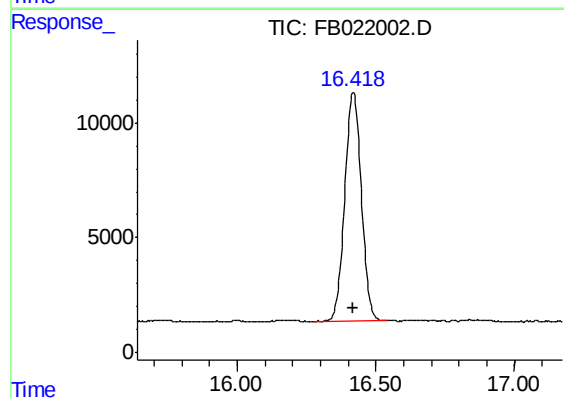

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: 0.000 min
Response: 415708
Conc: 17.63 ng/ml