

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081319\
 Data File : FB022003.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2019 13:13
 Operator : DD/AJ
 Sample : K4089-01MSD
 Misc : 5.06/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 13 15:26:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	276543	20.265 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	733551	26.601 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	642159	24.293 ng/ml
3) t n-Heptane	7.952	191315	7.716 ng/ml
4) t Benzene	8.087	289925	9.924 ng/ml
6) t Toluene	10.834	596203	28.975 ng/ml
7) t Ethylbenzene	13.280	205004	9.854 ng/ml
8) t m-Xylene	13.413	437486	19.693 ng/ml
9) t O-Xylene	14.143	454723	19.768 ng/ml
10) t 1,2,4-Trimethylbenzene	16.422	437934	18.575 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081319\
Data File : FB022003.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2019 13:13
Operator : DD/AJ
Sample : K4089-01MSD
Misc : 5.06/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 13 15:26:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

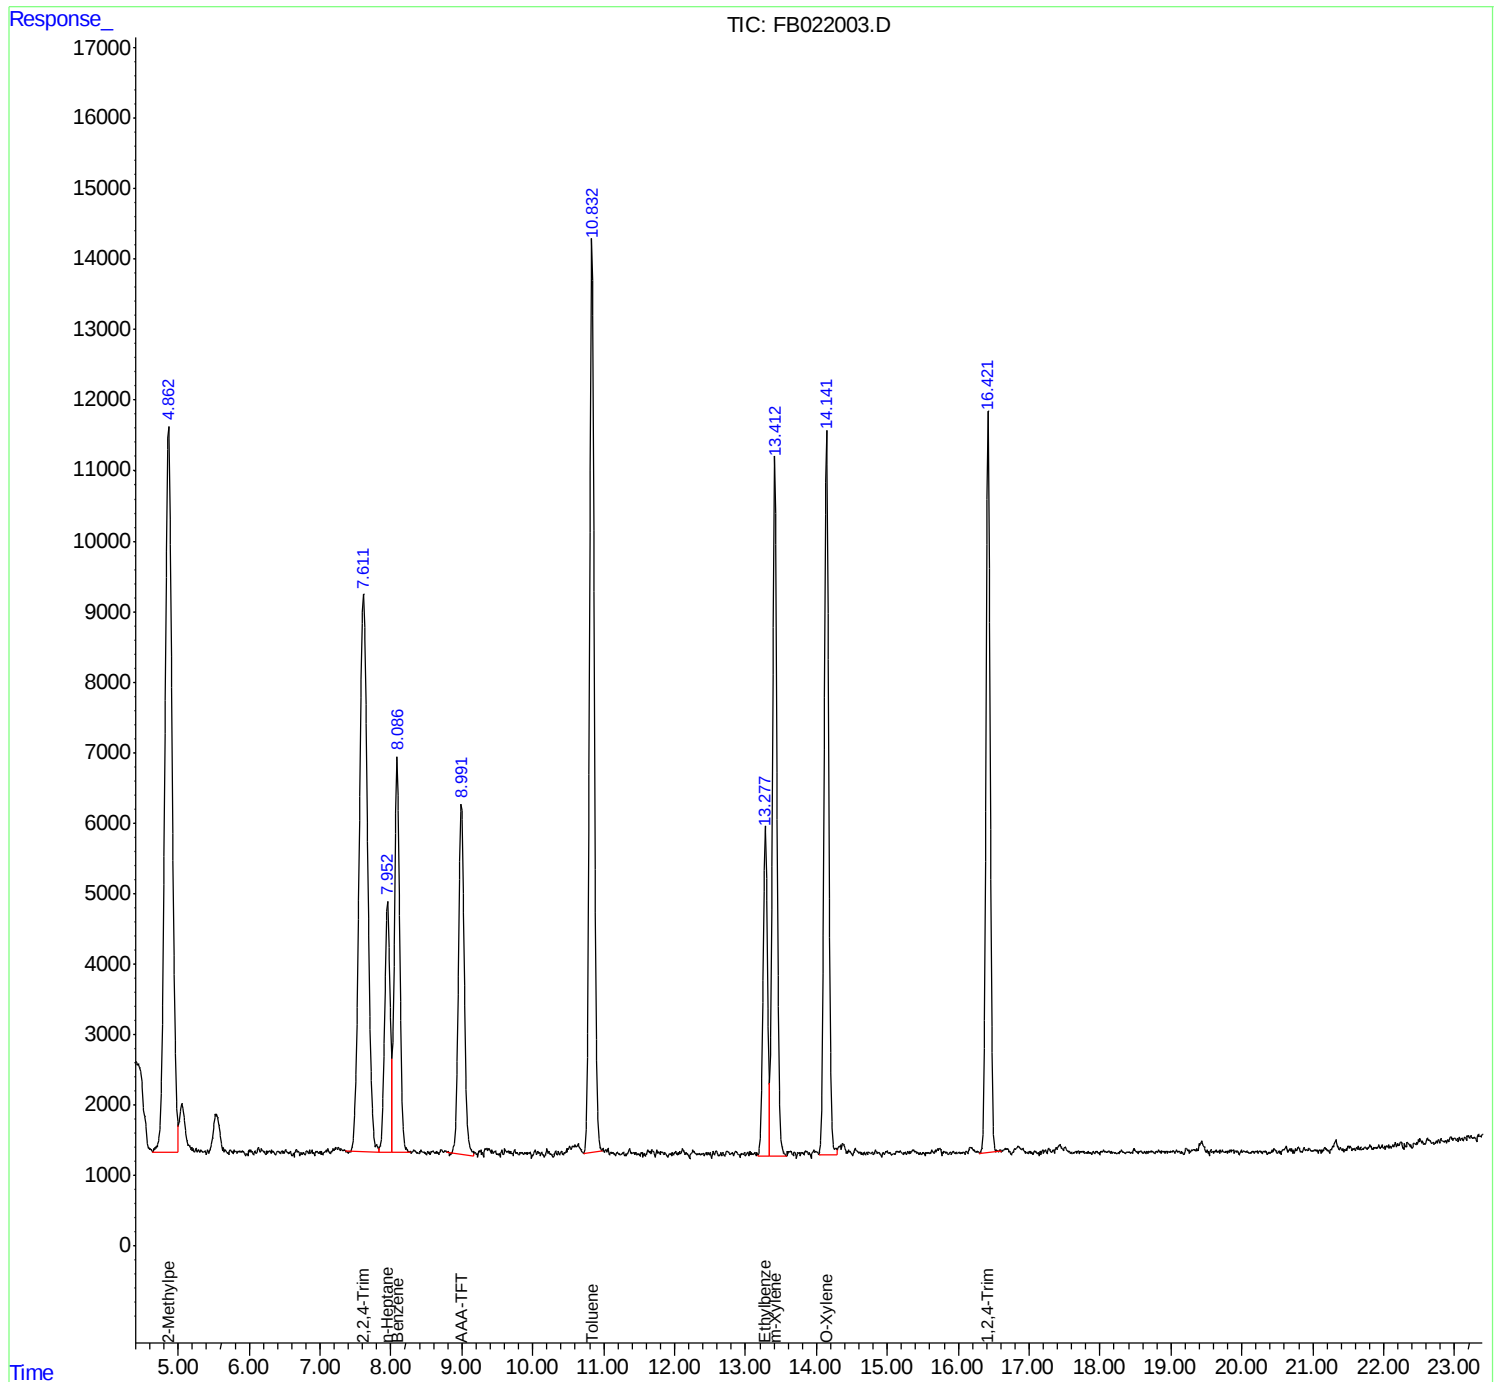

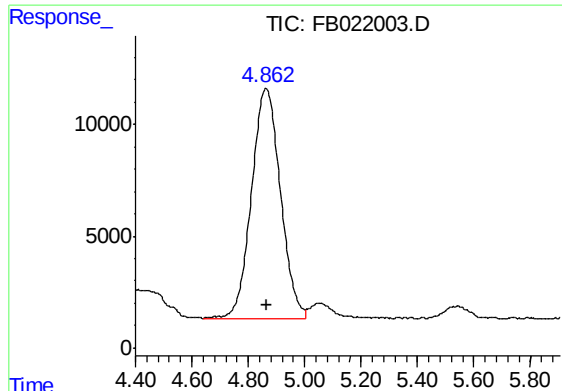


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 733551
Conc: 26.60 ng/ml

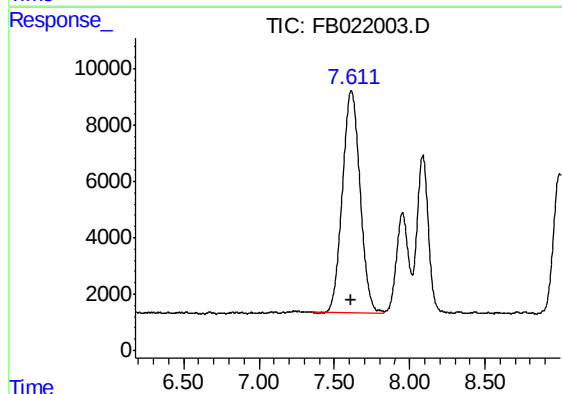


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 642159
Conc: 24.29 ng/ml

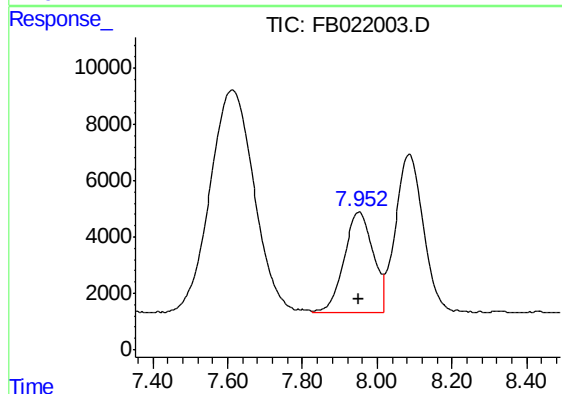


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.000 min
Response: 191315
Conc: 7.72 ng/ml

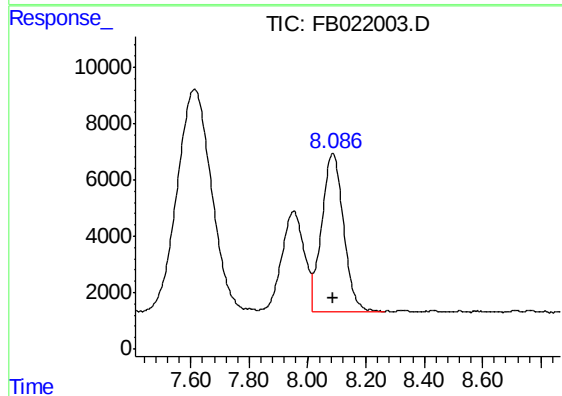


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 289925
Conc: 9.92 ng/ml

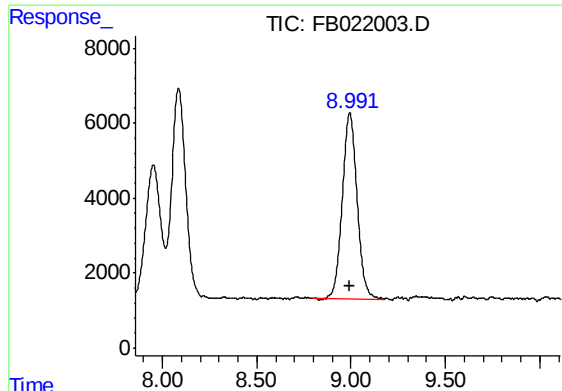


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 276543
Conc: 20.26 ng/ml

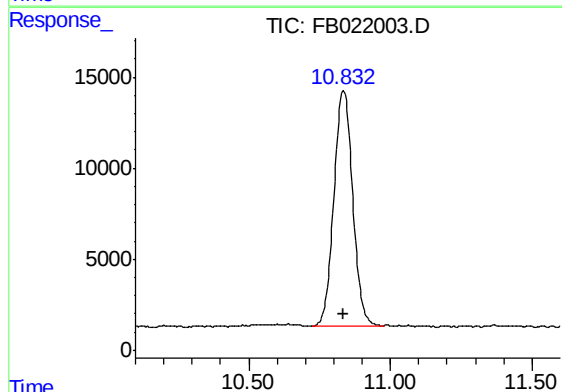


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.001 min
Response: 596203
Conc: 28.98 ng/ml

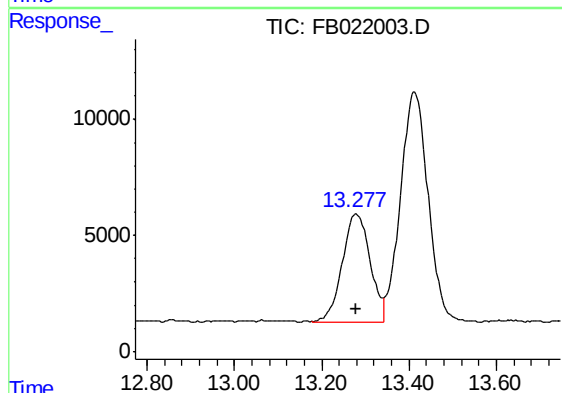


#7 Ethylbenzene

R.T.: 13.280 min
Delta R.T.: 0.002 min
Response: 205004
Conc: 9.85 ng/ml

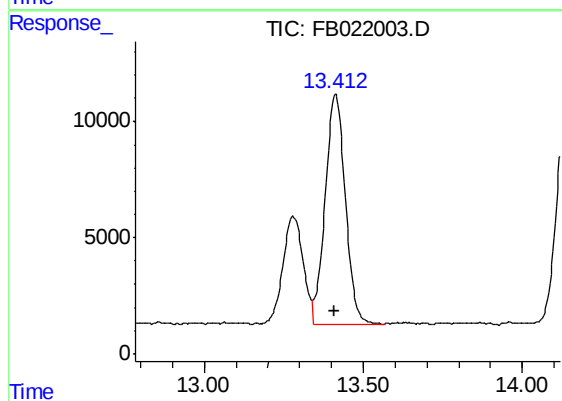

#8 m-Xylene

R.T.: 13.413 min
Delta R.T.: 0.002 min
Response: 437486
Conc: 19.69 ng/ml

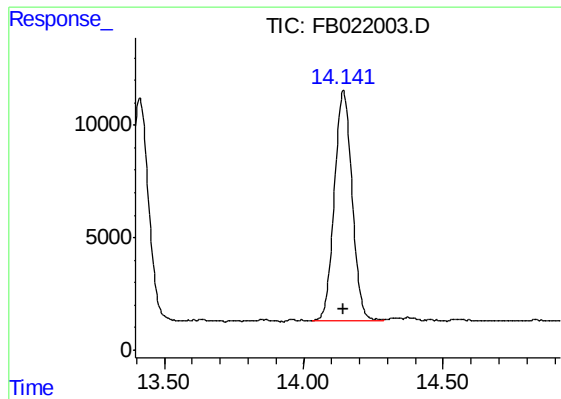


#9 O-Xylene

R.T.: 14.143 min

Delta R.T.: 0.002 min

Response: 454723

Conc: 19.77 ng/ml

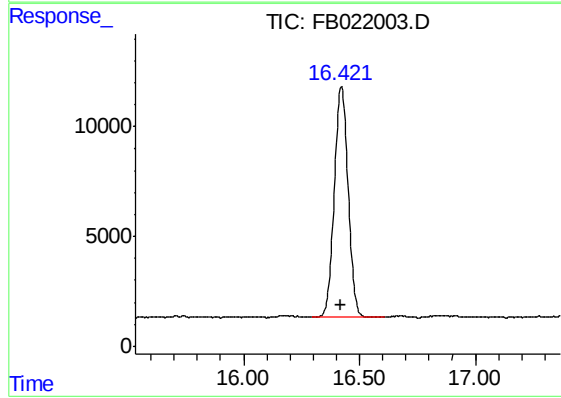

#10 1,2,4-Trimethylbenzene

R.T.: 16.422 min

Delta R.T.: 0.003 min

Response: 437934

Conc: 18.57 ng/ml