

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081320\
 Data File : FB024745.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2020 9:53
 Operator : DD/AJ
 Sample : BSF0810S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 14 01:47:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
 Quant Title :
 QLast Update : Mon Aug 10 12:11:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	391047	18.938 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	731180	30.384 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	843918	30.445 ng/ml
3) t n-Heptane	7.758	276694	10.176 ng/ml
4) t Benzene	7.892	342466	9.759 ng/ml
6) t Toluene	10.629	995876	28.911 ng/ml
7) t Ethylbenzene	13.069	288947	9.026 ng/ml
8) t m-Xylene	13.201	577859	18.518 ng/ml
9) t O-Xylene	13.929	561372	18.562 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	464567	18.916 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081320\
Data File : FB024745.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2020 9:53
Operator : DD/AJ
Sample : BSF0810S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 14 01:47:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

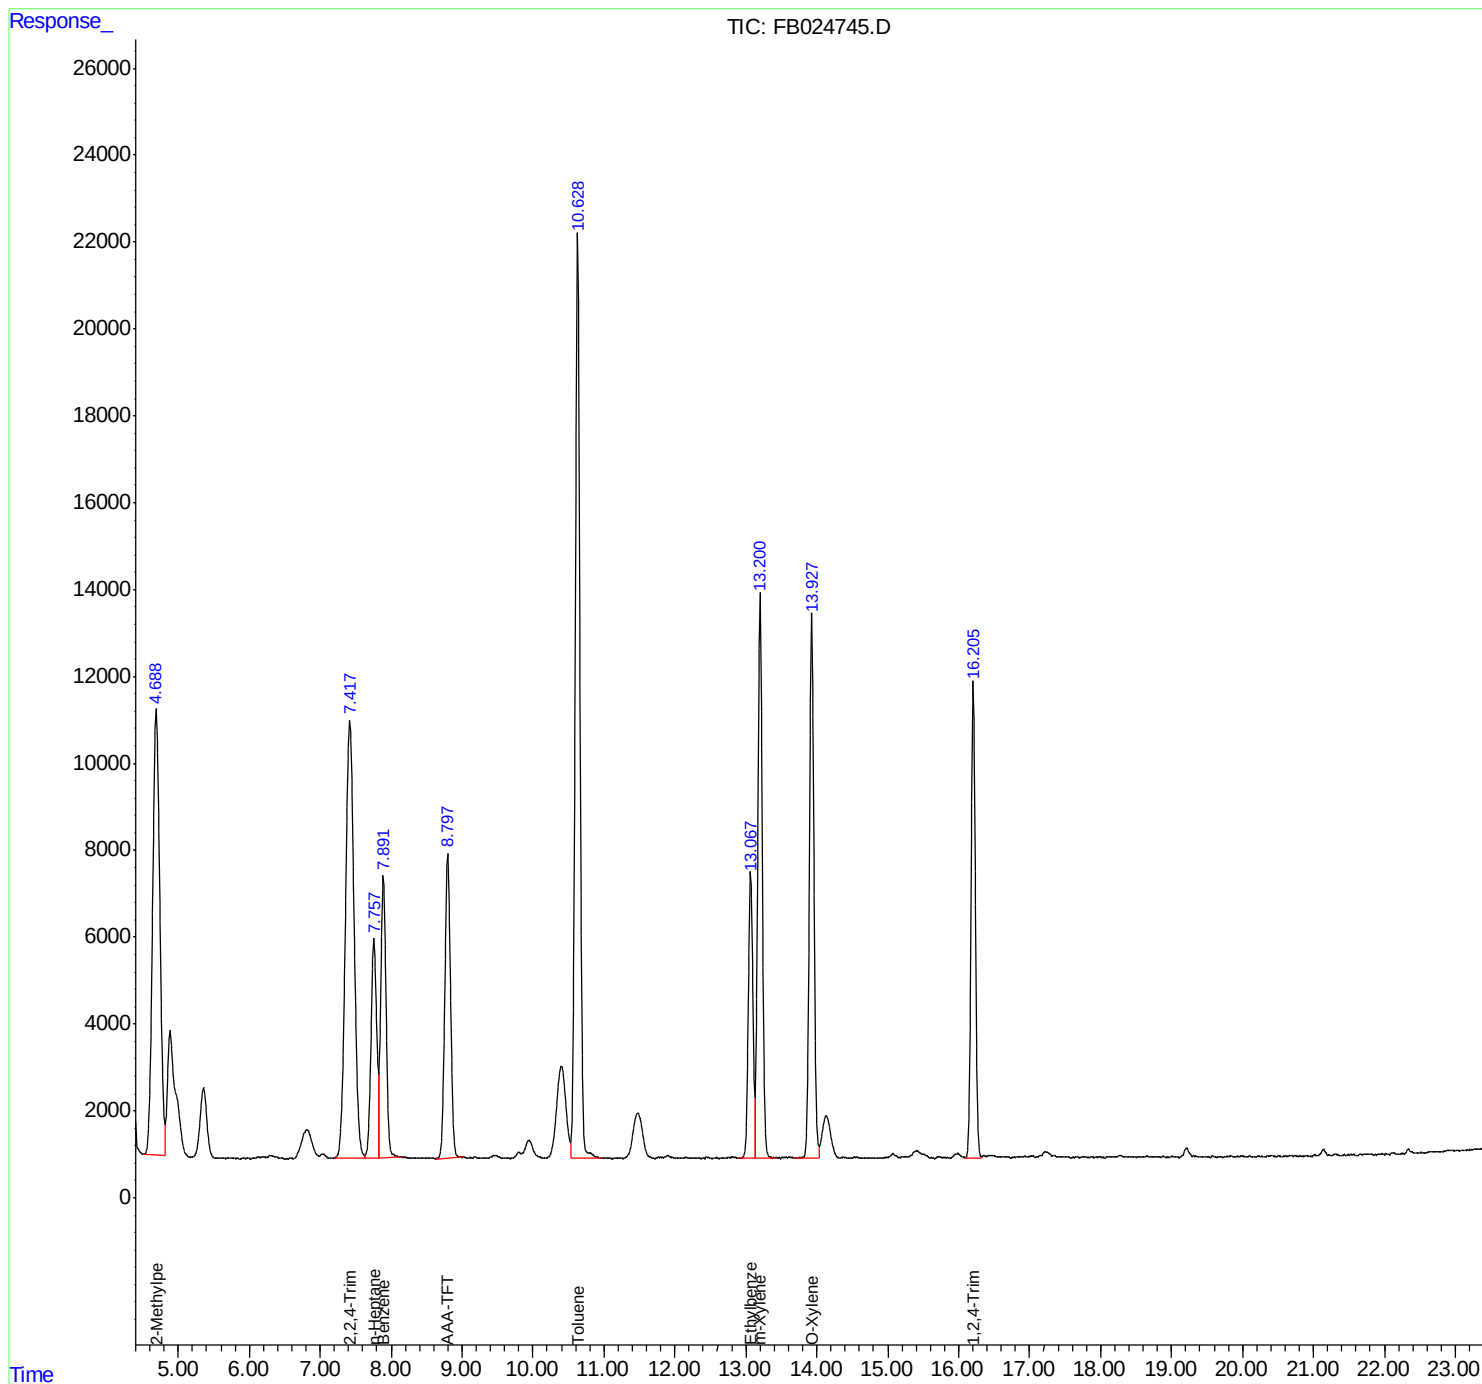

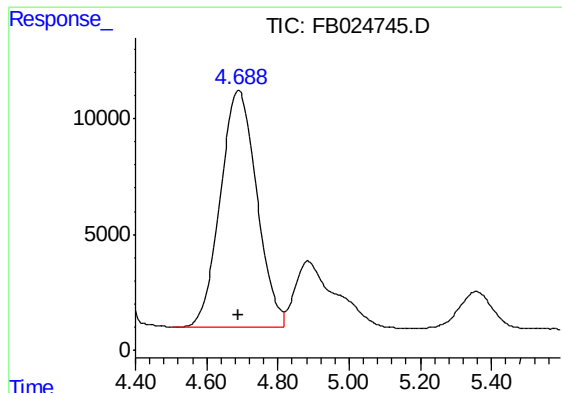


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 731180
Conc: 30.38 ng/ml

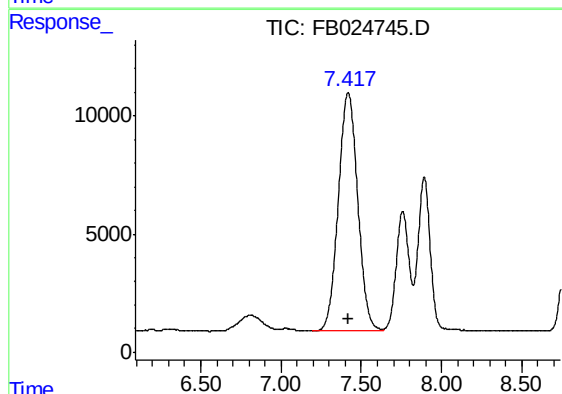


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 843918
Conc: 30.44 ng/ml

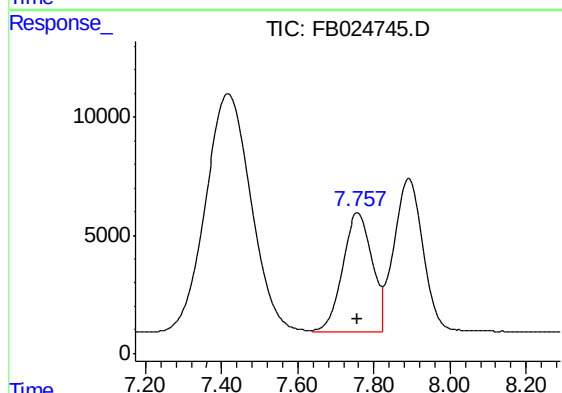


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 276694
Conc: 10.18 ng/ml

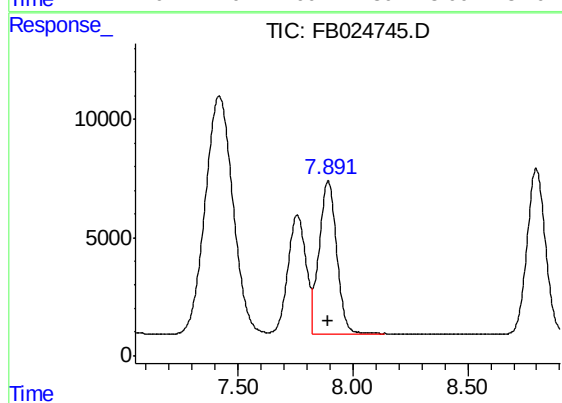


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 342466
Conc: 9.76 ng/ml

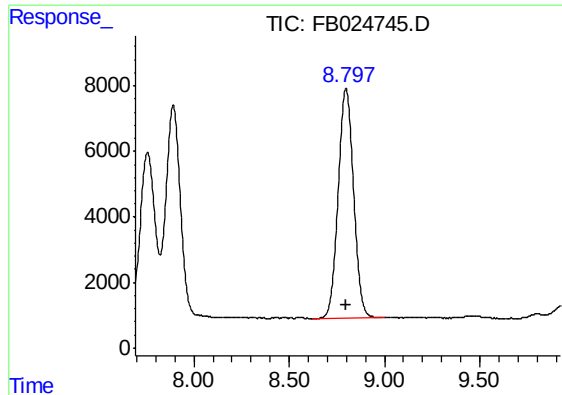


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 391047
Conc: 18.94 ng/ml

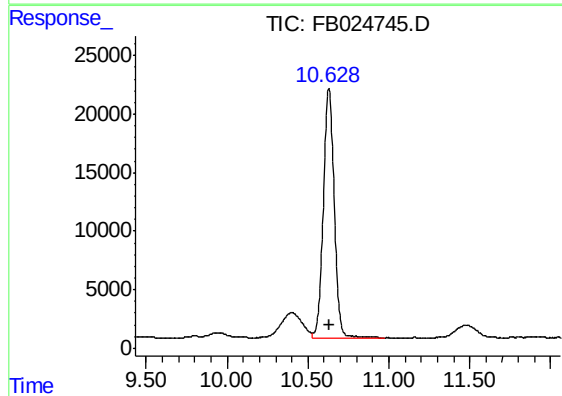


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 995876
Conc: 28.91 ng/ml

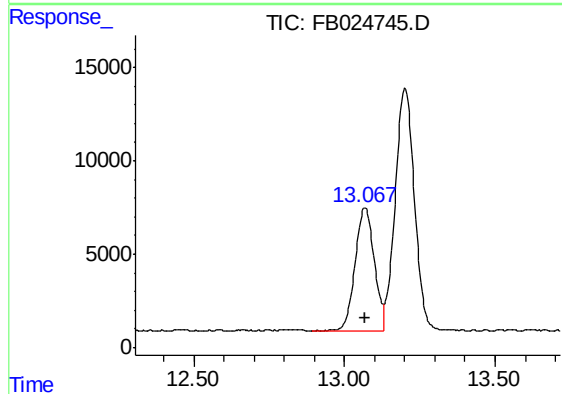


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.000 min
Response: 288947
Conc: 9.03 ng/ml

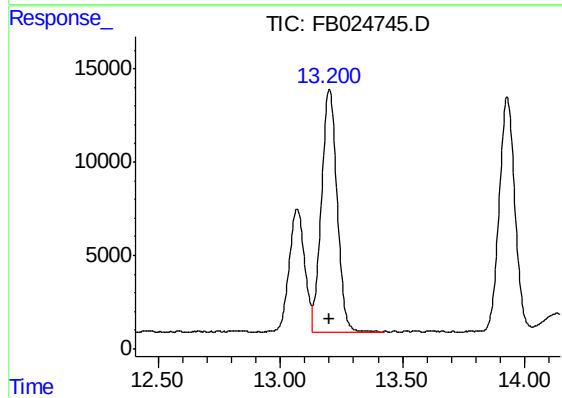


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: 0.000 min
Response: 577859
Conc: 18.52 ng/ml

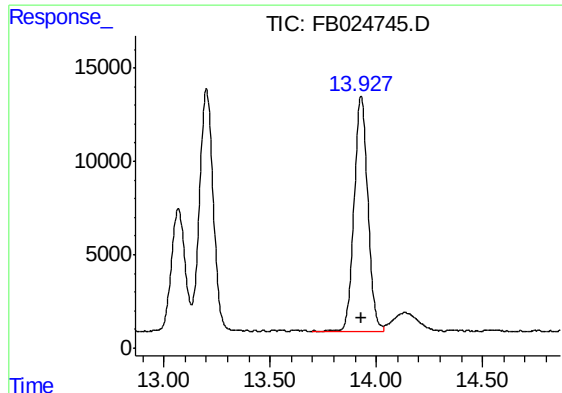

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 561372
Conc: 18.56 ng/ml

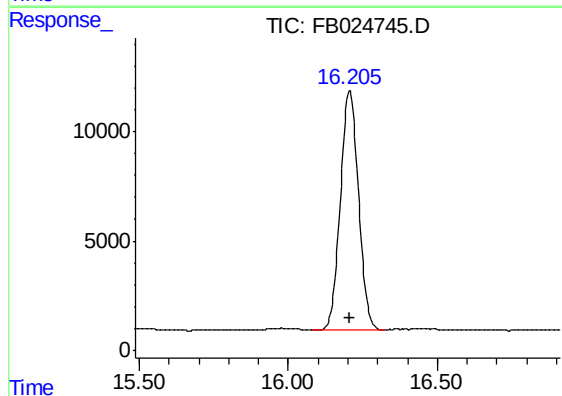

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 464567
Conc: 18.92 ng/ml