

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
 Data File : FB026148.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2021 16:40
 Operator : AJ/MA
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 13 22:06:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
 Quant Title :
 QLast Update : Fri Aug 13 22:06:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.846	73688	4.853 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.846	168134	7.675 ng/ml
2) t 2,2,4-Trimethylpentane	7.509	175296	8.224 ng/ml
3) t n-Heptane	7.821	68959	2.105 ng/ml
4) t Benzene	7.960	73038	2.188 ng/ml
6) t Toluene	10.657	211153	7.178 ng/ml
7) t Ethylbenzene	13.077	59292	2.401 ng/ml
8) t m-Xylene	13.209	117080	4.945 ng/ml
9) t O-Xylene	13.933	103678	4.933 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	108420	5.468 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
Data File : FB026148.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2021 16:40
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 13 22:06:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:06:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

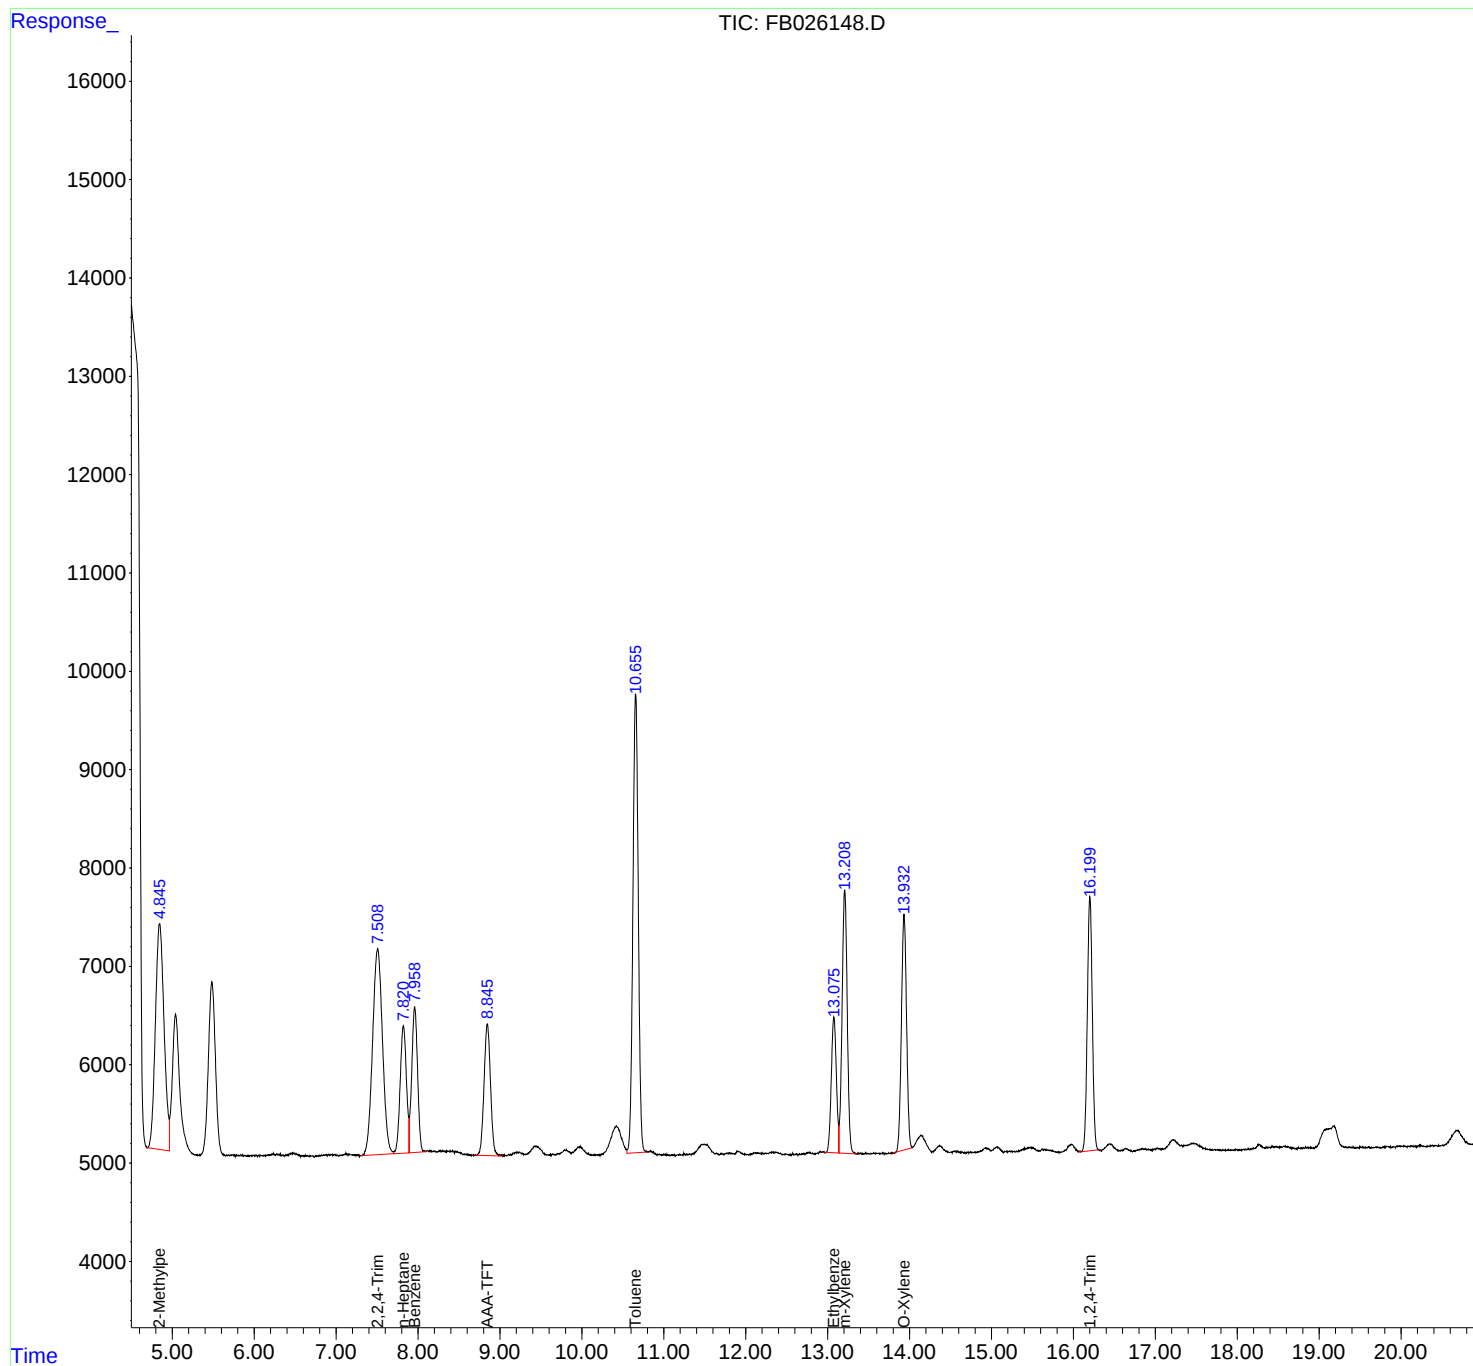


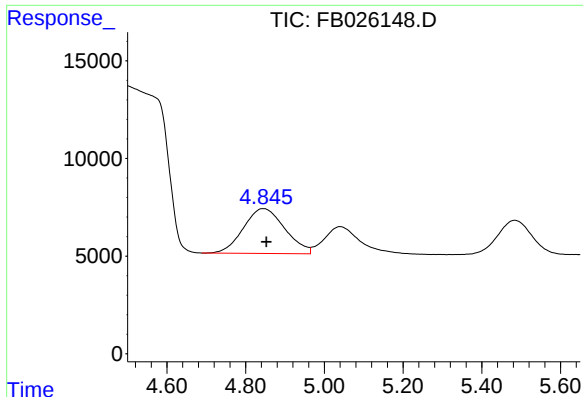

#1 2-Methylpentane


R.T.: 4.846 min
Delta R.T.: -0.007 min
Response: 168134
Conc: 7.68 ng/ml

Instrument :
FID_B
ClientSampleId :

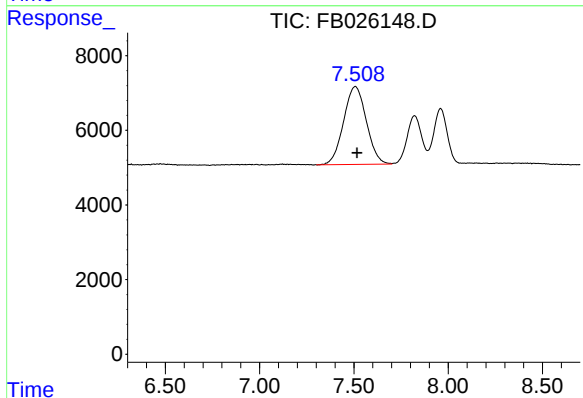


#2 2,2,4-Trimethylpentane

R.T.: 7.509 min
Delta R.T.: -0.008 min
Response: 175296
Conc: 8.22 ng/ml

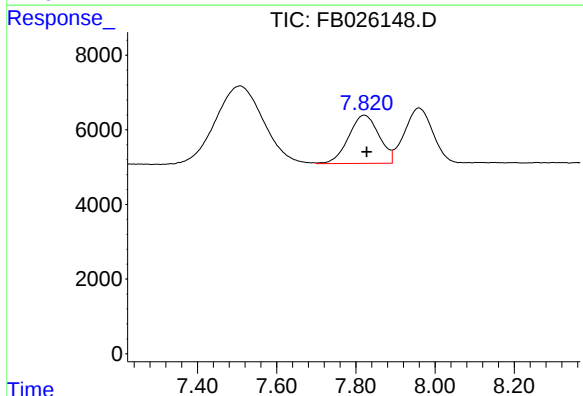


#3 n-Heptane

R.T.: 7.821 min
Delta R.T.: -0.006 min
Response: 68959
Conc: 2.10 ng/ml

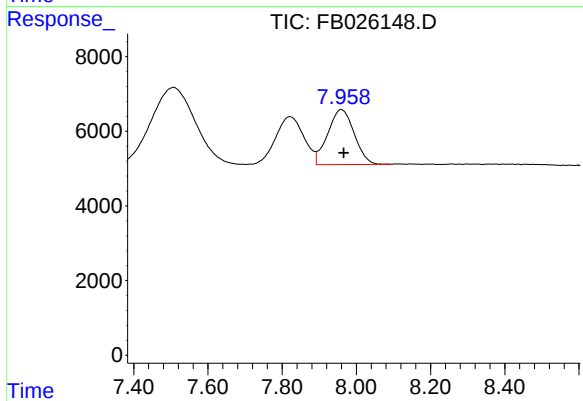

#4 Benzene


R.T.: 7.960 min
Delta R.T.: -0.006 min
Response: 73038
Conc: 2.19 ng/ml

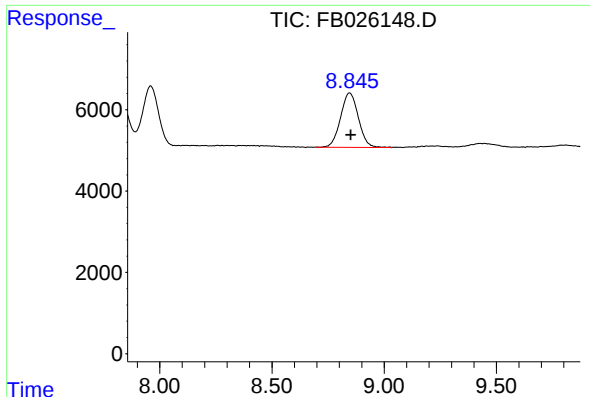

#5 AAA-TFT


R.T.: 8.846 min
Delta R.T.: -0.005 min
Response: 73688
Conc: 4.85 ng/ml

Instrument :
FID_B
ClientSampleId :

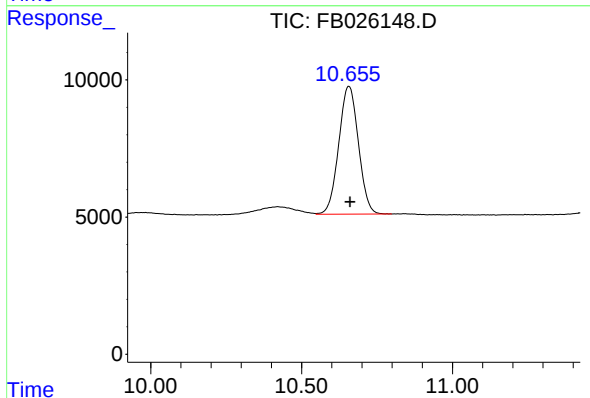


#6 Toluene

R.T.: 10.657 min
Delta R.T.: -0.004 min
Response: 211153
Conc: 7.18 ng/ml

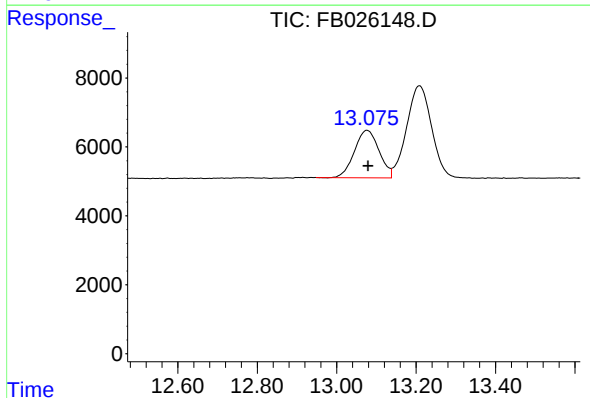


#7 Ethylbenzene

R.T.: 13.077 min
Delta R.T.: -0.002 min
Response: 59292
Conc: 2.40 ng/ml

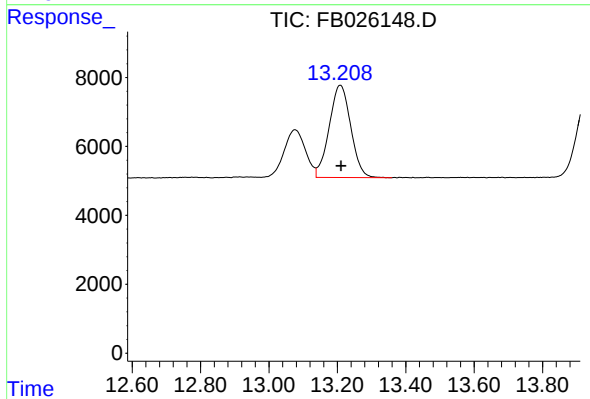

#8 m-Xylene


R.T.: 13.209 min
Delta R.T.: -0.002 min
Response: 117080
Conc: 4.94 ng/ml

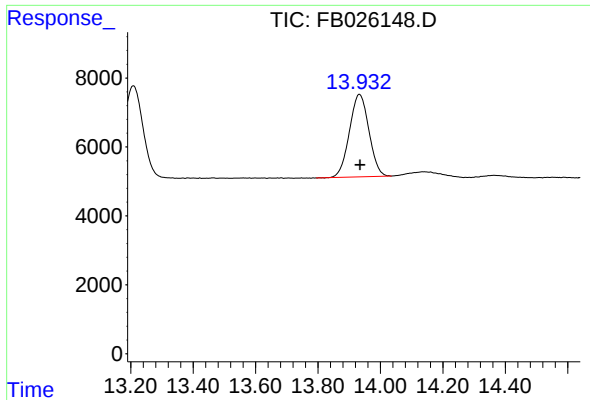

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: -0.002 min
Response: 103678
Conc: 4.93 ng/ml

Instrument :
FID_B
ClientSampleId :

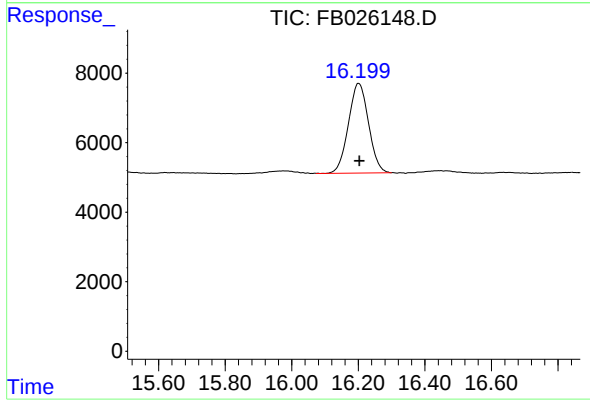

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.002 min
Response: 108420
Conc: 5.47 ng/ml