

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
 Data File : FB026150.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2021 18:00
 Operator : AJ/MA
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 13 22:07:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
 Quant Title :
 QLast Update : Fri Aug 13 22:06:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.851	303671	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.853	657199	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.517	639484	30.000 ng/ml
3) t n-Heptane	7.828	327665	10.000 ng/ml
4) t Benzene	7.966	333750	10.000 ng/ml
6) t Toluene	10.661	882443	30.000 ng/ml
7) t Ethylbenzene	13.079	246899	10.000 ng/ml
8) t m-Xylene	13.211	473536	20.000 ng/ml
9) t O-Xylene	13.935	420354	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	396581	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
Data File : FB026150.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2021 18:00
Operator : AJ/MA
Sample : 20 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 13 22:07:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:06:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

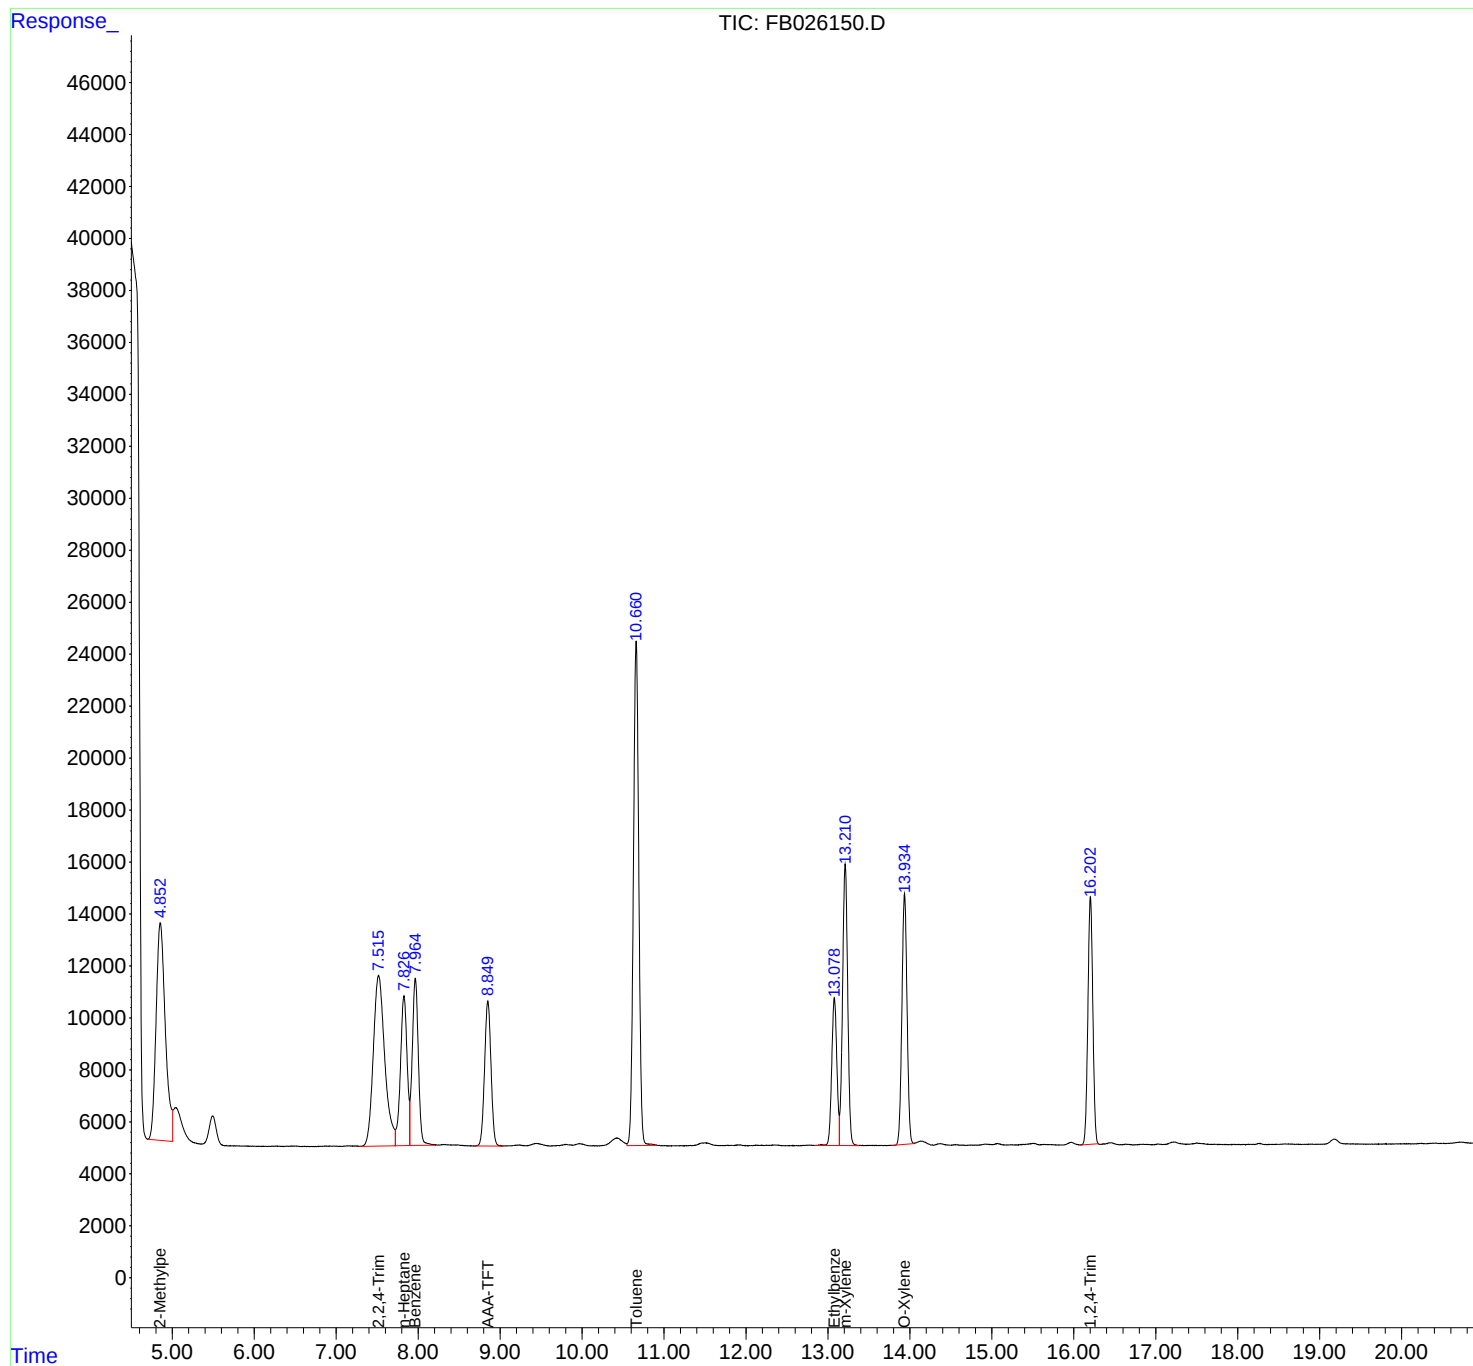


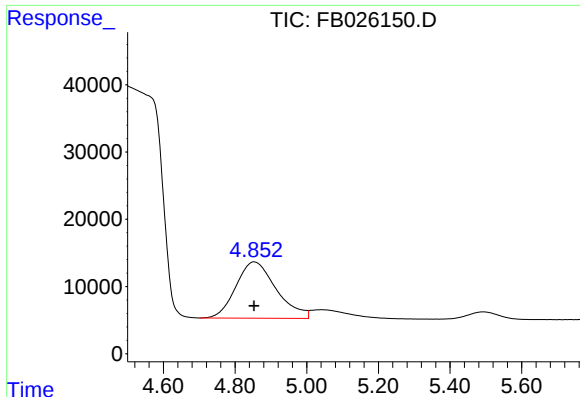

#1 2-Methylpentane


R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 657199
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :

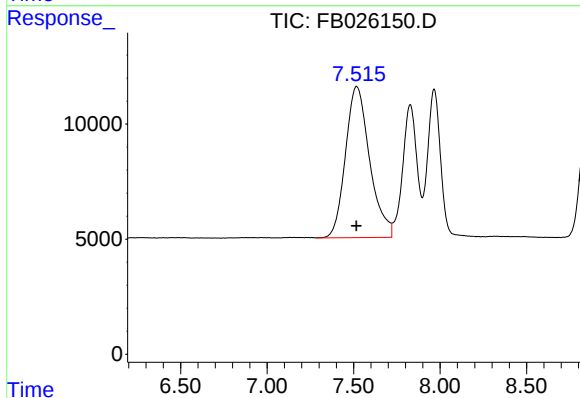


#2 2,2,4-Trimethylpentane

R.T.: 7.517 min
Delta R.T.: 0.000 min
Response: 639484
Conc: 30.00 ng/ml

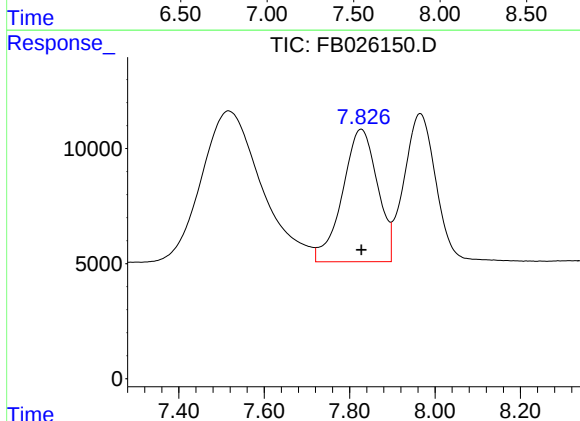


#3 n-Heptane

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 327665
Conc: 10.00 ng/ml

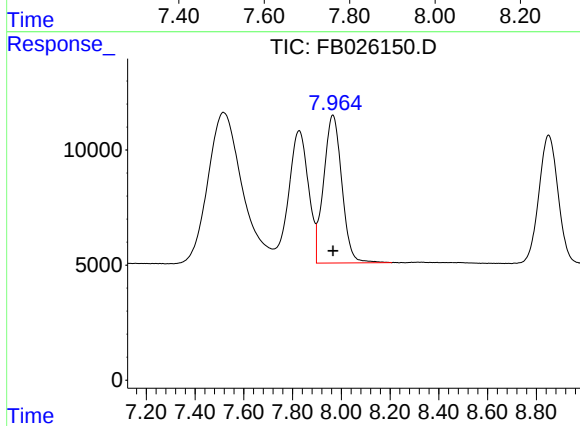

#4 Benzene


R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 333750
Conc: 10.00 ng/ml

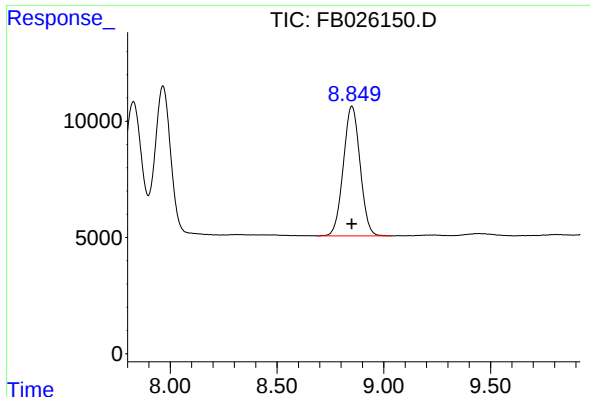

#5 AAA-TFT


R.T.: 8.851 min
Delta R.T.: 0.000 min
Response: 303671
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

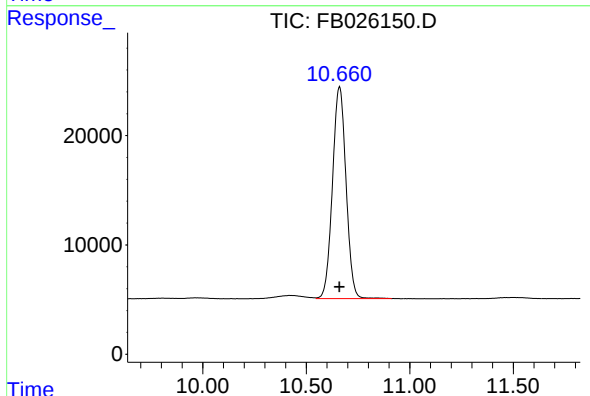


#6 Toluene

R.T.: 10.661 min
Delta R.T.: 0.000 min
Response: 882443
Conc: 30.00 ng/ml

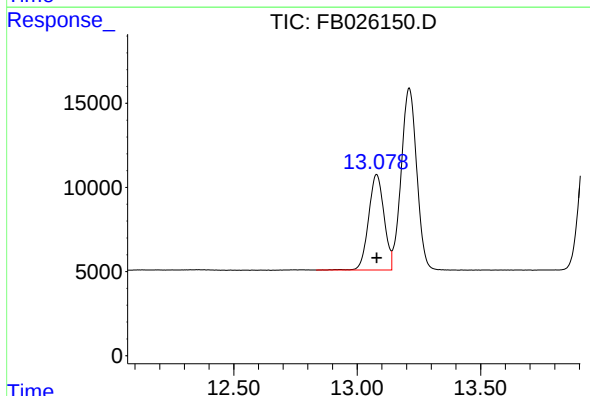


#7 Ethylbenzene

R.T.: 13.079 min
Delta R.T.: 0.000 min
Response: 246899
Conc: 10.00 ng/ml

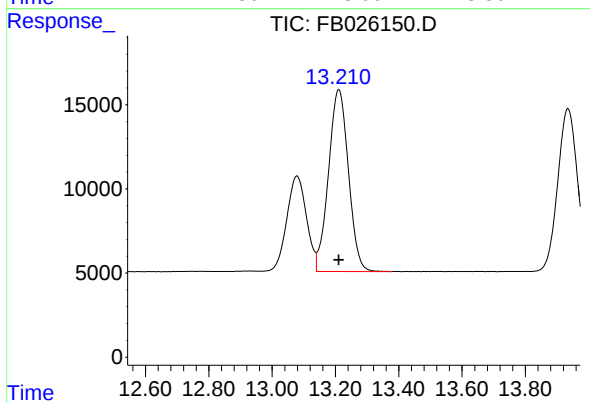

#8 m-Xylene


R.T.: 13.211 min
Delta R.T.: 0.000 min
Response: 473536
Conc: 20.00 ng/ml

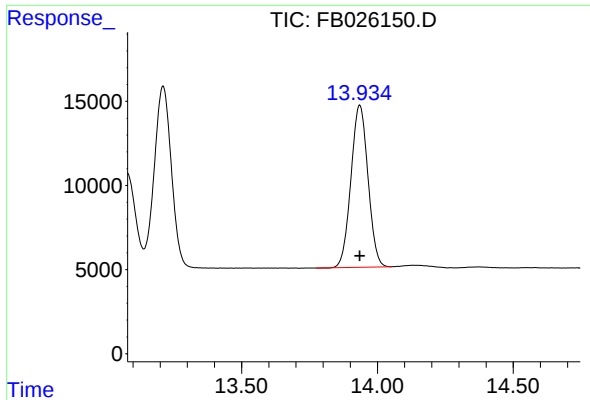

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.000 min
Response: 420354
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

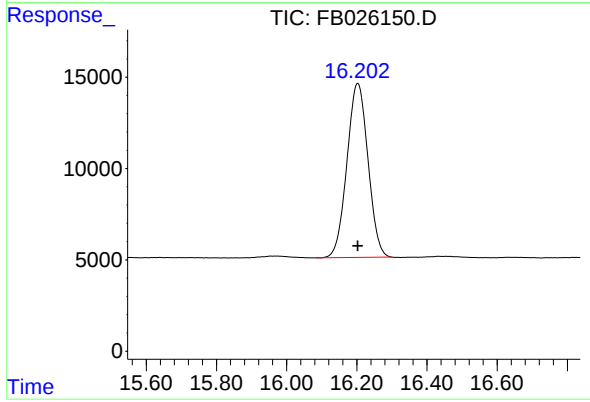

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: 0.000 min
Response: 396581
Conc: 20.00 ng/ml