

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
 Data File : FB026152.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2021 19:20
 Operator : AJ/MA
 Sample : 100 GRO STD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 13 22:07:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
 Quant Title :
 QLast Update : Fri Aug 13 22:06:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.847	1514025	99.715 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.842	3488430	159.241 ng/ml
2) t 2,2,4-Trimethylpentane	7.515	3176163	149.003 ng/ml
3) t n-Heptane	7.822	1610623	49.155 ng/ml
4) t Benzene	7.960	1666572	49.935 ng/ml
6) t Toluene	10.658	4399567	149.570 ng/ml
7) t Ethylbenzene	13.077	1233905	49.976 ng/ml
8) t m-Xylene	13.209	2357355	99.564 ng/ml
9) t O-Xylene	13.934	2095566	99.705 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	1935957	97.632 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
Data File : FB026152.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2021 19:20
Operator : AJ/MA
Sample : 100 GRO STD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 13 22:07:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:06:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

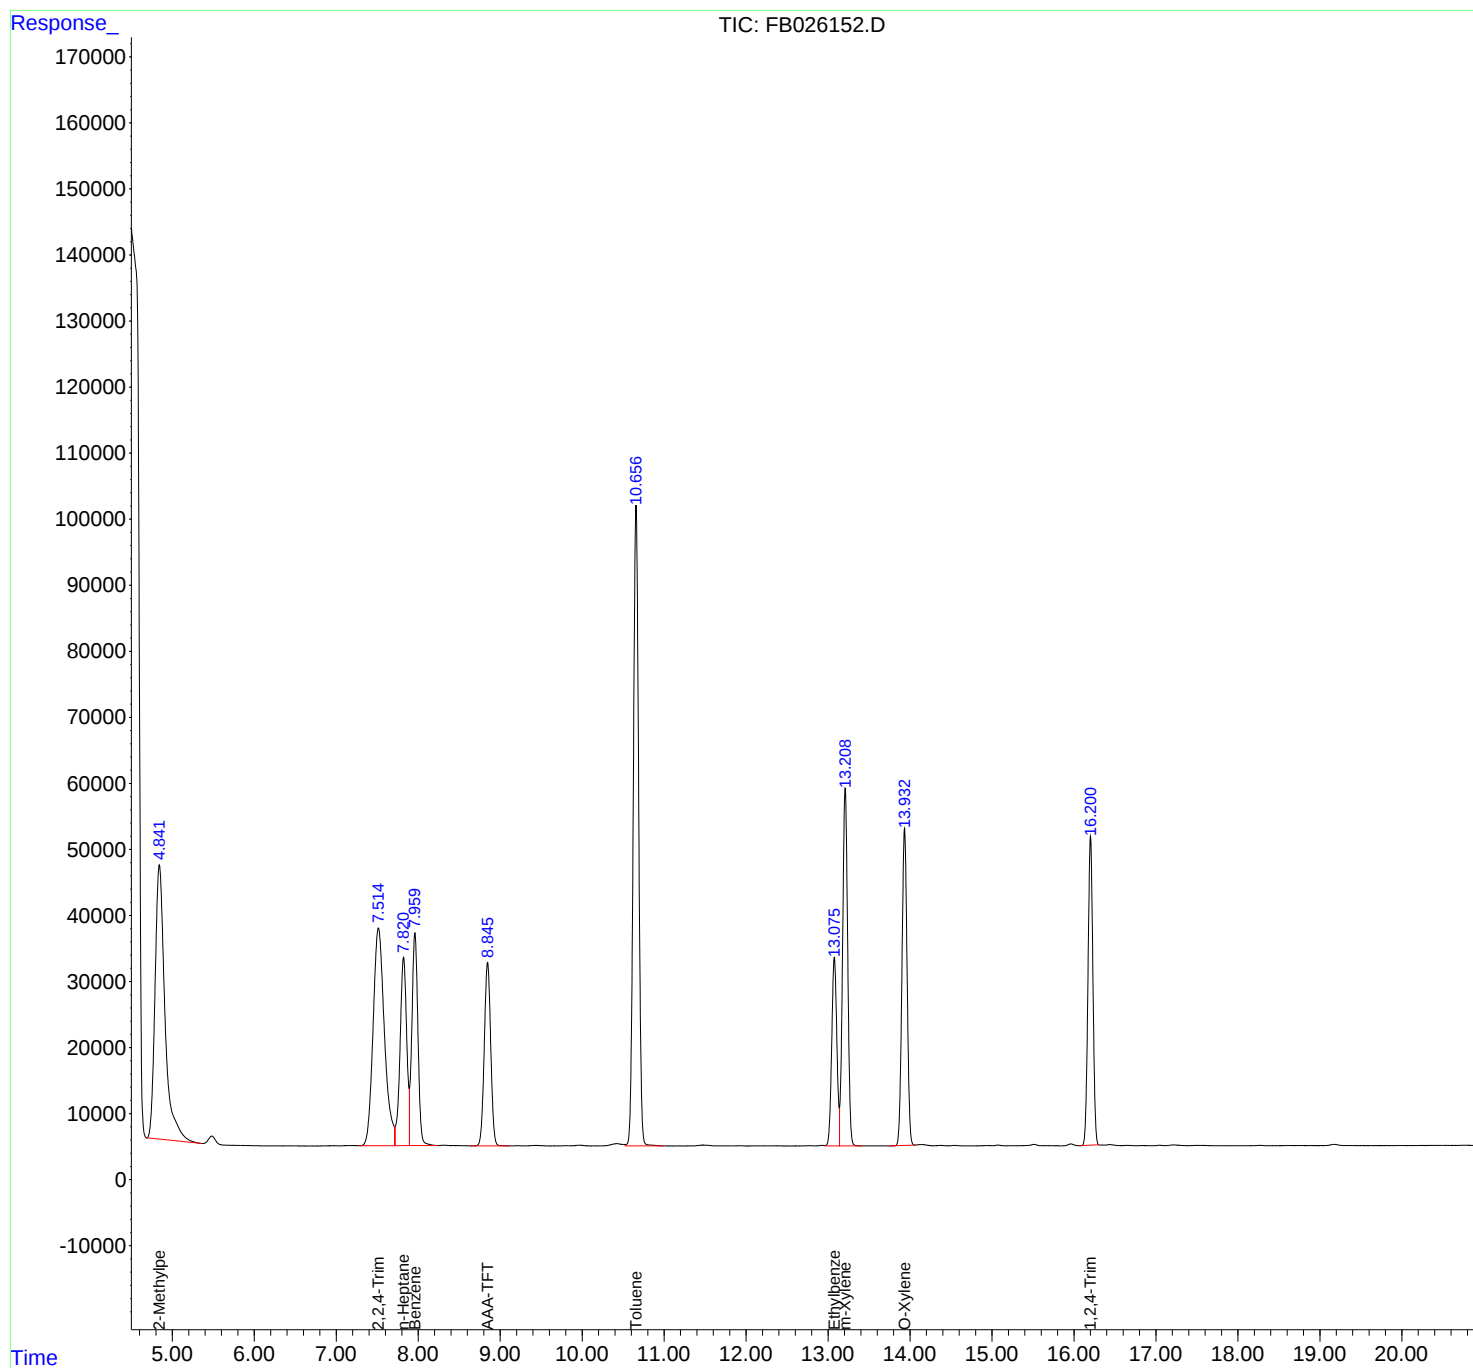


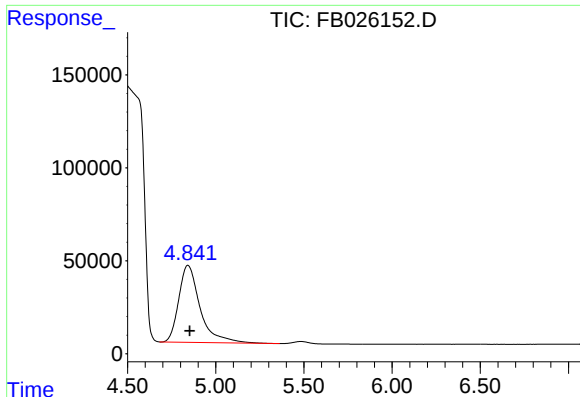

#1 2-Methylpentane


R.T.: 4.842 min
Delta R.T.: -0.011 min
Response: 3488430
Conc: 159.24 ng/ml

Instrument :
FID_B
ClientSampleId :

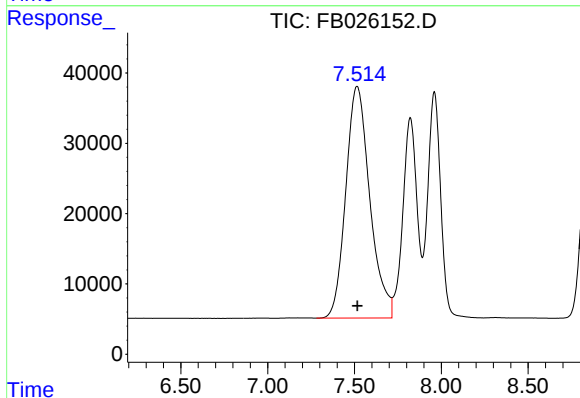


#2 2,2,4-Trimethylpentane

R.T.: 7.515 min
Delta R.T.: -0.002 min
Response: 3176163
Conc: 149.00 ng/ml

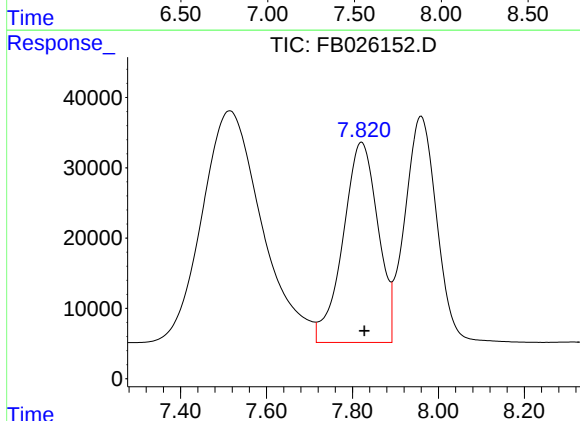


#3 n-Heptane

R.T.: 7.822 min
Delta R.T.: -0.006 min
Response: 1610623
Conc: 49.15 ng/ml

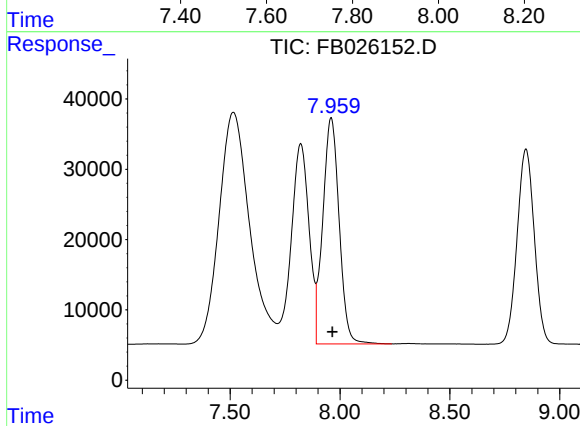

#4 Benzene


R.T.: 7.960 min
Delta R.T.: -0.006 min
Response: 1666572
Conc: 49.93 ng/ml

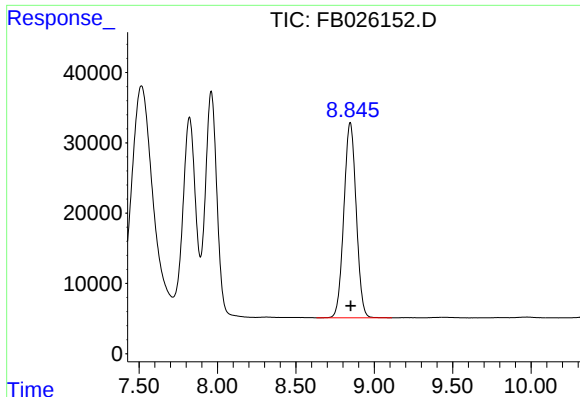

#5 AAA-TFT


R.T.: 8.847 min
Delta R.T.: -0.004 min
Response: 1514025
Conc: 99.71 ng/ml

Instrument :
FID_B
ClientSampleId :

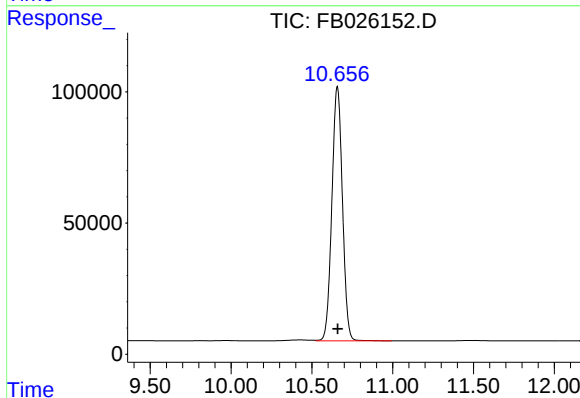


#6 Toluene

R.T.: 10.658 min
Delta R.T.: -0.003 min
Response: 4399567
Conc: 149.57 ng/ml

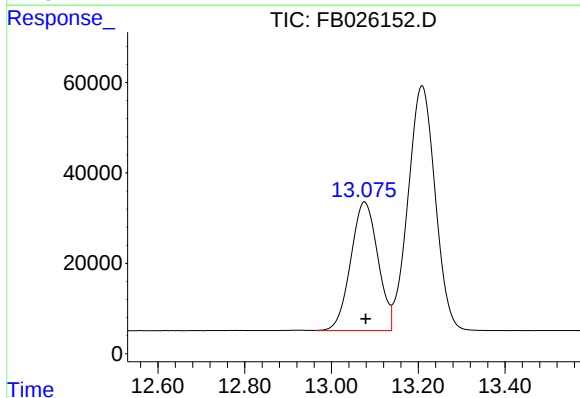


#7 Ethylbenzene

R.T.: 13.077 min
Delta R.T.: -0.002 min
Response: 1233905
Conc: 49.98 ng/ml

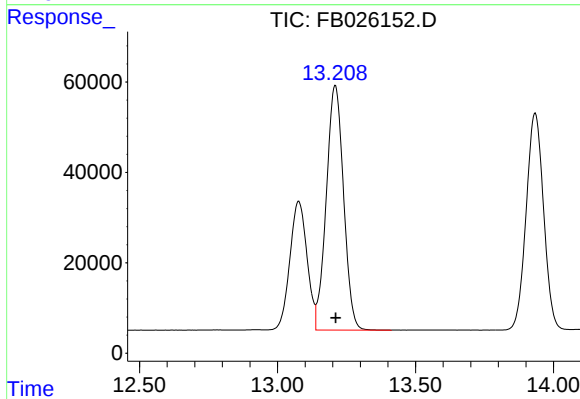

#8 m-Xylene

R.T.: 13.209 min
Delta R.T.: -0.002 min
Response: 2357355
Conc: 99.56 ng/ml

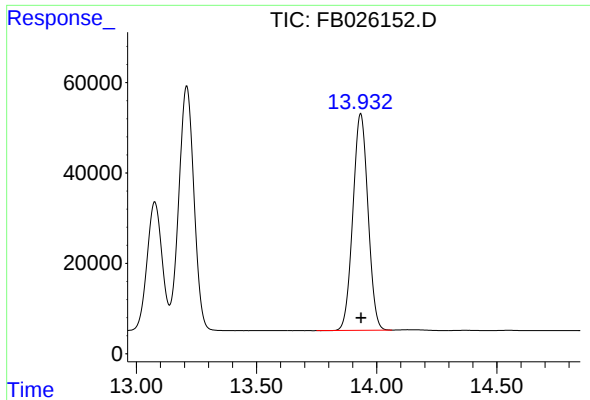

#9 O-Xylene


R.T.: 13.934 min

Delta R.T.: -0.002 min

Response: 2095566

Conc: 99.70 ng/ml

Instrument :
FID_B
ClientSampleId :

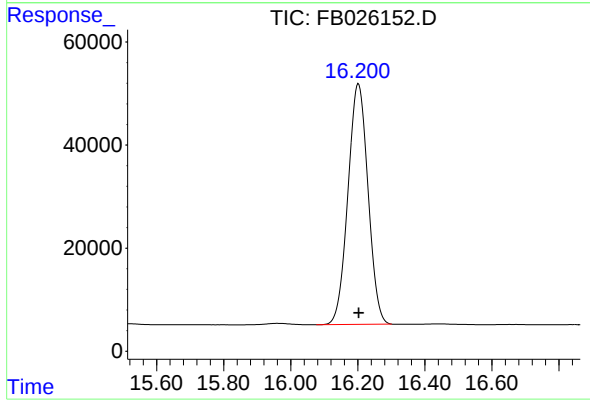

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min

Delta R.T.: -0.001 min

Response: 1935957

Conc: 97.63 ng/ml