

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
 Data File : FB026153.D
 Signal(s) : FID2B.CH
 Acq On : 13 Aug 2021 20:00
 Operator : AJ/MA
 Sample : FB081321GROICV
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 13 22:14:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
 Quant Title :
 QLast Update : Fri Aug 13 22:11:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.843	286028	19.194 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.835	653335	28.939 ng/ml
2) t 2,2,4-Trimethylpentane	7.503	684128	31.120 ng/ml
3) t n-Heptane	7.818	272222	9.036 ng/ml
4) t Benzene	7.956	297385	9.412 ng/ml
6) t Toluene	10.655	852444	29.613 ng/ml
7) t Ethylbenzene	13.076	242087	10.028 ng/ml
8) t m-Xylene	13.208	470244	20.120 ng/ml
9) t O-Xylene	13.933	424470	20.402 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	416641	20.653 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
Data File : FB026153.D
Signal(s) : FID2B.CH
Acq On : 13 Aug 2021 20:00
Operator : AJ/MA
Sample : FB081321GROICV
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 13 22:14:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:11:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

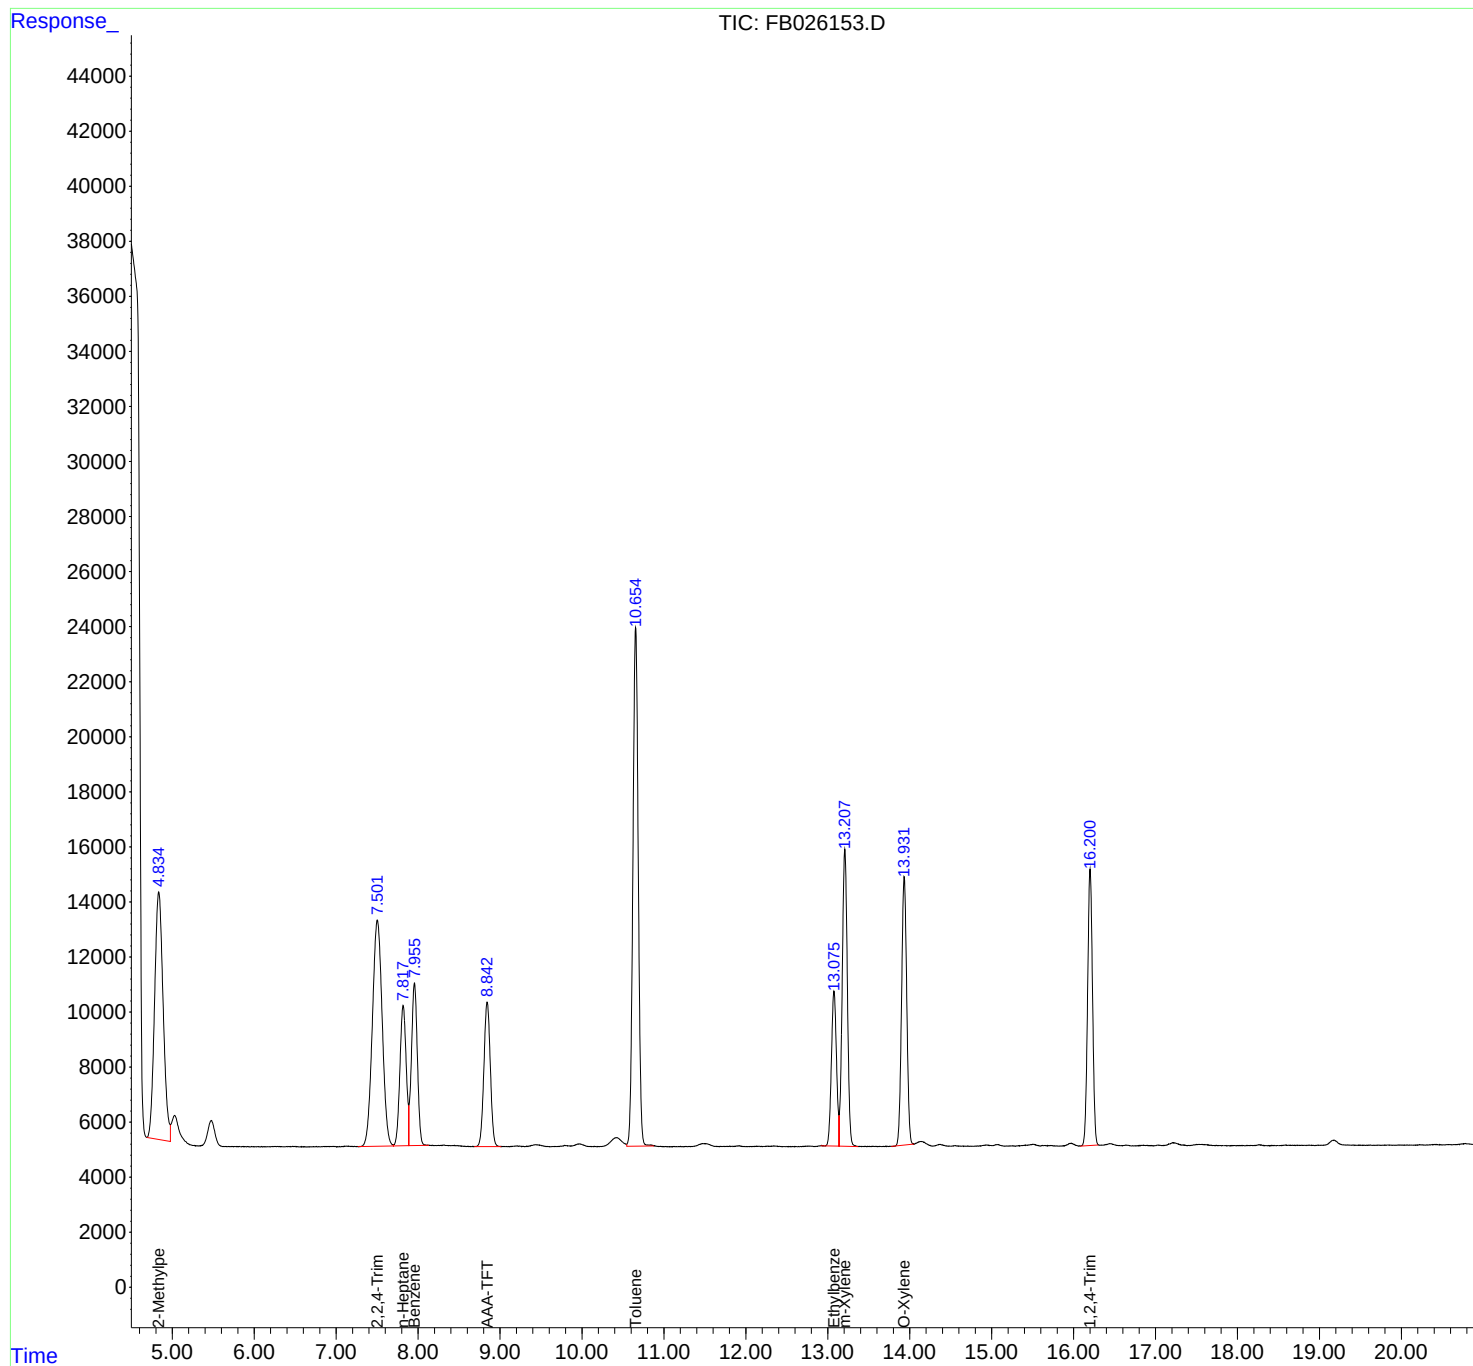


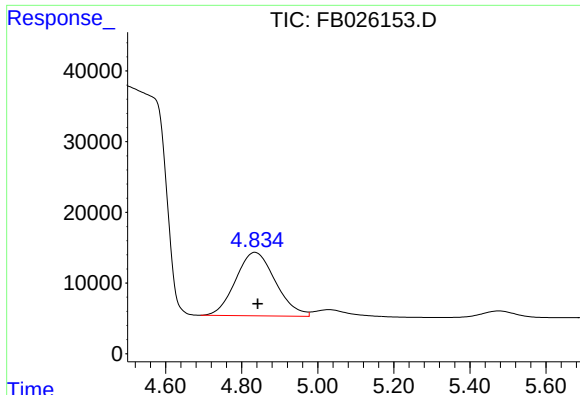

#1 2-Methylpentane


R.T.: 4.835 min
Delta R.T.: -0.007 min
Response: 653335
Conc: 28.94 ng/ml

Instrument :
FID_B
ClientSampleId :

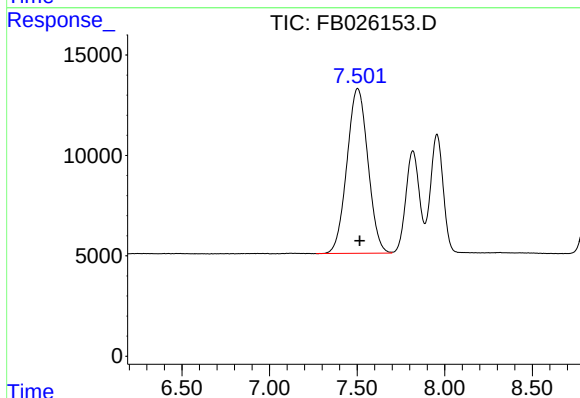


#2 2,2,4-Trimethylpentane

R.T.: 7.503 min
Delta R.T.: -0.012 min
Response: 684128
Conc: 31.12 ng/ml

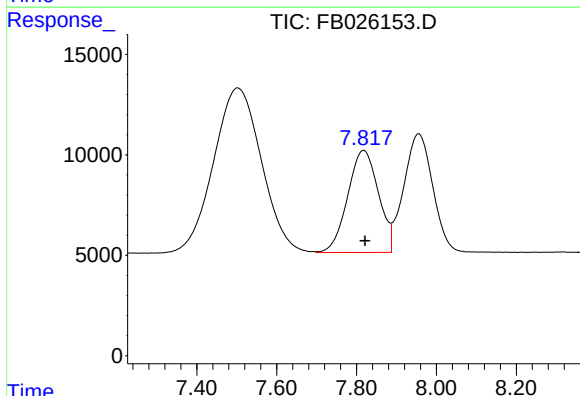


#3 n-Heptane

R.T.: 7.818 min
Delta R.T.: -0.003 min
Response: 272222
Conc: 9.04 ng/ml

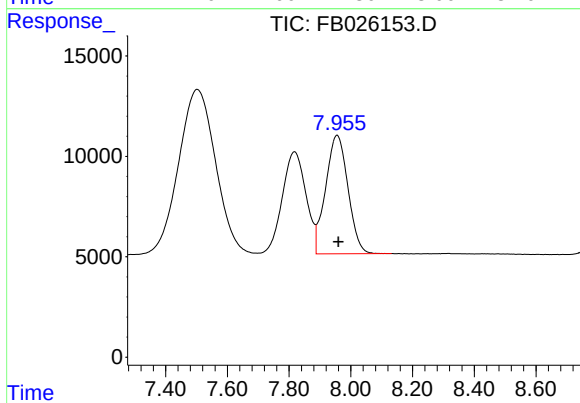

#4 Benzene


R.T.: 7.956 min
Delta R.T.: -0.004 min
Response: 297385
Conc: 9.41 ng/ml

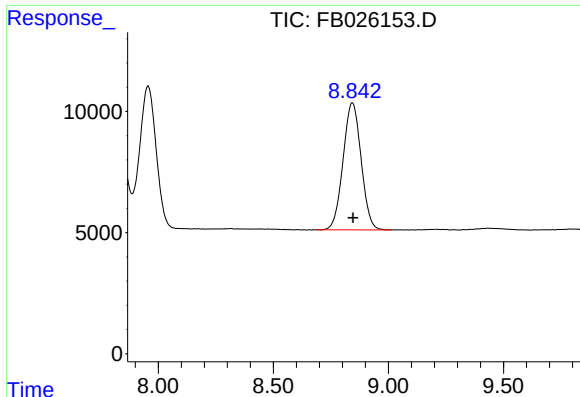

#5 AAA-TFT


R.T.: 8.843 min
Delta R.T.: -0.003 min
Response: 286028
Conc: 19.19 ng/ml

Instrument :
FID_B
ClientSampleId :

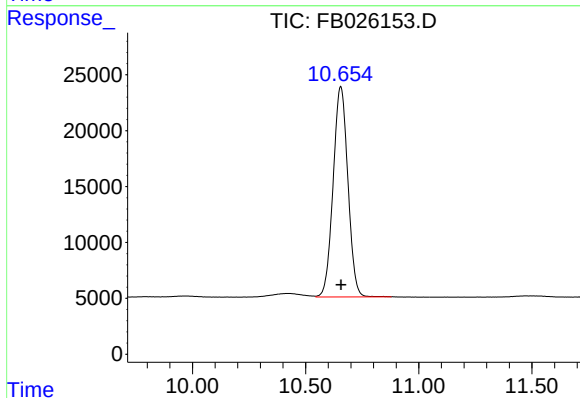


#6 Toluene

R.T.: 10.655 min
Delta R.T.: -0.002 min
Response: 852444
Conc: 29.61 ng/ml

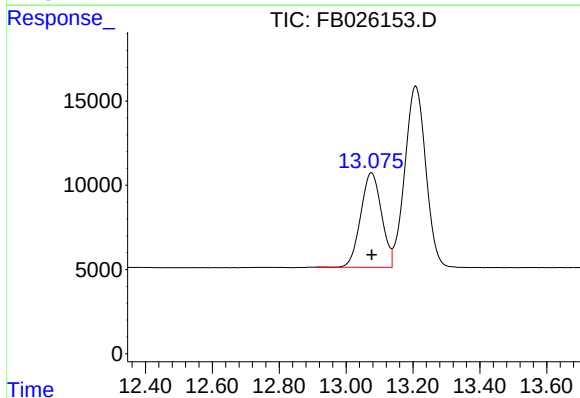


#7 Ethylbenzene

R.T.: 13.076 min
Delta R.T.: 0.000 min
Response: 242087
Conc: 10.03 ng/ml

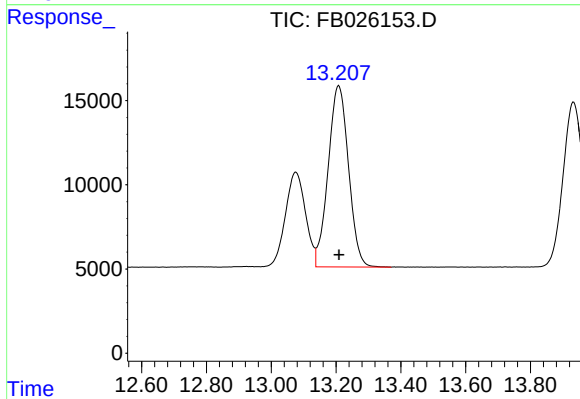

#8 m-Xylene


R.T.: 13.208 min
Delta R.T.: 0.000 min
Response: 470244
Conc: 20.12 ng/ml

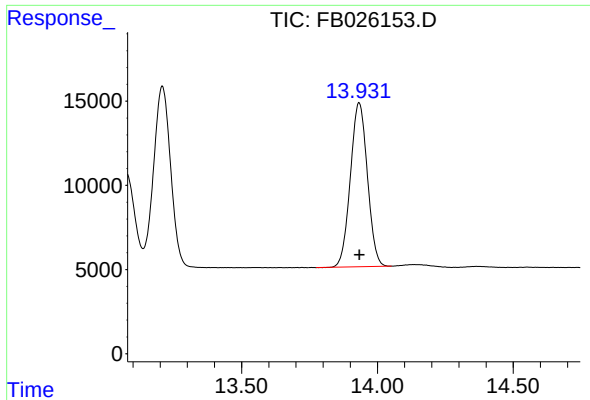

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 424470
Conc: 20.40 ng/ml

Instrument :
FID_B
ClientSampleId :

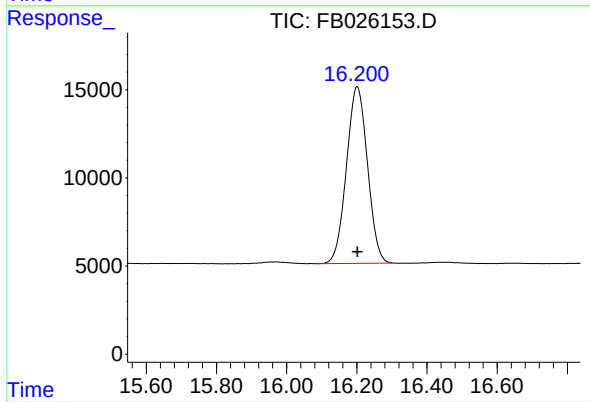

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.000 min
Response: 416641
Conc: 20.65 ng/ml