

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB081321\  
 Data File : FB026156.D  
 Signal(s) : FID2B.CH  
 Acq On : 13 Aug 2021 23:16  
 Operator : AJ/MA  
 Sample : BSF0813S1  
 Misc : 5.01G/5.00 ML DI WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Aug 14 03:20:08 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB081321.M  
 Quant Title :  
 QLast Update : Fri Aug 13 22:11:30 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
5) s AAA-TFT	8.853	290005	19.461 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	675156	29.906 ng/ml
2) t 2,2,4-Trimethylpentane	7.517	687673	31.281 ng/ml
3) t n-Heptane	7.830	281535	9.345 ng/ml
4) t Benzene	7.969	311816	9.868 ng/ml
6) t Toluene	10.662	852712	29.623 ng/ml
7) t Ethylbenzene	13.080	240906	9.979 ng/ml
8) t m-Xylene	13.211	462453	19.787 ng/ml
9) t O-Xylene	13.935	418165	20.099 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	390291	19.347 ng/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB081321\  
 Data File : FB026156.D  
 Signal(s) : FID2B.CH  
 Acq On : 13 Aug 2021 23:16  
 Operator : AJ/MA  
 Sample : BSF0813S1  
 Misc : 5.01G/5.00 ML DI WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampled :

Integration File: Calibration.e  
 Quant Time: Aug 14 03:20:08 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB081321.M  
 Quant Title :  
 QLast Update : Fri Aug 13 22:11:30 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

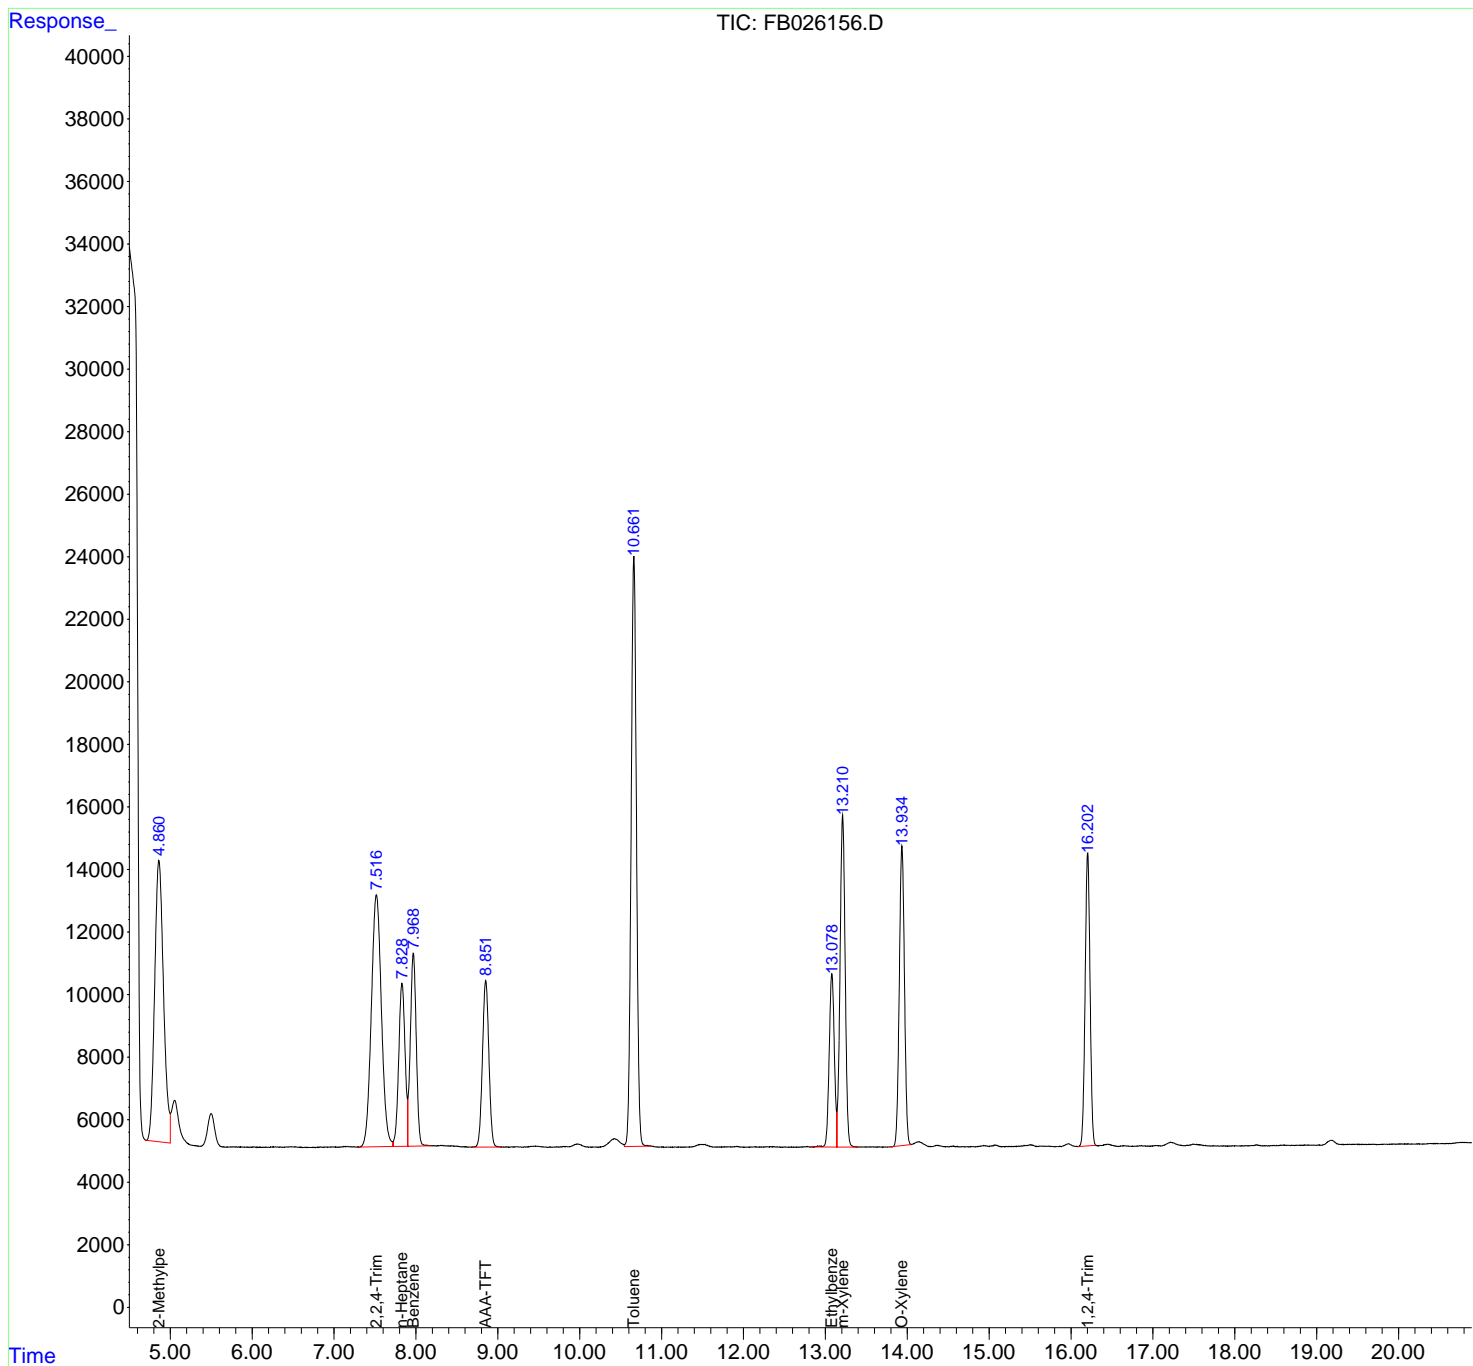

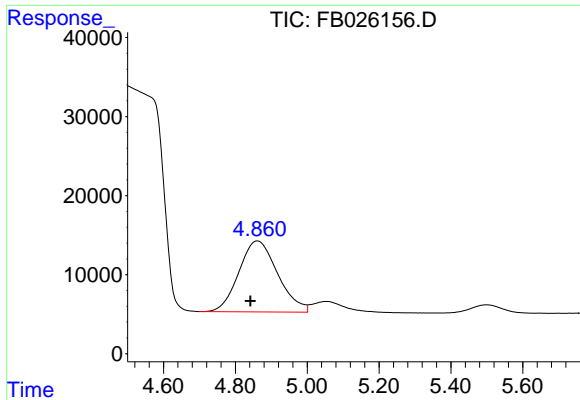


#1 2-Methylpentane  
 R.T.: 4.862 min  
 Delta R.T.: 0.020 min  
 Response: 675156  
 Conc: 29.91 ng/ml


Instrument :  
 FID\_B  
 ClientSampleId :

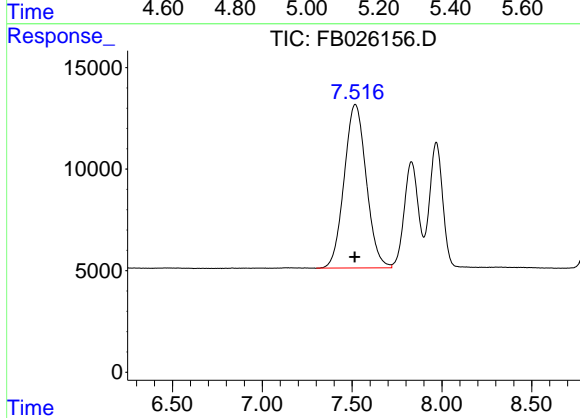


#2 2,2,4-Trimethylpentane  
 R.T.: 7.517 min  
 Delta R.T.: 0.002 min  
 Response: 687673  
 Conc: 31.28 ng/ml

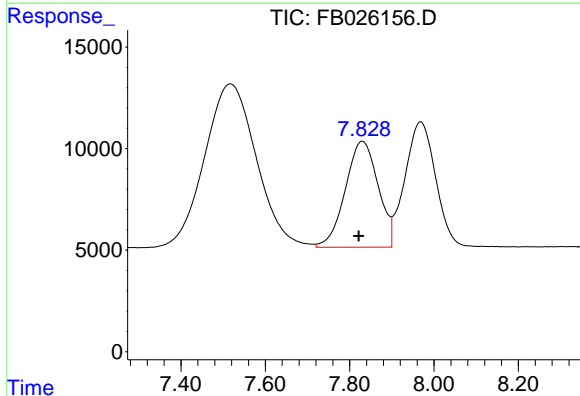

#3 n-Heptane  
 R.T.: 7.830 min  
 Delta R.T.: 0.009 min  
 Response: 281535  
 Conc: 9.35 ng/ml

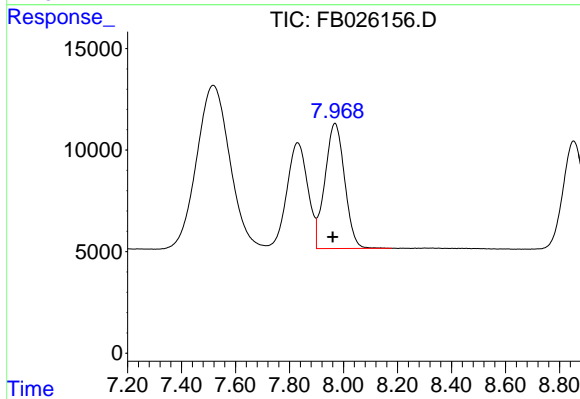


#4 Benzene  
 R.T.: 7.969 min  
 Delta R.T.: 0.009 min  
 Response: 311816  
 Conc: 9.87 ng/ml

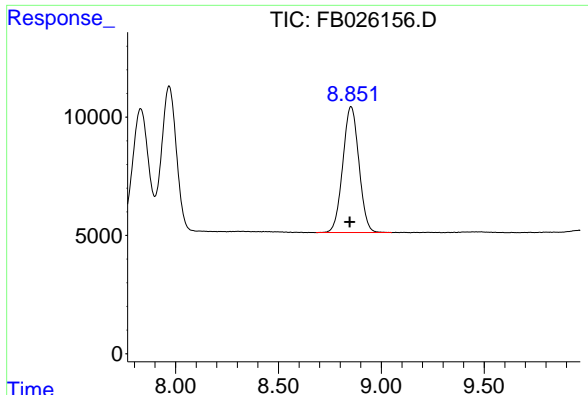


#5 AAA-TFT  
 R.T.: 8.853 min  
 Delta R.T.: 0.006 min  
 Response: 290005  
 Conc: 19.46 ng/ml


Instrument :  
 FID\_B  
 ClientSampled :

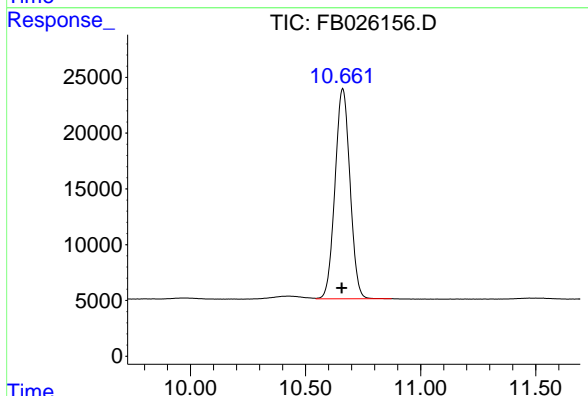


#6 Toluene  
 R.T.: 10.662 min  
 Delta R.T.: 0.004 min  
 Response: 852712  
 Conc: 29.62 ng/ml

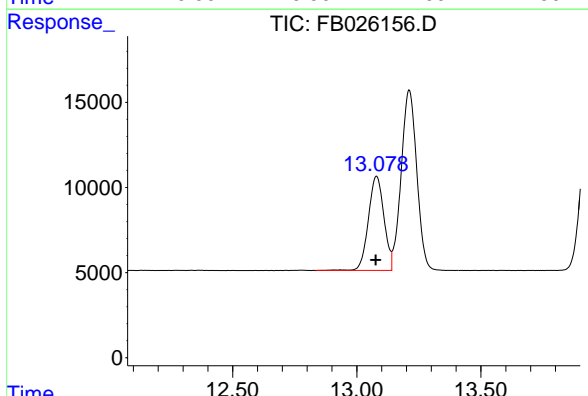

#7 Ethylbenzene  
 R.T.: 13.080 min  
 Delta R.T.: 0.003 min  
 Response: 240906  
 Conc: 9.98 ng/ml

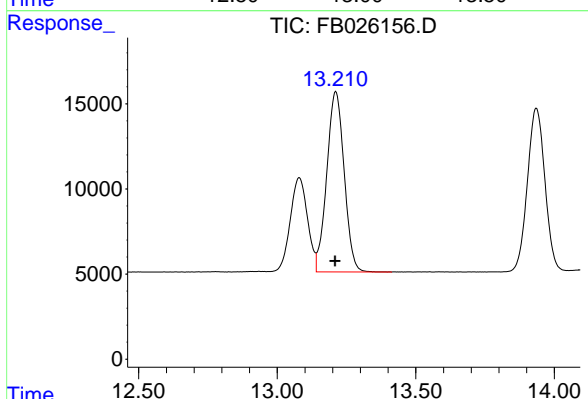


#8 m-Xylene  
 R.T.: 13.211 min  
 Delta R.T.: 0.002 min  
 Response: 462453  
 Conc: 19.79 ng/ml

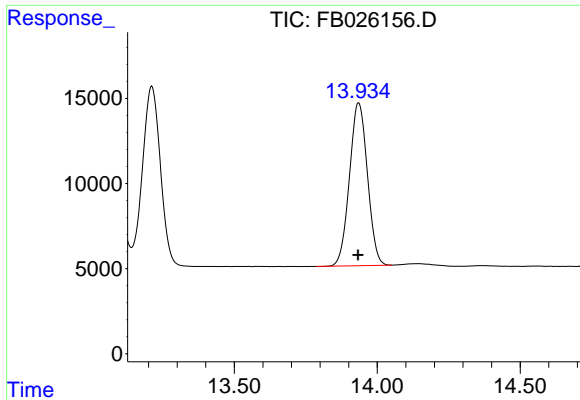

#9 O-Xylene

R.T.: 13.935 min  
Delta R.T.: 0.002 min  
Response: 418165  
Conc: 20.10 ng/ml

Instrument :  
FID\_B  
ClientSampled :

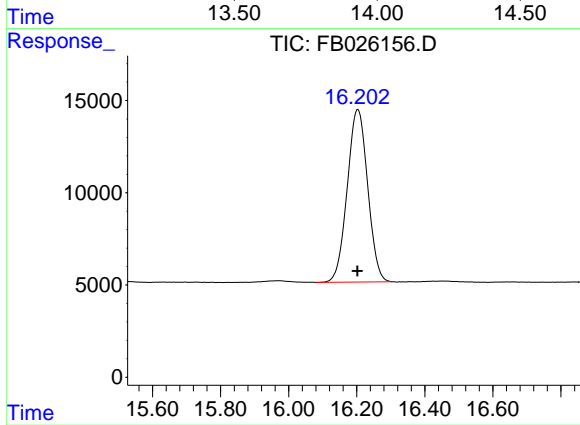

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min  
Delta R.T.: 0.002 min  
Response: 390291  
Conc: 19.35 ng/ml