

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
 Data File : FB026163.D
 Signal(s) : FID2B.CH
 Acq On : 14 Aug 2021 3:59
 Operator : AJ/MA
 Sample : M3408-14MS
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 14 05:39:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
 Quant Title :
 QLast Update : Fri Aug 13 22:11:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.844	305433	20.497 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.842	720499	31.914 ng/ml
2) t 2,2,4-Trimethylpentane	7.506	729095	33.165 ng/ml
3) t n-Heptane	7.819	285277	9.470 ng/ml
4) t Benzene	7.958	312918	9.903 ng/ml
6) t Toluene	10.655	856309	29.748 ng/ml
7) t Ethylbenzene	13.074	241039	9.984 ng/ml
8) t m-Xylene	13.207	464445	19.872 ng/ml
9) t O-Xylene	13.931	427765	20.560 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	411233	20.385 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
Data File : FB026163.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2021 3:59
Operator : AJ/MA
Sample : M3408-14MS
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 14 05:39:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:11:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

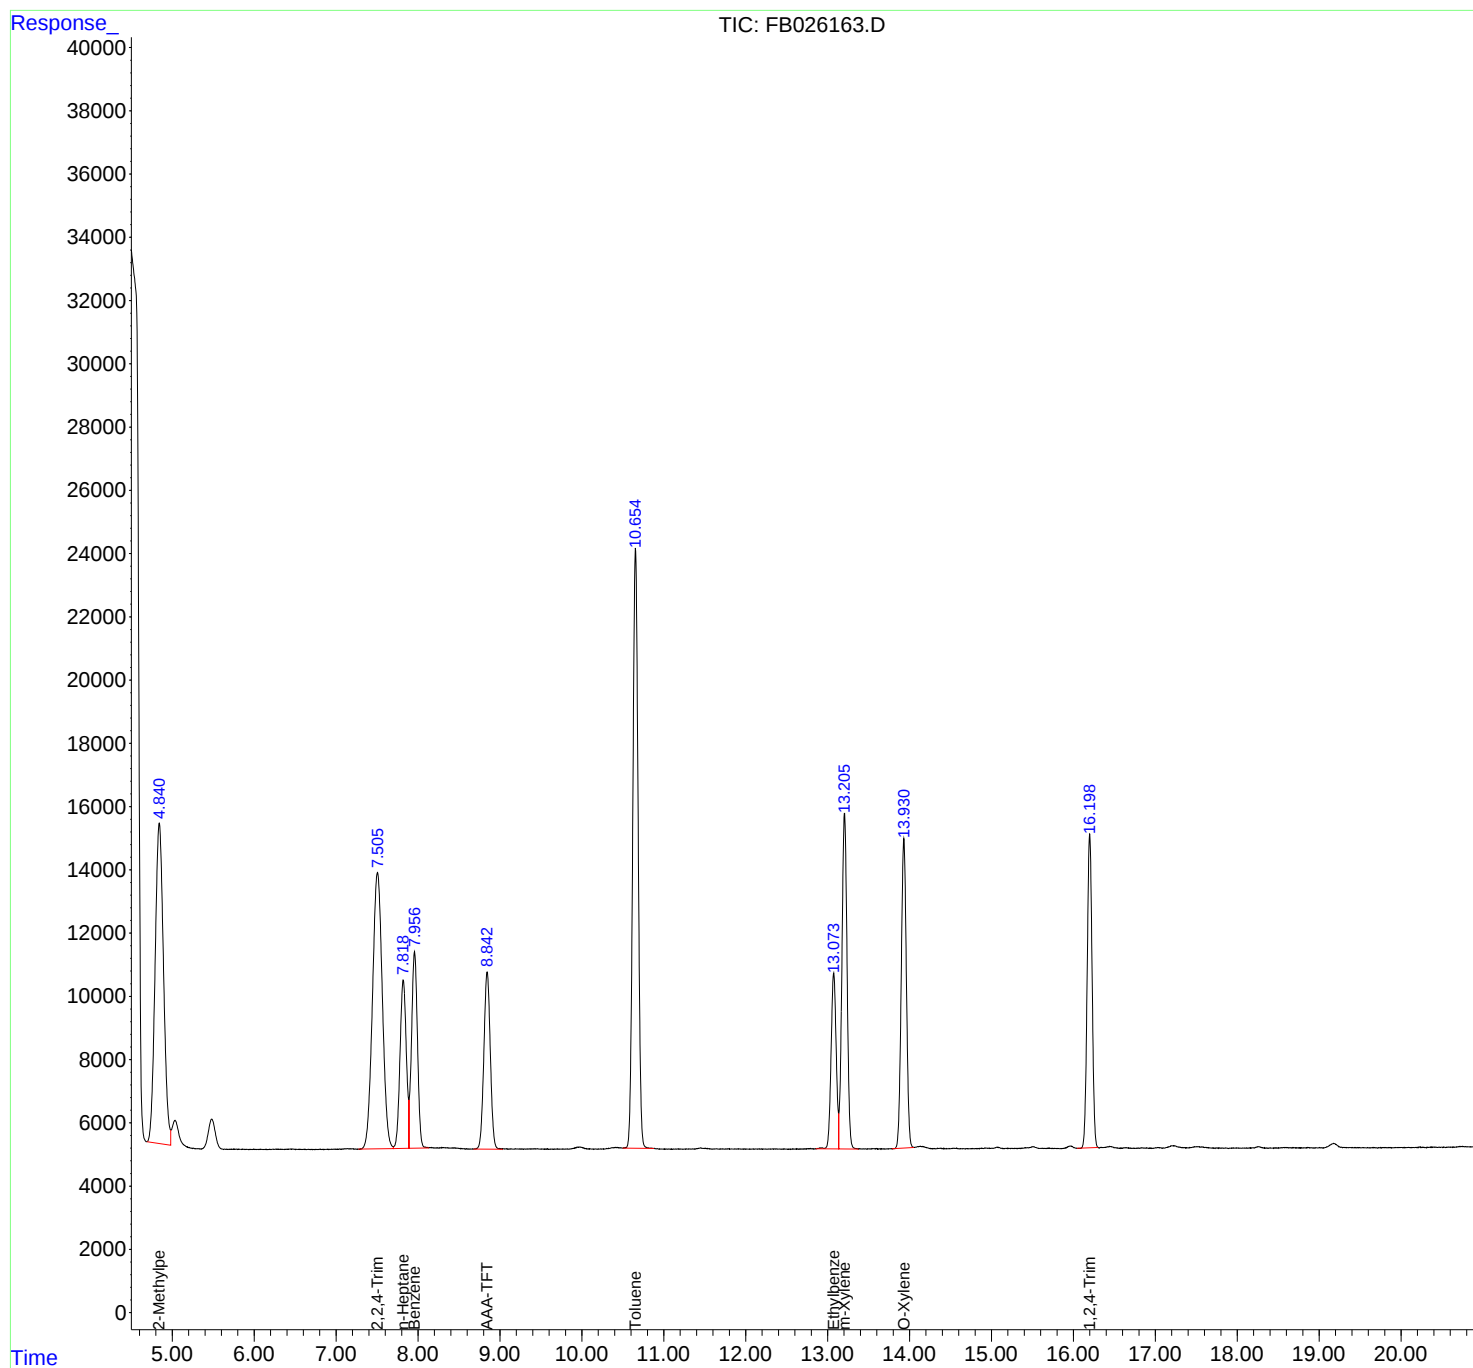


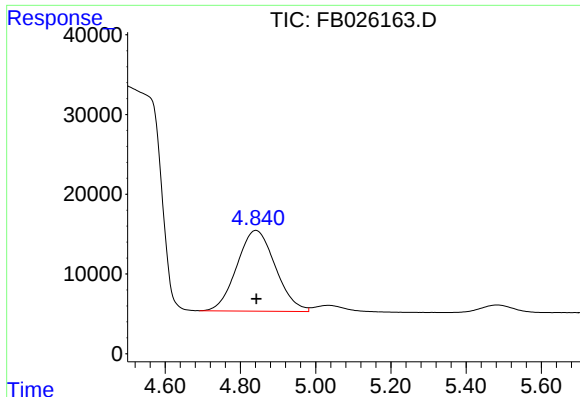

#1 2-Methylpentane


R.T.: 4.842 min
Delta R.T.: 0.000 min
Response: 720499
Conc: 31.91 ng/ml

Instrument :
FID_B
ClientSampleId :

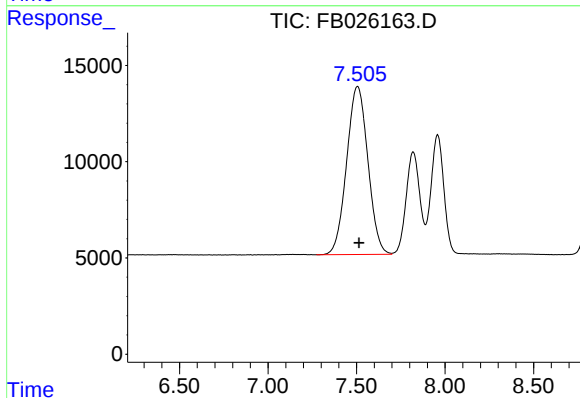


#2 2,2,4-Trimethylpentane

R.T.: 7.506 min
Delta R.T.: -0.009 min
Response: 729095
Conc: 33.16 ng/ml

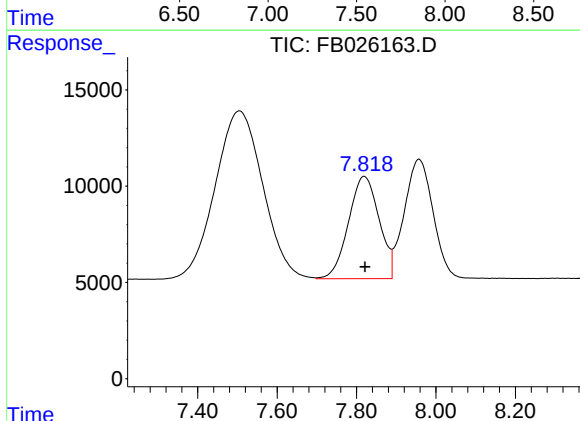


#3 n-Heptane

R.T.: 7.819 min
Delta R.T.: -0.002 min
Response: 285277
Conc: 9.47 ng/ml

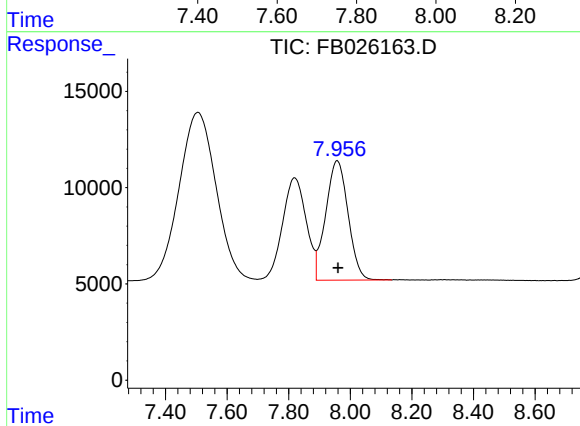

#4 Benzene


R.T.: 7.958 min
Delta R.T.: -0.002 min
Response: 312918
Conc: 9.90 ng/ml

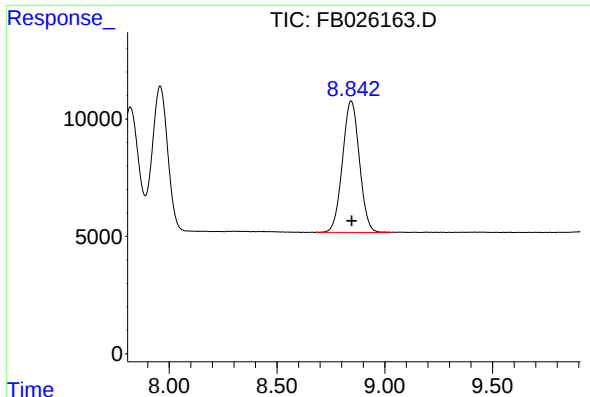

#5 AAA-TFT


R.T.: 8.844 min
Delta R.T.: -0.003 min
Response: 305433
Conc: 20.50 ng/ml

Instrument :
FID_B
ClientSampleId :

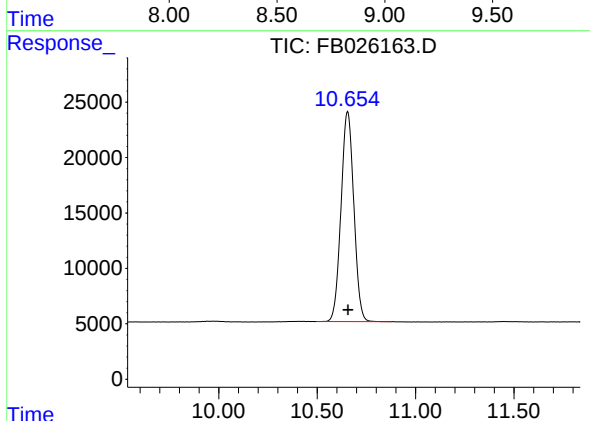


#6 Toluene

R.T.: 10.655 min
Delta R.T.: -0.003 min
Response: 856309
Conc: 29.75 ng/ml

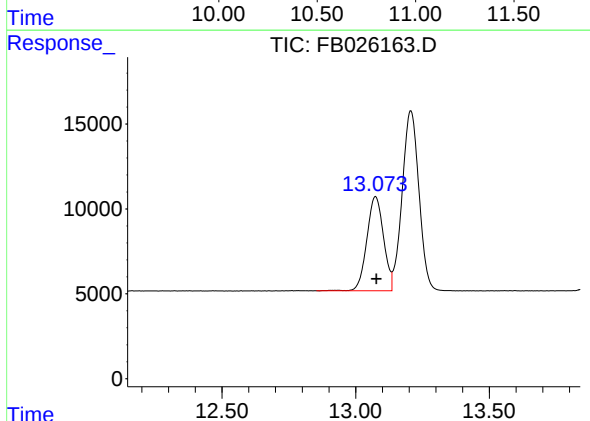


#7 Ethylbenzene

R.T.: 13.074 min
Delta R.T.: -0.002 min
Response: 241039
Conc: 9.98 ng/ml

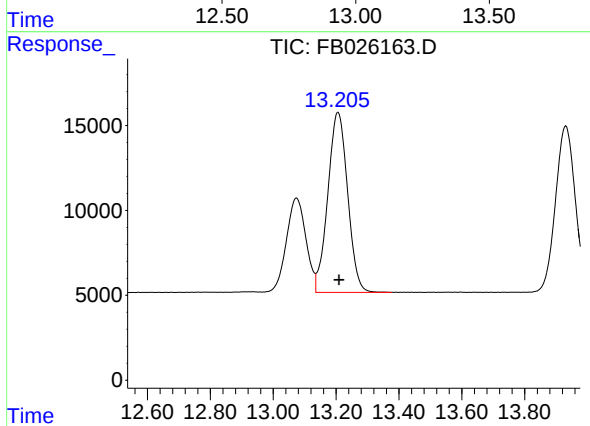

#8 m-Xylene


R.T.: 13.207 min
Delta R.T.: -0.003 min
Response: 464445
Conc: 19.87 ng/ml

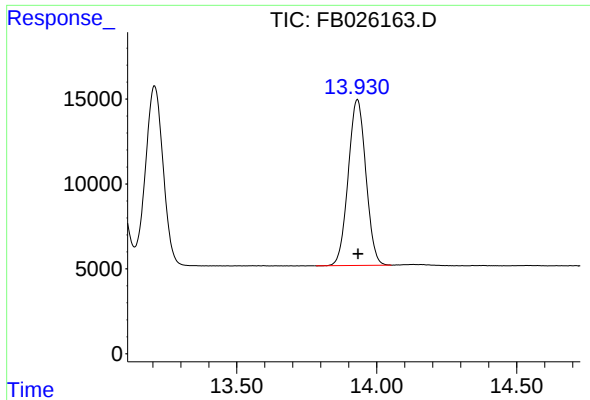

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.003 min
Response: 427765
Conc: 20.56 ng/ml

Instrument :
FID_B
ClientSampleId :

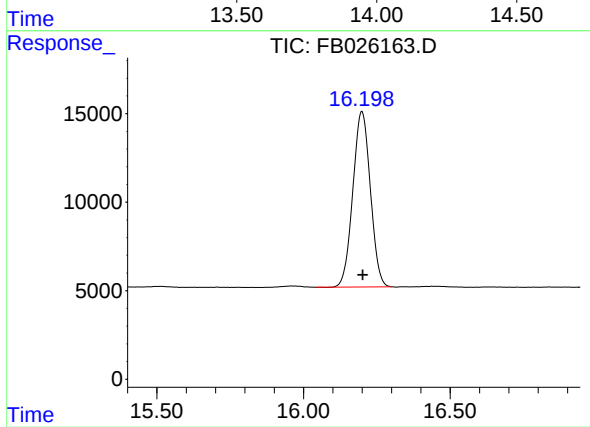

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: -0.003 min
Response: 411233
Conc: 20.38 ng/ml