

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
Data File : FB026174.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2021 11:55
Operator : AJ/MA
Sample : M3401-01
Misc : 5.01G/5.00ML DI WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 16 03:22:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:11:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.840	167291	11.226 ng/ml
Target Compounds			
4) t Benzene	7.957	9999	0.316 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
Data File : FB026174.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2021 11:55
Operator : AJ/MA
Sample : M3401-01
Misc : 5.01G/5.00ML DI WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 16 03:22:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:11:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

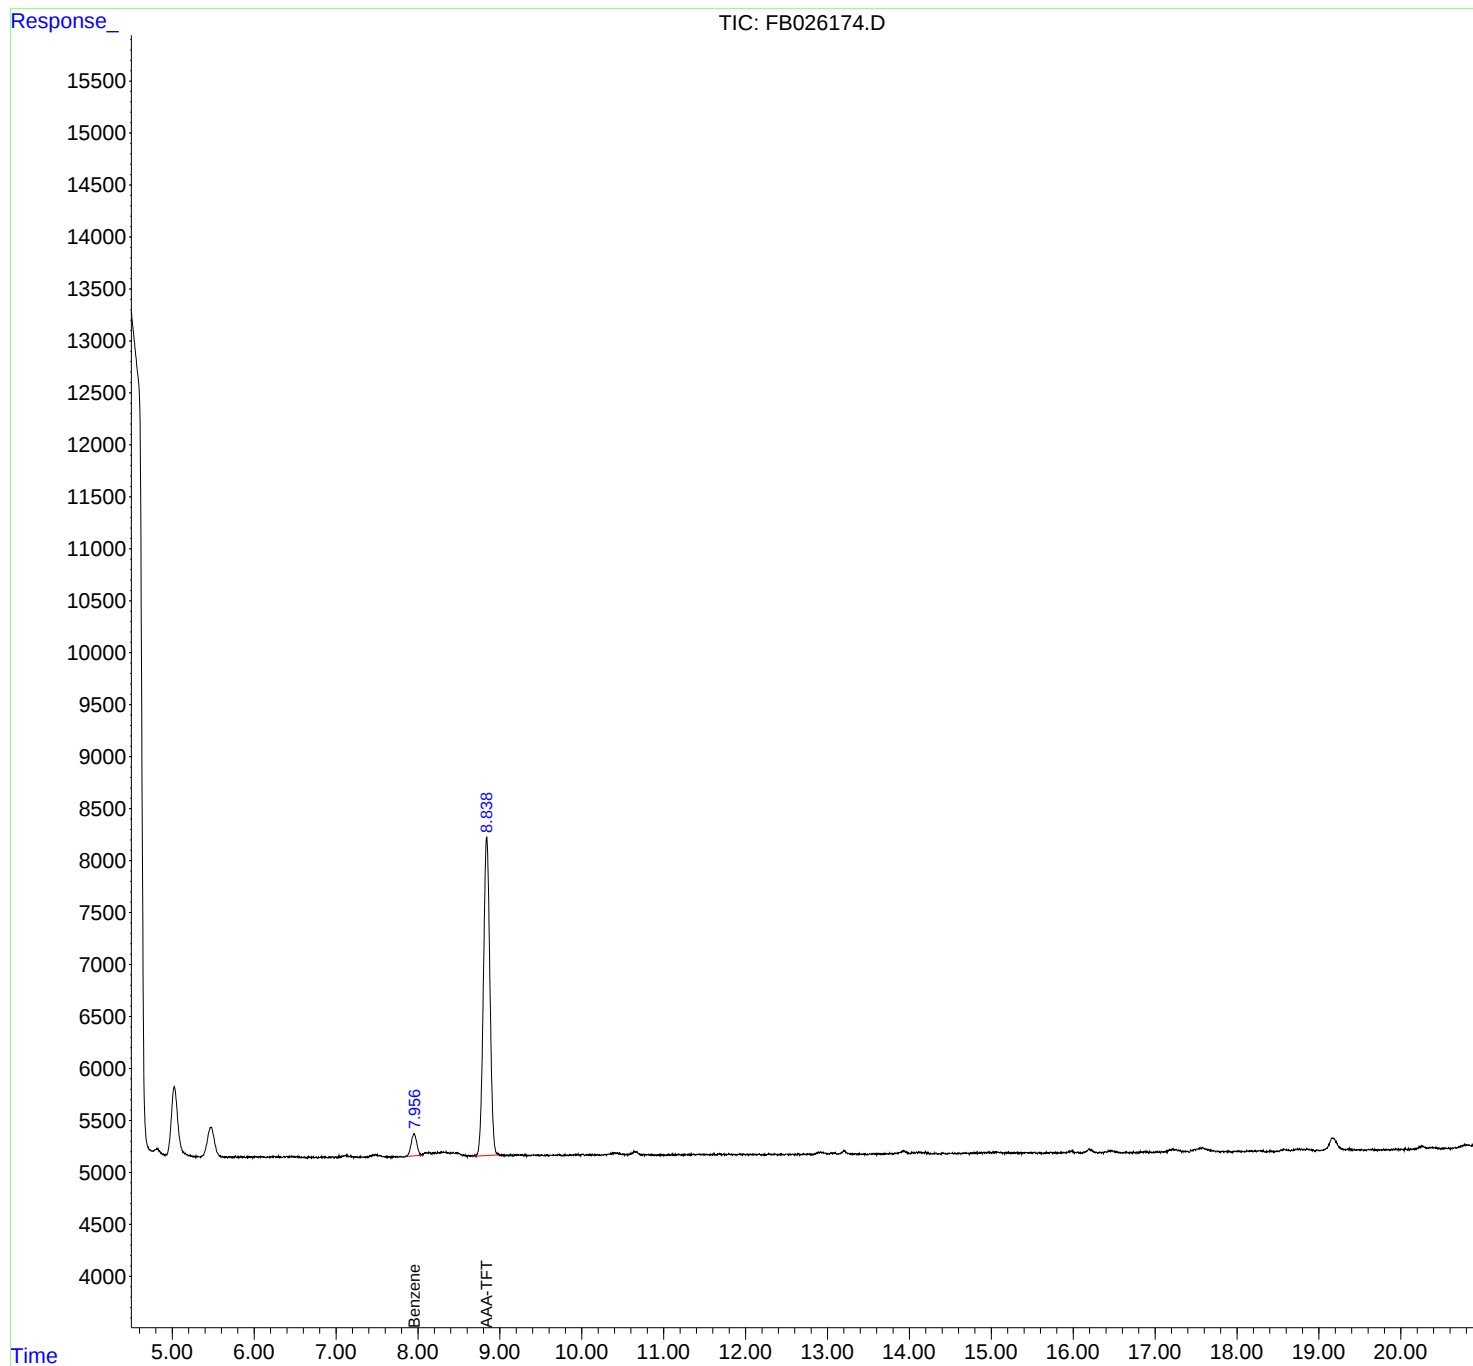


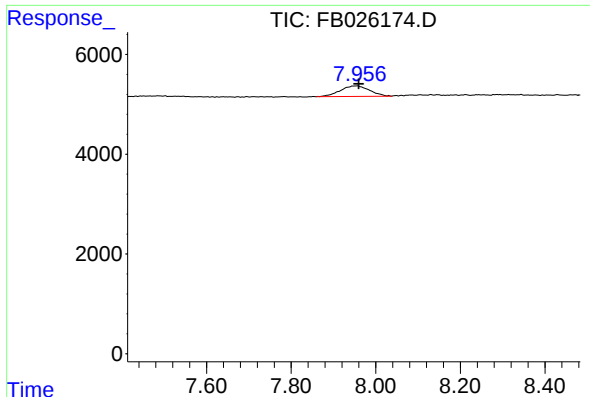

#4 Benzene

R.T.: 7.957 min
Delta R.T.: -0.003 min
Response: 9999
Conc: 0.32 ng/ml

Instrument :
FID_B
ClientSampleId :

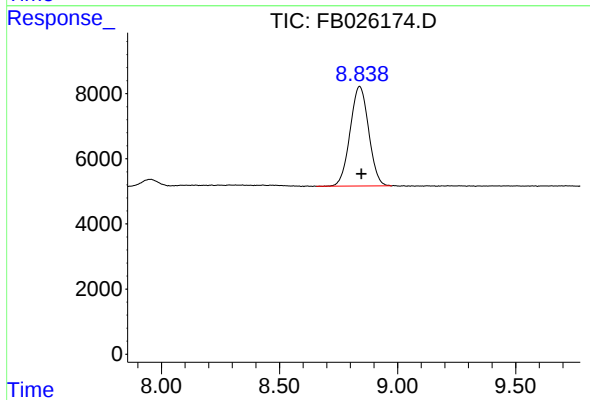

#5 AAA-TFT

R.T.: 8.840 min
Delta R.T.: -0.007 min
Response: 167291
Conc: 11.23 ng/ml