

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
 Data File : FB026164.D
 Signal(s) : FID2B.CH
 Acq On : 14 Aug 2021 4:40
 Operator : AJ/MA
 Sample : M3408-14MSD
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 34NMSD

Integration File: SAMPLE.e
 Quant Time: Aug 14 05:39:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
 Quant Title :
 QLast Update : Fri Aug 13 22:11:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.845	291370	19.553 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.847	702878	31.134 ng/ml
2) t 2,2,4-Trimethylpentane	7.507	713384	32.450 ng/ml
3) t n-Heptane	7.822	276287	9.171 ng/ml
4) t Benzene	7.960	312239	9.882 ng/ml
6) t Toluene	10.656	862352	29.958 ng/ml
7) t Ethylbenzene	13.075	245054	10.151 ng/ml
8) t m-Xylene	13.207	473094	20.242 ng/ml
9) t O-Xylene	13.931	440200	21.158 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	432869	21.457 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081321\
Data File : FB026164.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2021 4:40
Operator : AJ/MA
Sample : M3408-14MSD
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
34NMSD

Integration File: SAMPLE.e
Quant Time: Aug 14 05:39:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:11:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

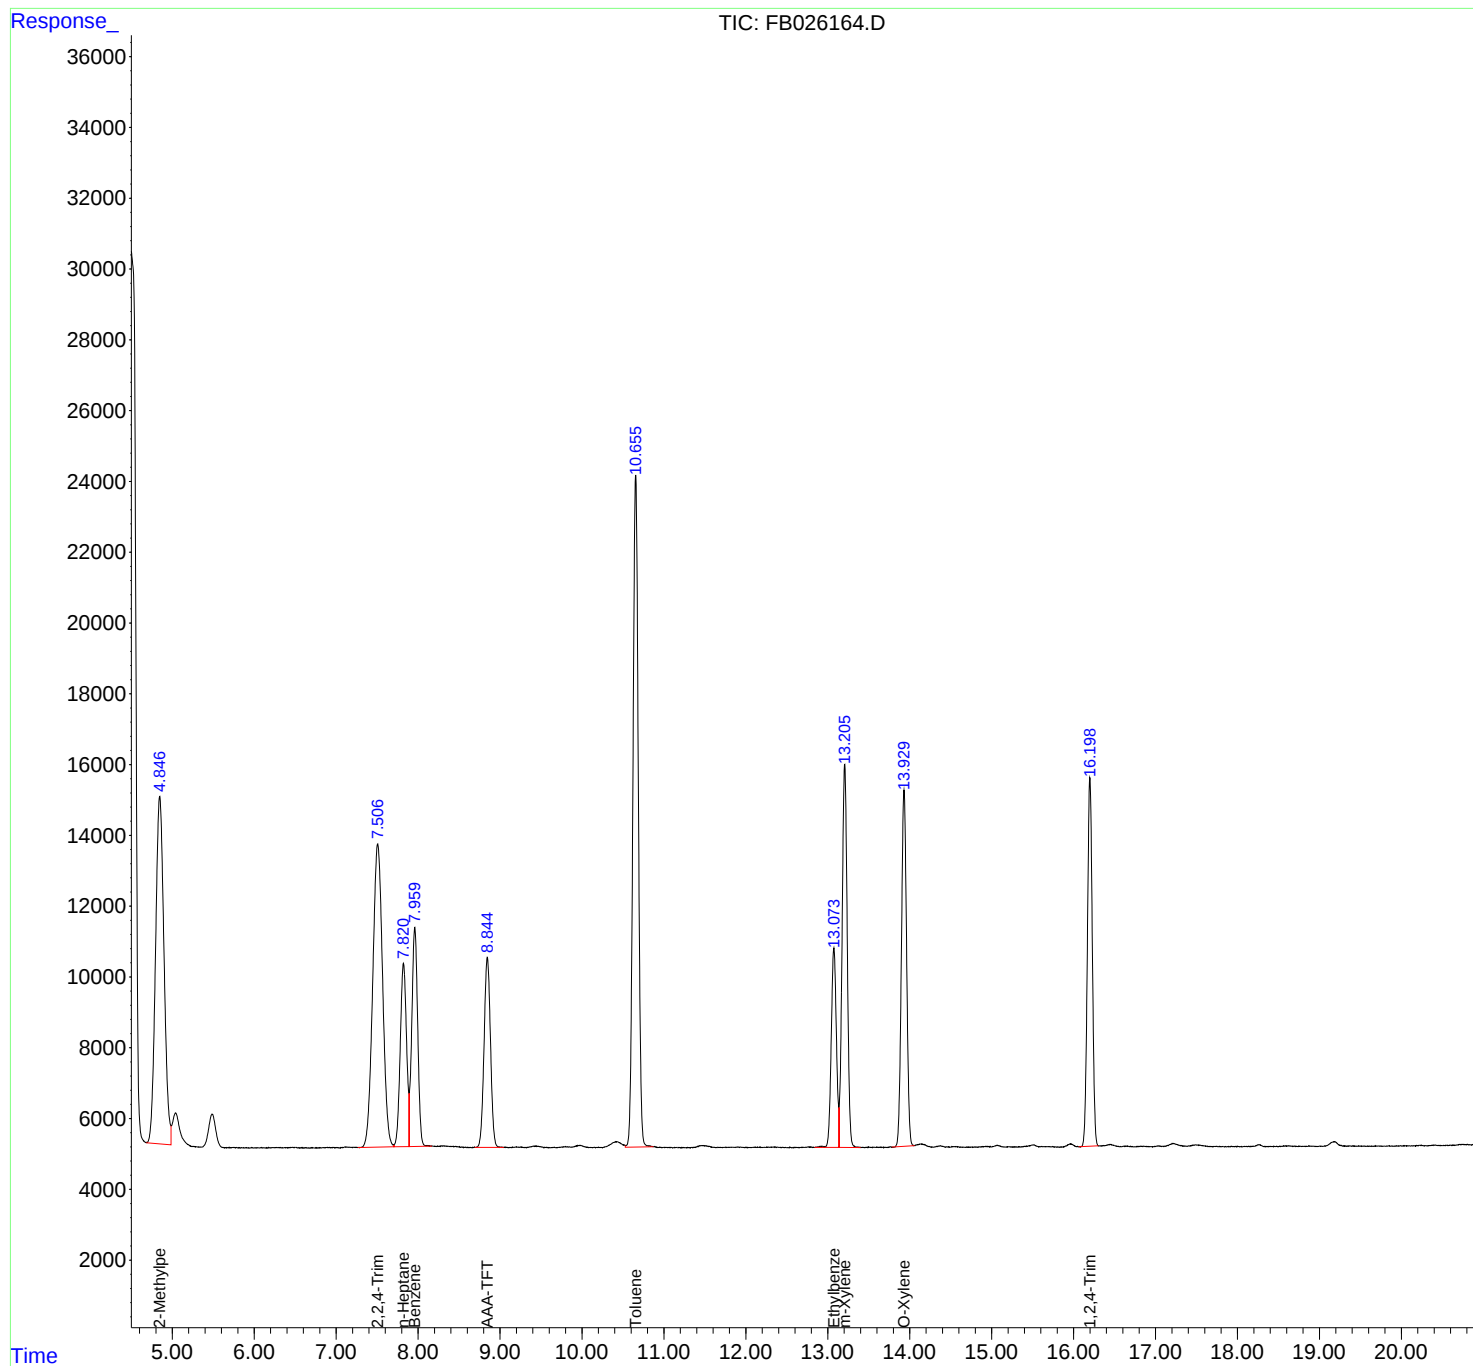


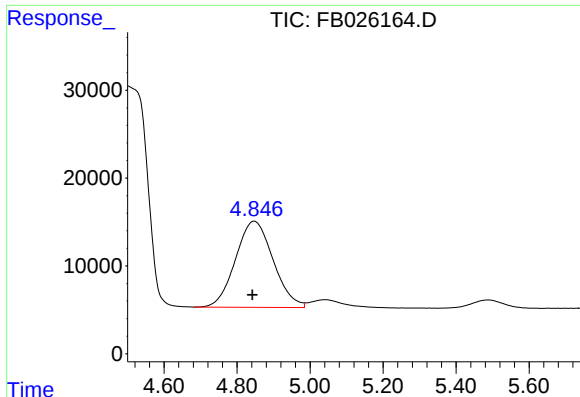

#1 2-Methylpentane


R.T.: 4.847 min
Delta R.T.: 0.005 min
Response: 702878
Conc: 31.13 ng/ml

Instrument :
FID_B
ClientSampleId :
34NMSD

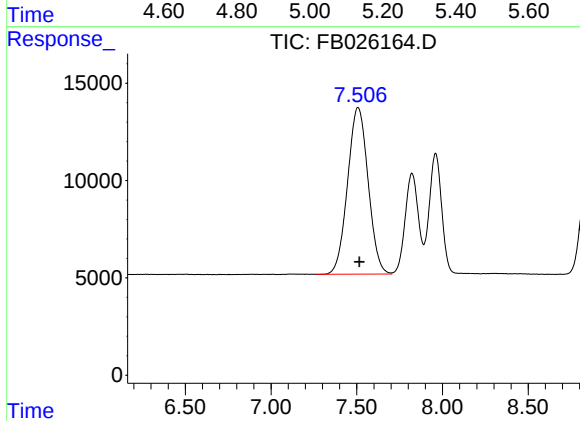


#2 2,2,4-Trimethylpentane

R.T.: 7.507 min
Delta R.T.: -0.008 min
Response: 713384
Conc: 32.45 ng/ml

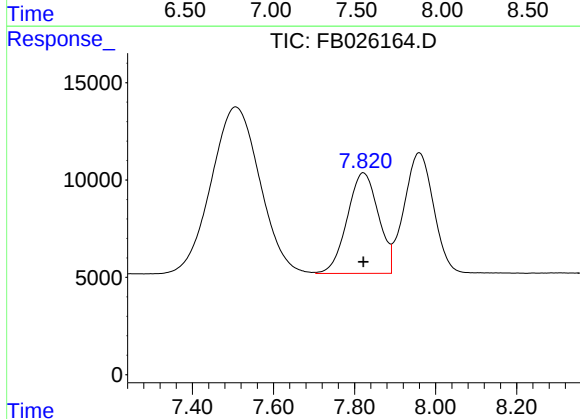


#3 n-Heptane

R.T.: 7.822 min
Delta R.T.: 0.000 min
Response: 276287
Conc: 9.17 ng/ml

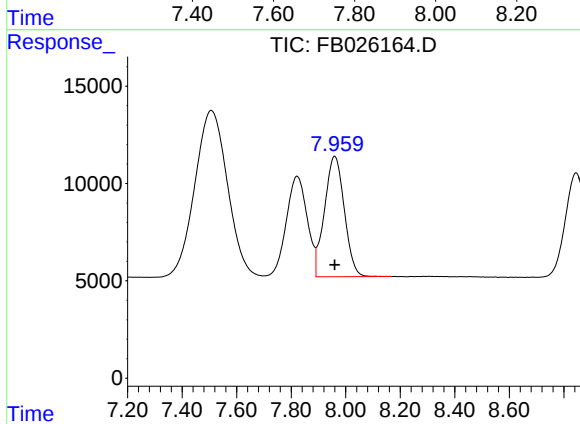

#4 Benzene


R.T.: 7.960 min
Delta R.T.: 0.000 min
Response: 312239
Conc: 9.88 ng/ml

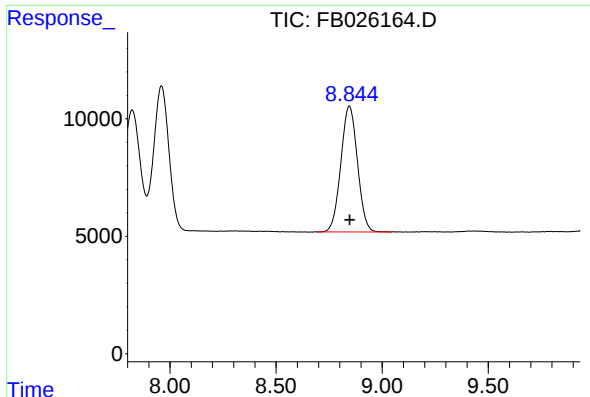

#5 AAA-TFT


R.T.: 8.845 min
Delta R.T.: -0.001 min
Response: 291370
Conc: 19.55 ng/ml

Instrument :
FID_B
ClientSampleId :
34NMSD

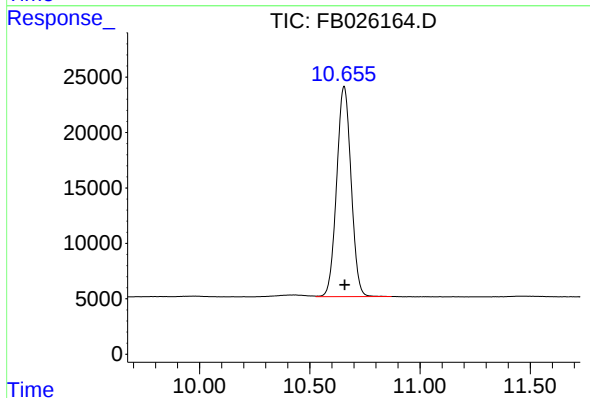


#6 Toluene

R.T.: 10.656 min
Delta R.T.: -0.002 min
Response: 862352
Conc: 29.96 ng/ml

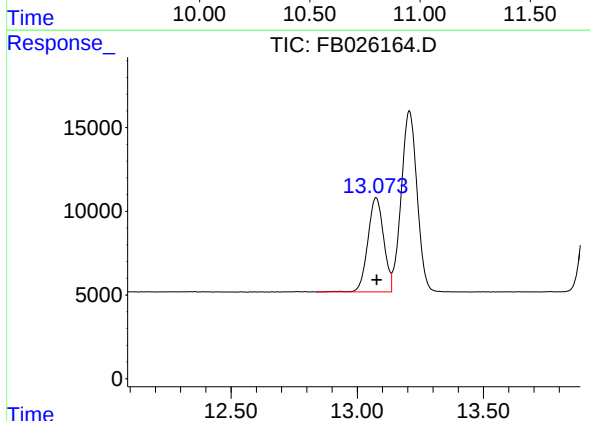


#7 Ethylbenzene

R.T.: 13.075 min
Delta R.T.: -0.002 min
Response: 245054
Conc: 10.15 ng/ml

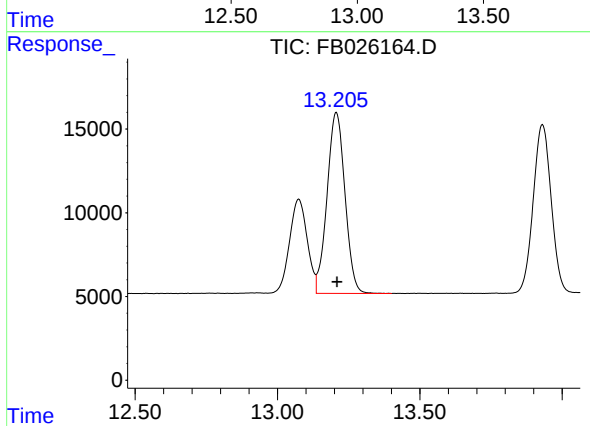

#8 m-Xylene


R.T.: 13.207 min
Delta R.T.: -0.003 min
Response: 473094
Conc: 20.24 ng/ml

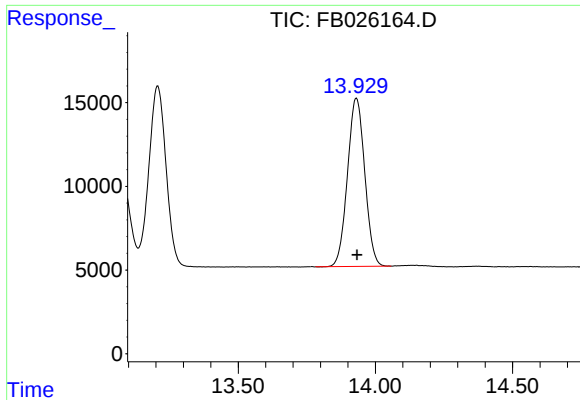

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.003 min
Response: 440200
Conc: 21.16 ng/ml

Instrument :
FID_B
ClientSampleId :
34NMSD

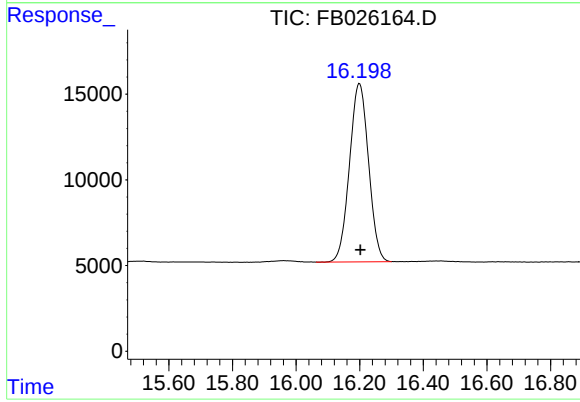

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: -0.003 min
Response: 432869
Conc: 21.46 ng/ml