

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081419\
 Data File : FB022013.D
 Signal(s) : FID2B.CH
 Acq On : 14 Aug 2019 16:55
 Operator : DD/AJ
 Sample : K4340-03MSD
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 15 08:07:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.993	298206	21.852 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	738620	26.785 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	603057	22.813 ng/ml
3) t n-Heptane	7.951	181913	7.337 ng/ml
4) t Benzene	8.087	287588	9.844 ng/ml
6) t Toluene	10.834	582631	28.316 ng/ml
7) t Ethylbenzene	13.280	188433	9.057 ng/ml
8) t m-Xylene	13.412	396071	17.829 ng/ml
9) t O-Xylene	14.142	414683	18.028 ng/ml
10) t 1,2,4-Trimethylbenzene	16.422	411251	17.443 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081419\
Data File : FB022013.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2019 16:55
Operator : DD/AJ
Sample : K4340-03MSD
Misc : 5.05/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 15 08:07:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

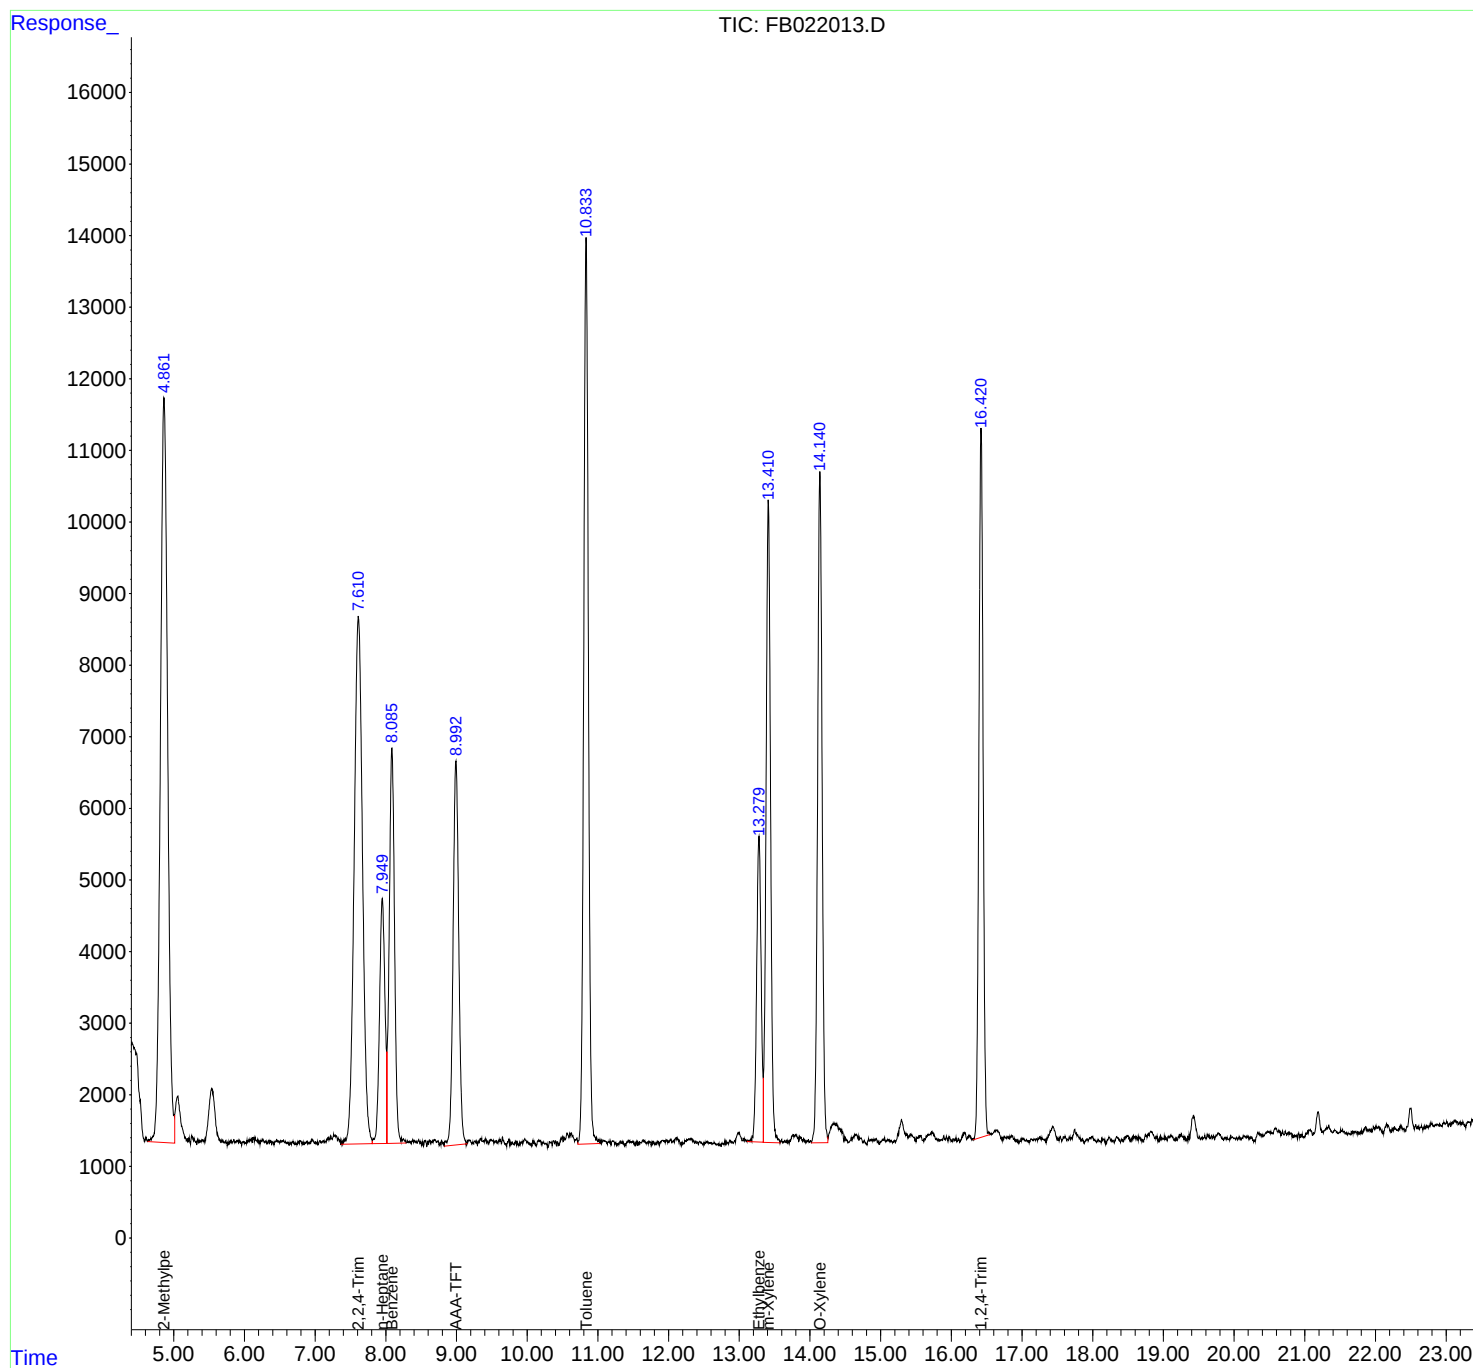

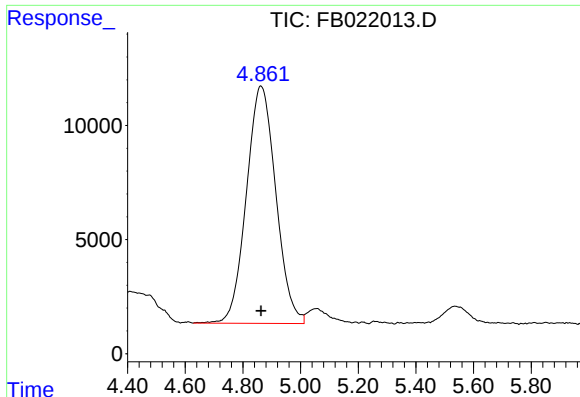


#1 2-Methylpentane

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 738620
Conc: 26.78 ng/ml

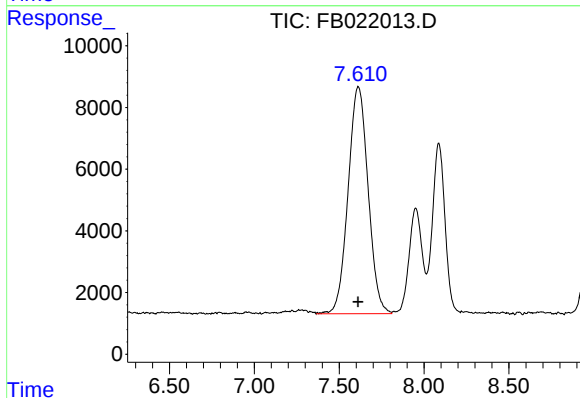


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 603057
Conc: 22.81 ng/ml

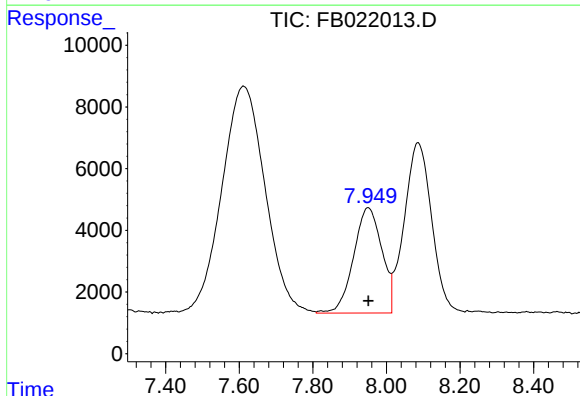


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 181913
Conc: 7.34 ng/ml

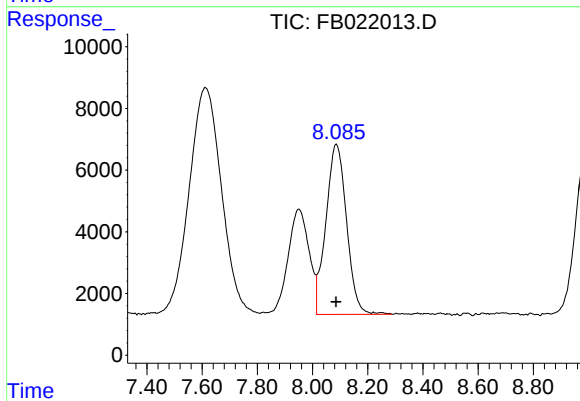


#4 Benzene

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 287588
Conc: 9.84 ng/ml

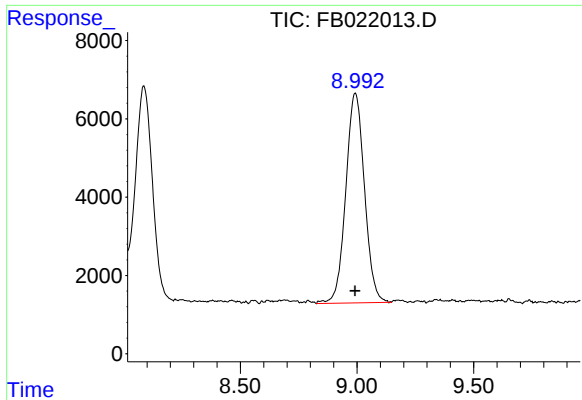


#5 AAA-TFT

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 298206
Conc: 21.85 ng/ml

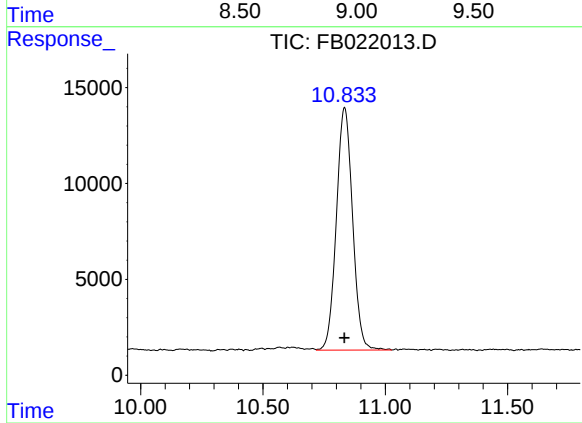


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.000 min
Response: 582631
Conc: 28.32 ng/ml

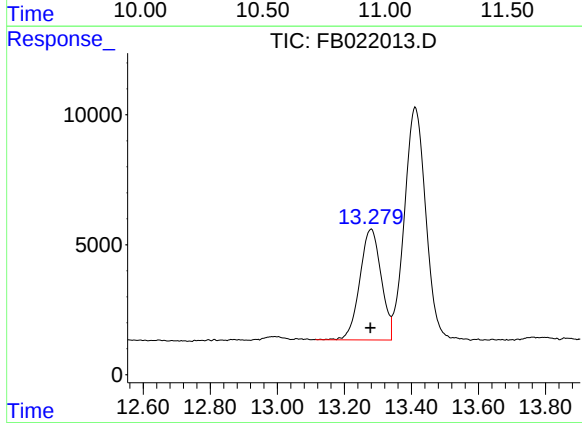


#7 Ethylbenzene

R.T.: 13.280 min
Delta R.T.: 0.002 min
Response: 188433
Conc: 9.06 ng/ml

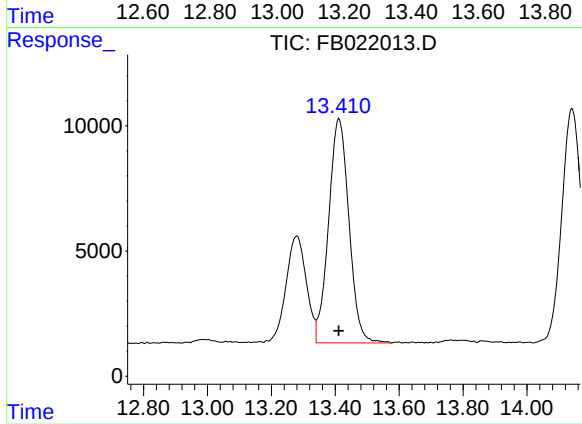


#8 m-Xylene

R.T.: 13.412 min
Delta R.T.: 0.001 min
Response: 396071
Conc: 17.83 ng/ml

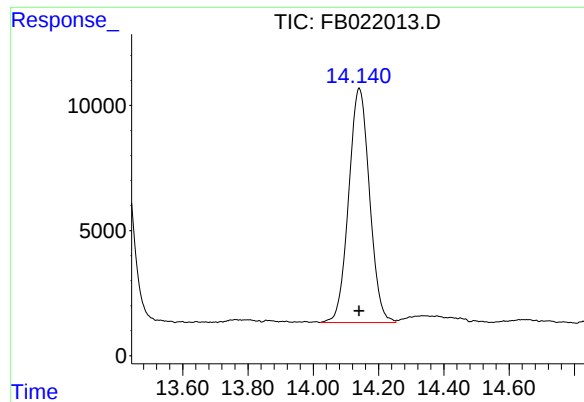

#9 O-Xylene

R.T.: 14.142 min
Delta R.T.: 0.001 min
Response: 414683
Conc: 18.03 ng/ml

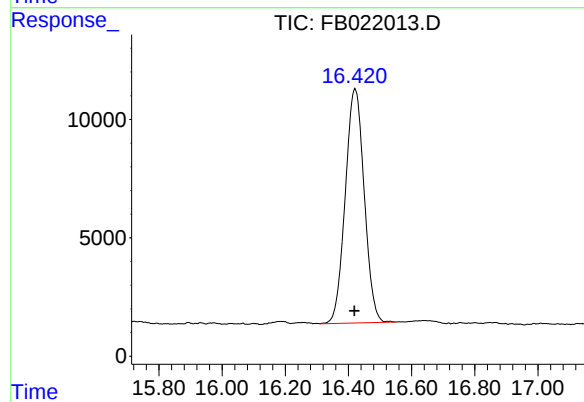

#10 1,2,4-Trimethylbenzene

R.T.: 16.422 min
Delta R.T.: 0.002 min
Response: 411251
Conc: 17.44 ng/ml