

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081419\
 Data File : FB022012.D
 Signal(s) : FID2B.CH
 Acq On : 14 Aug 2019 16:24
 Operator : DD/AJ
 Sample : K4340-03MS
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 15 08:07:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
 Quant Title :
 QLast Update : Mon Jul 15 13:30:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	290599	21.295 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	760299	27.571 ng/ml
2) t 2,2,4-Trimethylpentane	7.613	677412	25.626 ng/ml
3) t n-Heptane	7.953	208441	8.407 ng/ml
4) t Benzene	8.088	293495	10.046 ng/ml
6) t Toluene	10.834	606787	29.490 ng/ml
7) t Ethylbenzene	13.279	210894	10.137 ng/ml
8) t m-Xylene	13.412	431571	19.427 ng/ml
9) t O-Xylene	14.141	449718	19.551 ng/ml
10) t 1,2,4-Trimethylbenzene	16.421	451330	19.143 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081419\
Data File : FB022012.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2019 16:24
Operator : DD/AJ
Sample : K4340-03MS
Misc : 5.03/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 15 08:07:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB071519.M
Quant Title :
QLast Update : Mon Jul 15 13:30:07 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

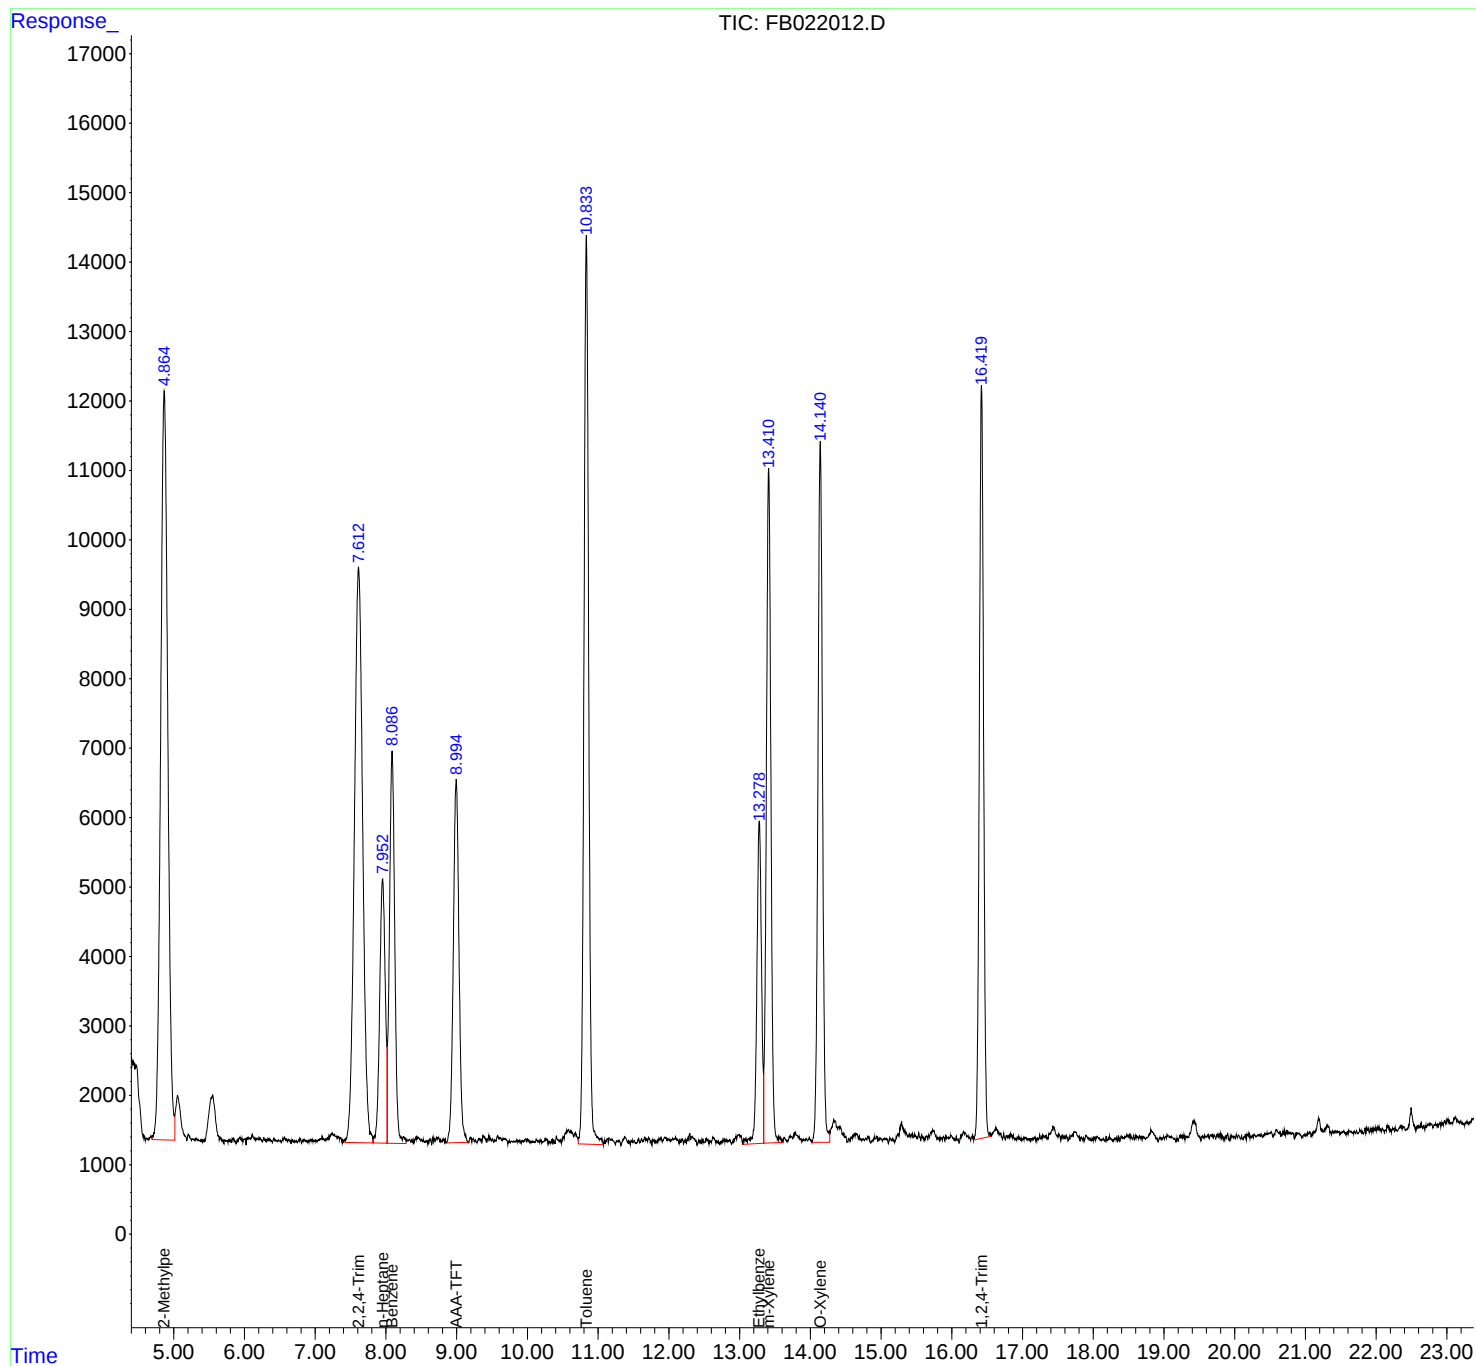

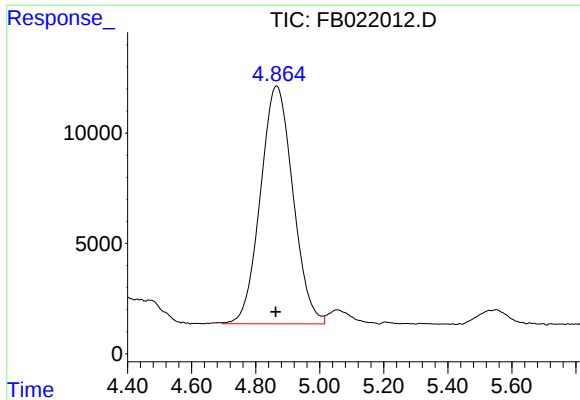


#1 2-Methylpentane

R.T.: 4.866 min
Delta R.T.: 0.003 min
Response: 760299
Conc: 27.57 ng/ml

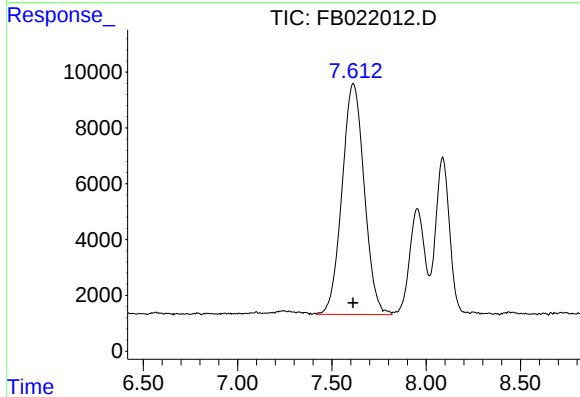


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 677412
Conc: 25.63 ng/ml

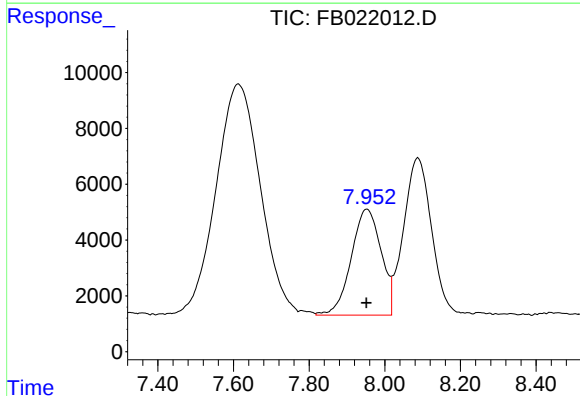


#3 n-Heptane

R.T.: 7.953 min
Delta R.T.: 0.002 min
Response: 208441
Conc: 8.41 ng/ml

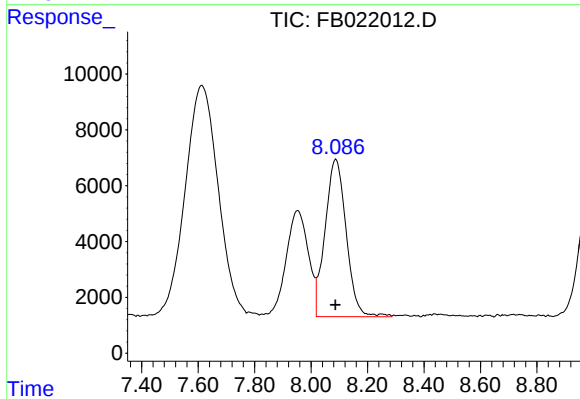


#4 Benzene

R.T.: 8.088 min
Delta R.T.: 0.002 min
Response: 293495
Conc: 10.05 ng/ml

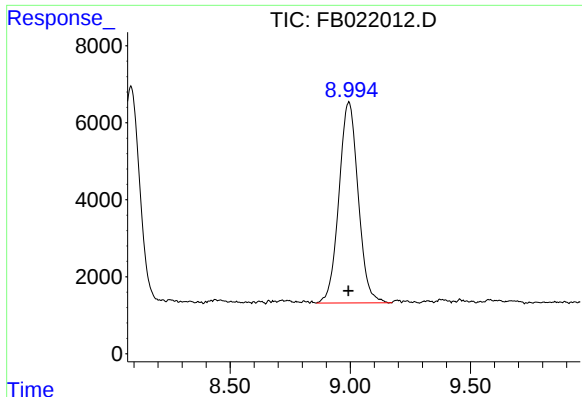


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 290599
Conc: 21.29 ng/ml

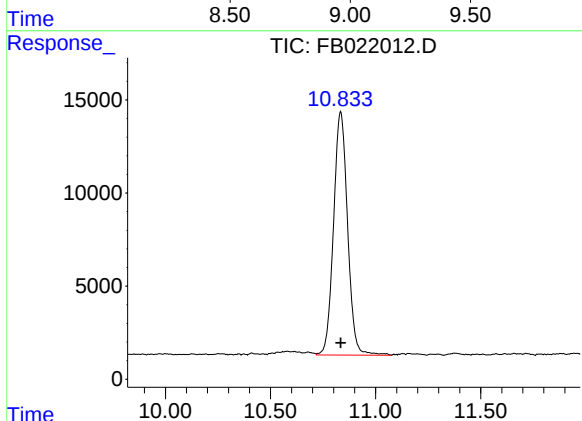


#6 Toluene

R.T.: 10.834 min
Delta R.T.: 0.000 min
Response: 606787
Conc: 29.49 ng/ml

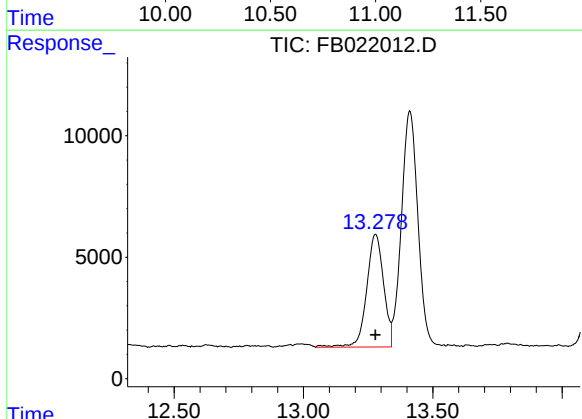


#7 Ethylbenzene

R.T.: 13.279 min
Delta R.T.: 0.001 min
Response: 210894
Conc: 10.14 ng/ml

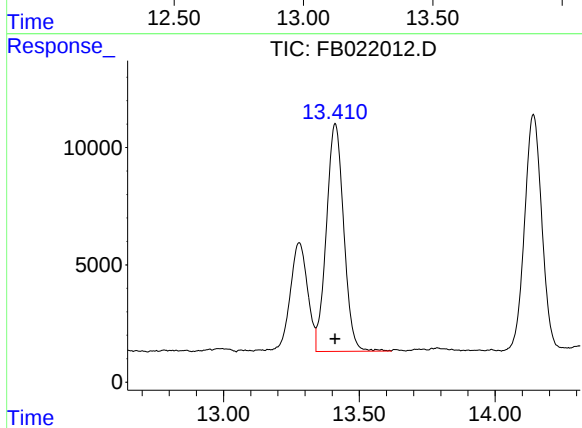


#8 m-Xylene

R.T.: 13.412 min
Delta R.T.: 0.000 min
Response: 431571
Conc: 19.43 ng/ml

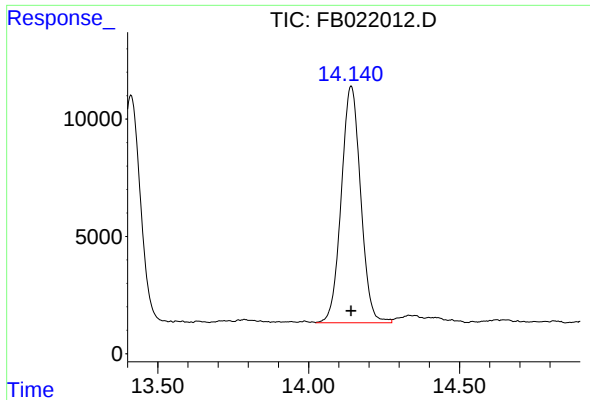

#9 O-Xylene

R.T.: 14.141 min
Delta R.T.: 0.000 min
Response: 449718
Conc: 19.55 ng/ml

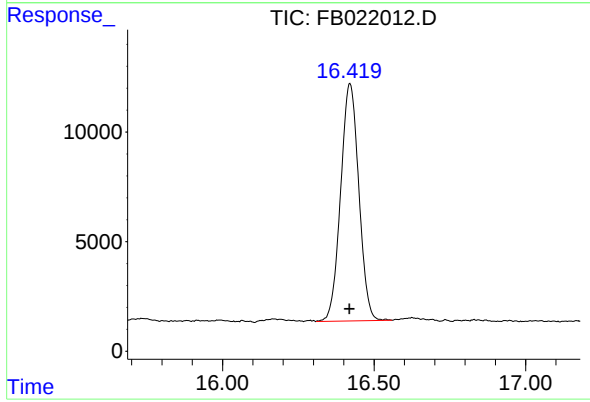

#10 1,2,4-Trimethylbenzene

R.T.: 16.421 min
Delta R.T.: 0.002 min
Response: 451330
Conc: 19.14 ng/ml