

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081423\
 Data File : FB030241.D
 Signal(s) : FID2B.CH
 Acq On : 14 Aug 2023 9:06
 Operator : YP/AJ
 Sample : 20 PPB GRO CCC
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO CCC

Integration File: Calibration.e
 Quant Time: Aug 15 02:28:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	272121	22.140 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	432252	26.166 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	505952	27.266 ng/ml
3) t n-Heptane	7.742	156376	8.128 ng/ml
4) t Benzene	7.879	221743	9.426 ng/ml
6) t Toluene	10.612	645822	28.181 ng/ml
7) t Ethylbenzene	13.047	209076	9.741 ng/ml
8) t m-Xylene	13.180	403677	19.195 ng/ml
9) t O-Xylene	13.907	404303	19.700 ng/ml
10) t 1,2,4-Trimethylbenzene	16.182	418951	21.404 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081423\
Data File : FB030241.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2023 9:06
Operator : YP/AJ
Sample : 20 PPB GRO CCC
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO CCC

Integration File: Calibration.e
Quant Time: Aug 15 02:28:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

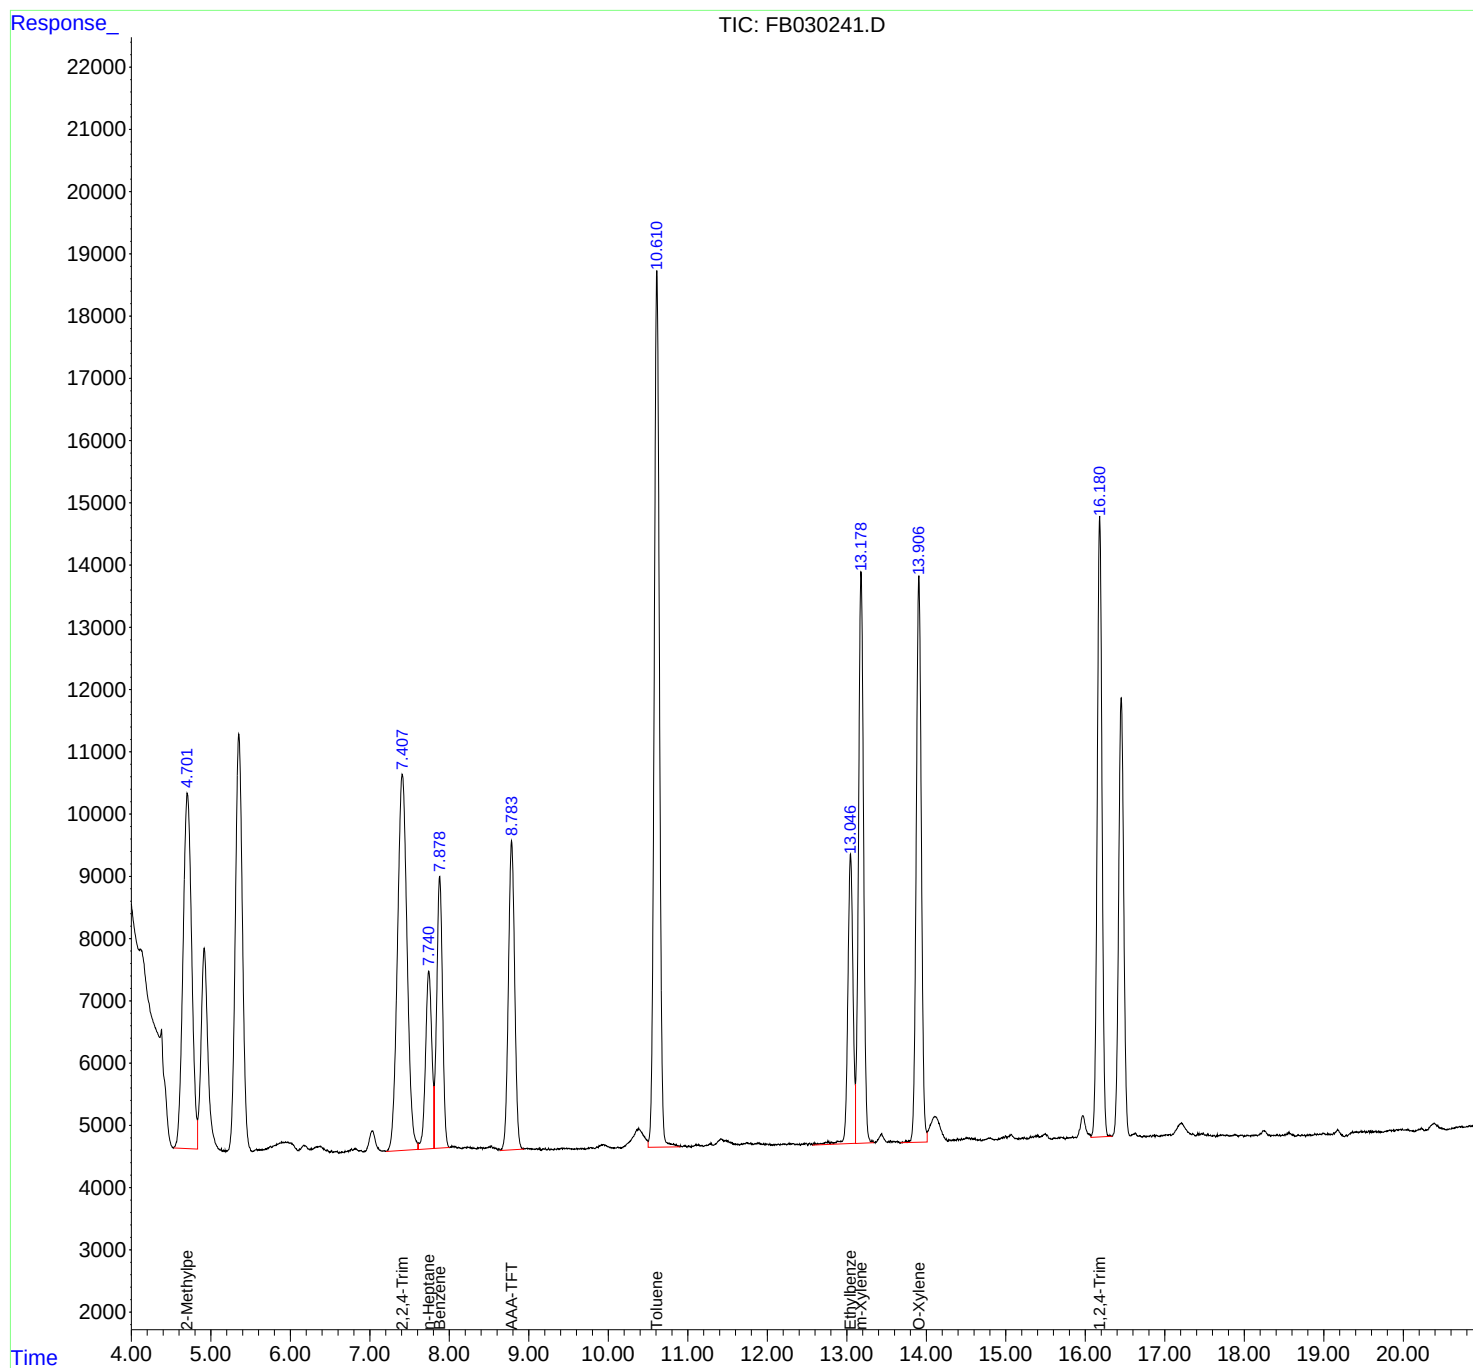


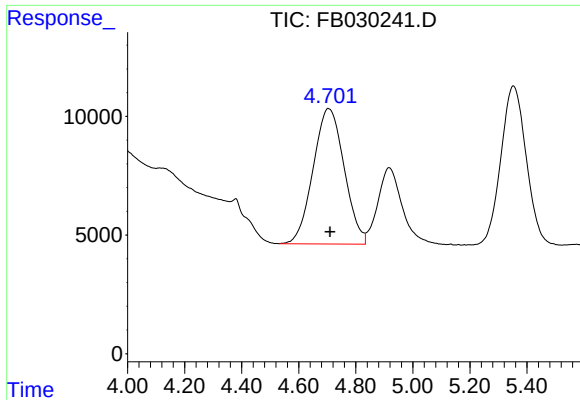

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.007 min
Response: 432252
Conc: 26.17 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO CCC

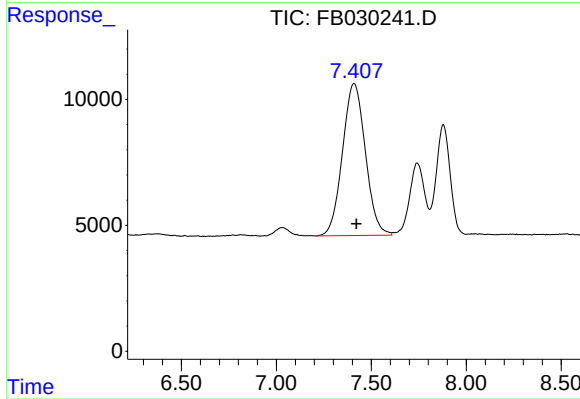


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.012 min
Response: 505952
Conc: 27.27 ng/ml

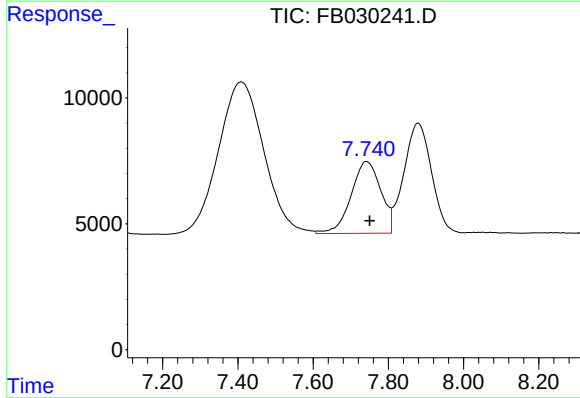


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: -0.008 min
Response: 156376
Conc: 8.13 ng/ml

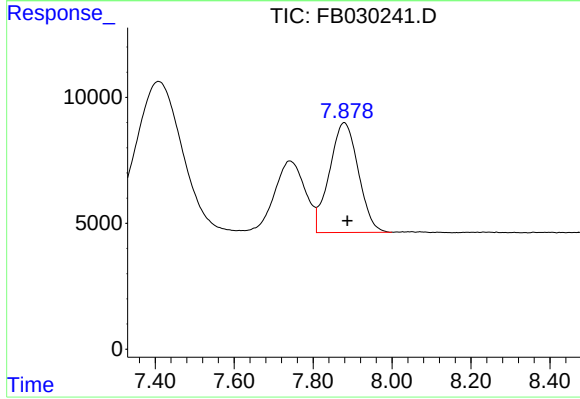

#4 Benzene


R.T.: 7.879 min
Delta R.T.: -0.008 min
Response: 221743
Conc: 9.43 ng/ml

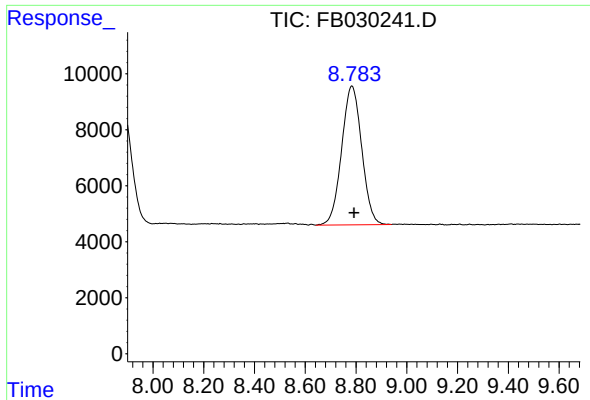

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: -0.009 min
Response: 272121
Conc: 22.14 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO CCC

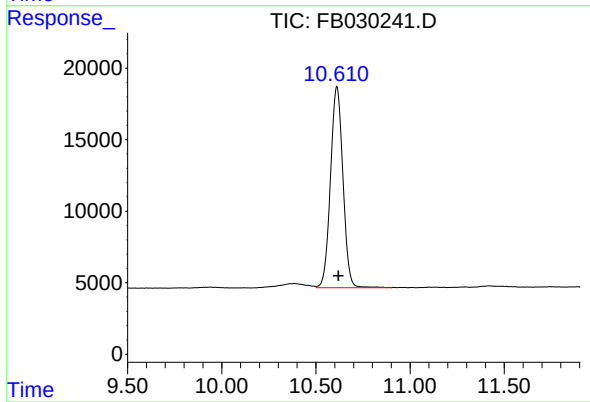


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.009 min
Response: 645822
Conc: 28.18 ng/ml

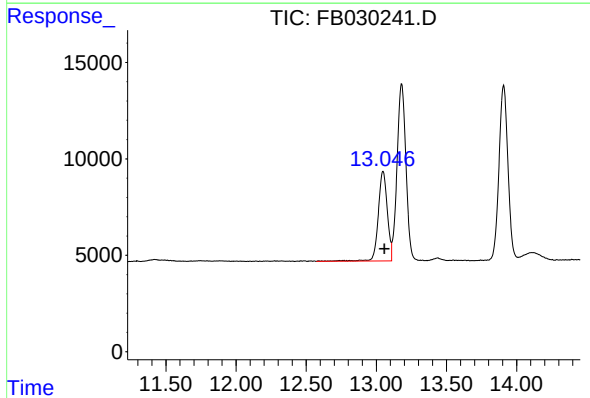


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.009 min
Response: 209076
Conc: 9.74 ng/ml

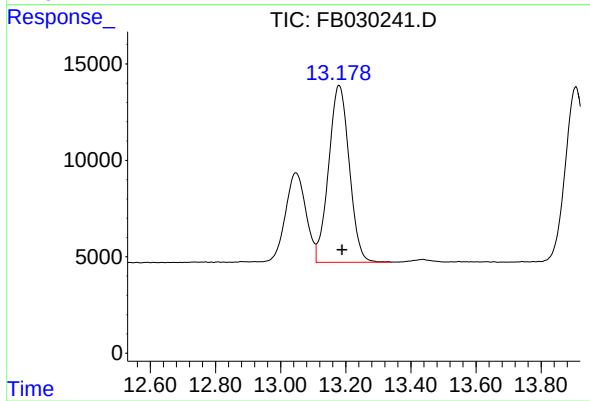

#8 m-Xylene


R.T.: 13.180 min
Delta R.T.: -0.009 min
Response: 403677
Conc: 19.20 ng/ml

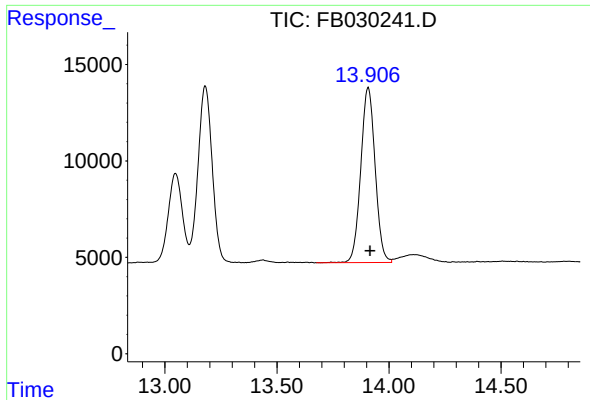

#9 O-Xylene

R.T.: 13.907 min
Delta R.T.: -0.009 min
Response: 404303
Conc: 19.70 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO CCC

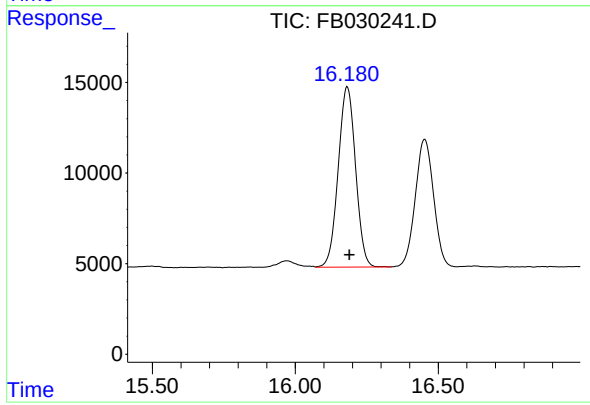

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: -0.008 min
Response: 418951
Conc: 21.40 ng/ml