

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081423\
 Data File : FB030244.D
 Signal(s) : FID2B.CH
 Acq On : 14 Aug 2023 11:12
 Operator : YP/AJ
 Sample : BSF0814S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0814S1

Integration File: Calibration.e
 Quant Time: Aug 15 02:28:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	238672	19.418 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	403564	24.429 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	512777	27.633 ng/ml
3) t n-Heptane	7.748	149621	7.777 ng/ml
4) t Benzene	7.885	210546	8.950 ng/ml
6) t Toluene	10.618	621193	27.106 ng/ml
7) t Ethylbenzene	13.054	196907	9.174 ng/ml
8) t m-Xylene	13.186	389513	18.522 ng/ml
9) t O-Xylene	13.913	383313	18.677 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	380183	19.423 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081423\
Data File : FB030244.D
Signal(s) : FID2B.CH
Acq On : 14 Aug 2023 11:12
Operator : YP/AJ
Sample : BSF0814S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0814S1

Integration File: Calibration.e
Quant Time: Aug 15 02:28:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

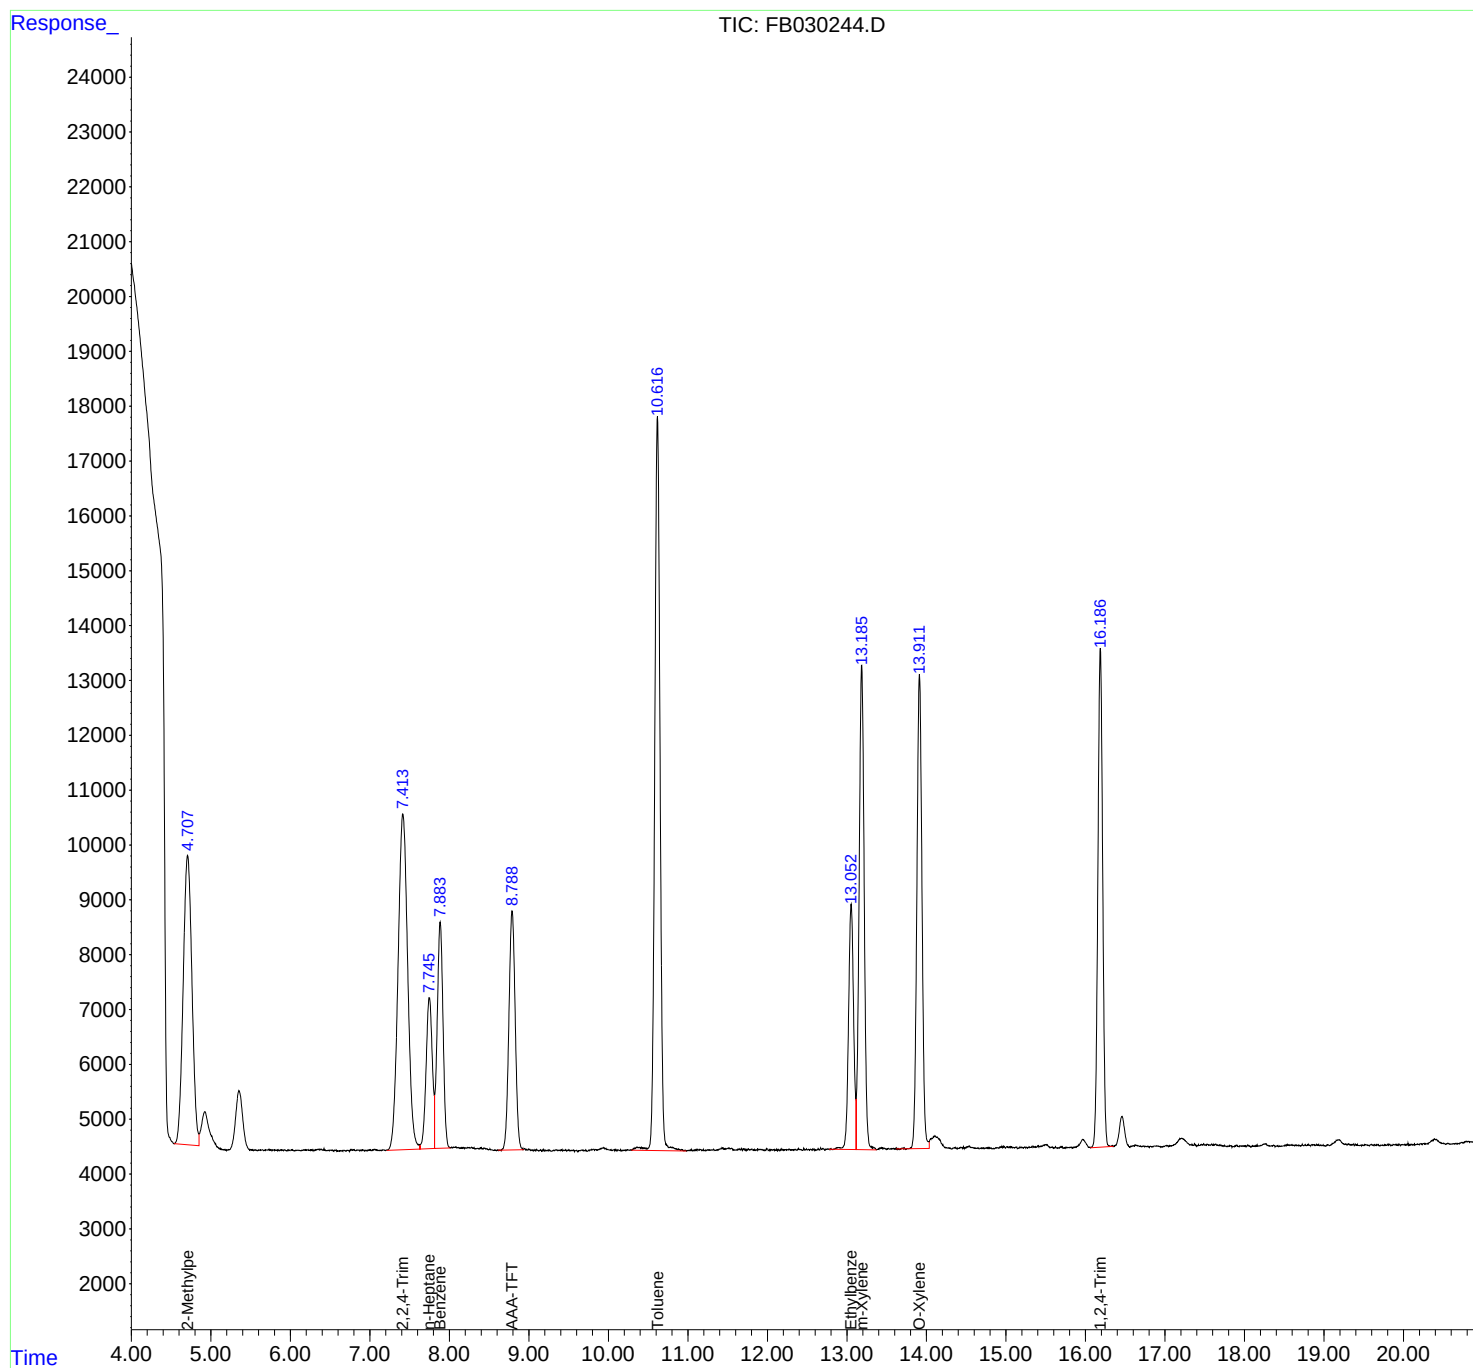


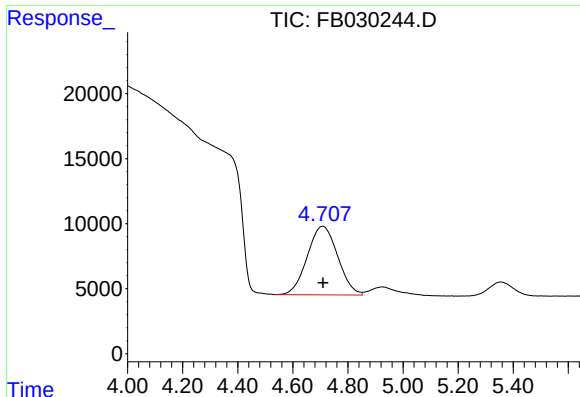

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 403564
Conc: 24.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0814S1

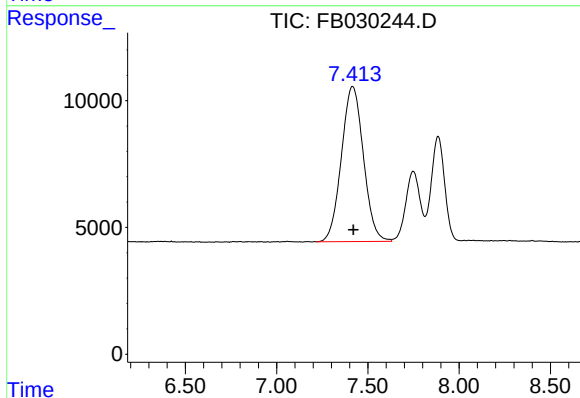


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.006 min
Response: 512777
Conc: 27.63 ng/ml

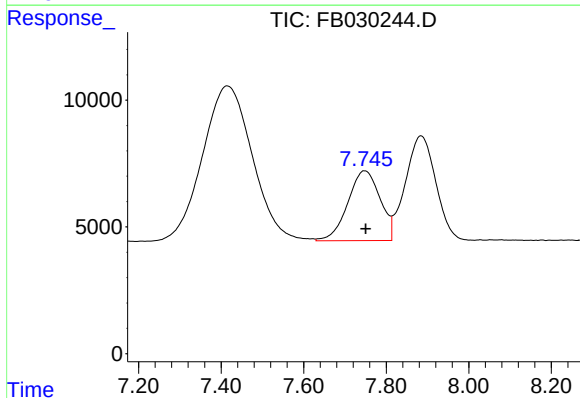


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 149621
Conc: 7.78 ng/ml

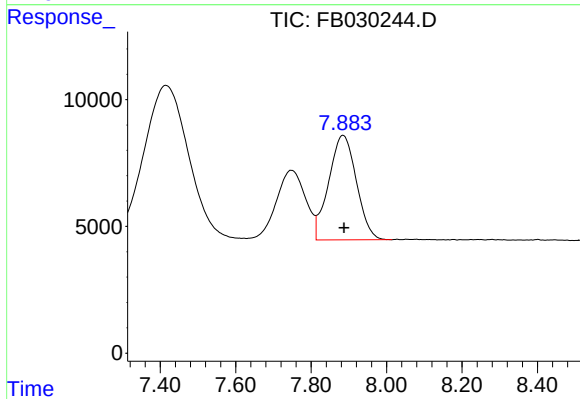

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 210546
Conc: 8.95 ng/ml

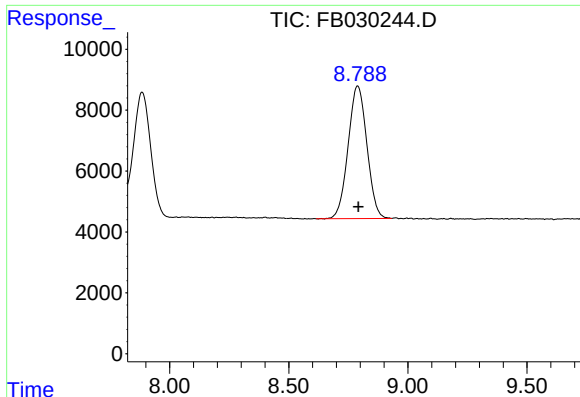

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.003 min
Response: 238672
Conc: 19.42 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0814S1

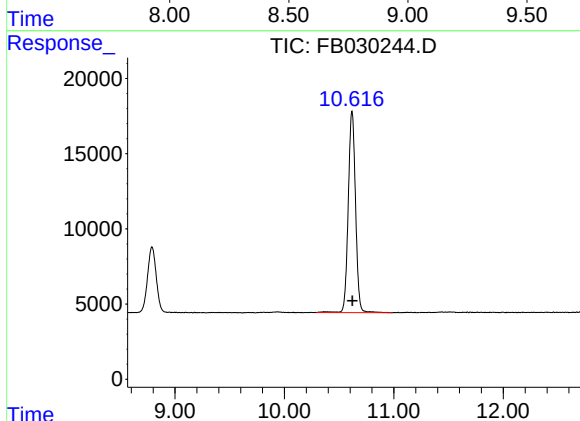


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 621193
Conc: 27.11 ng/ml

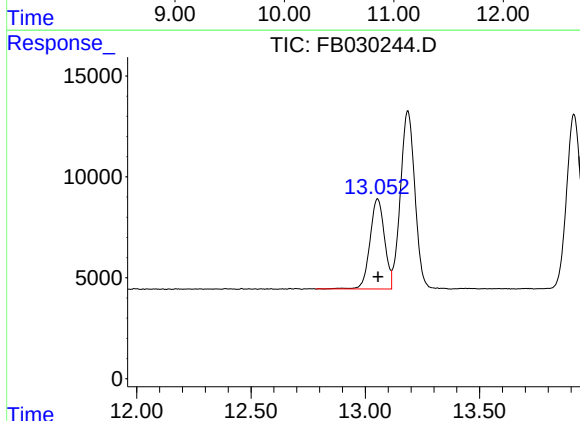


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.003 min
Response: 196907
Conc: 9.17 ng/ml

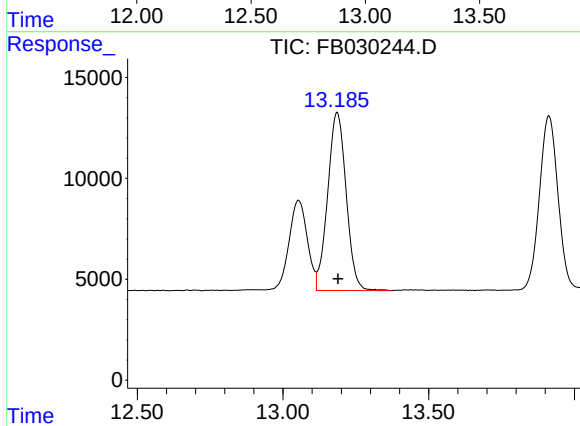

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.003 min
Response: 389513
Conc: 18.52 ng/ml

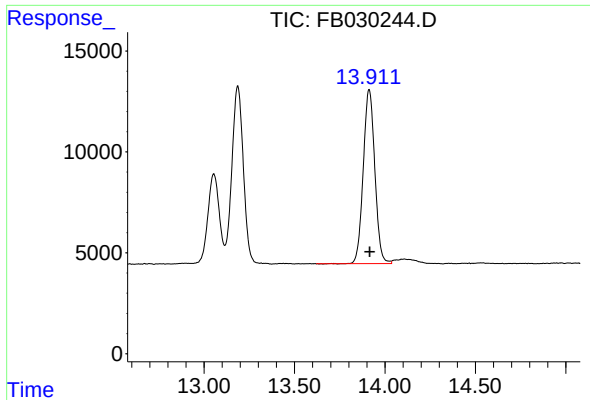

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.003 min
Response: 383313
Conc: 18.68 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0814S1

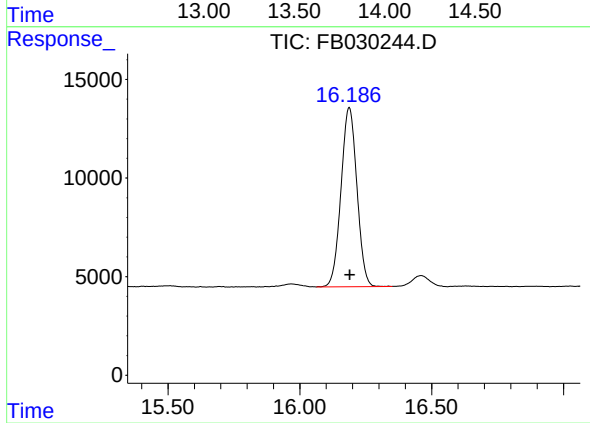

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.002 min
Response: 380183
Conc: 19.42 ng/ml