

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081423\
 Data File : FB030264.D
 Signal(s) : FID2B.CH
 Acq On : 15 Aug 2023 00:55
 Operator : YP/AJ
 Sample : BSF0814S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0814S3

Integration File: Calibration.e
 Quant Time: Aug 15 02:31:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
 Quant Title :
 QLast Update : Tue Jul 25 06:41:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	193886	15.775 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	412162	24.950 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	520020	28.024 ng/ml
3) t n-Heptane	7.751	157300	8.176 ng/ml
4) t Benzene	7.888	216787	9.215 ng/ml
6) t Toluene	10.620	644183	28.109 ng/ml
7) t Ethylbenzene	13.057	207570	9.671 ng/ml
8) t m-Xylene	13.189	404096	19.215 ng/ml
9) t O-Xylene	13.916	389502	18.978 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	371017	18.955 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081423\
Data File : FB030264.D
Signal(s) : FID2B.CH
Acq On : 15 Aug 2023 00:55
Operator : YP/AJ
Sample : BSF0814S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0814S3

Integration File: Calibration.e
Quant Time: Aug 15 02:31:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB072423.M
Quant Title :
QLast Update : Tue Jul 25 06:41:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

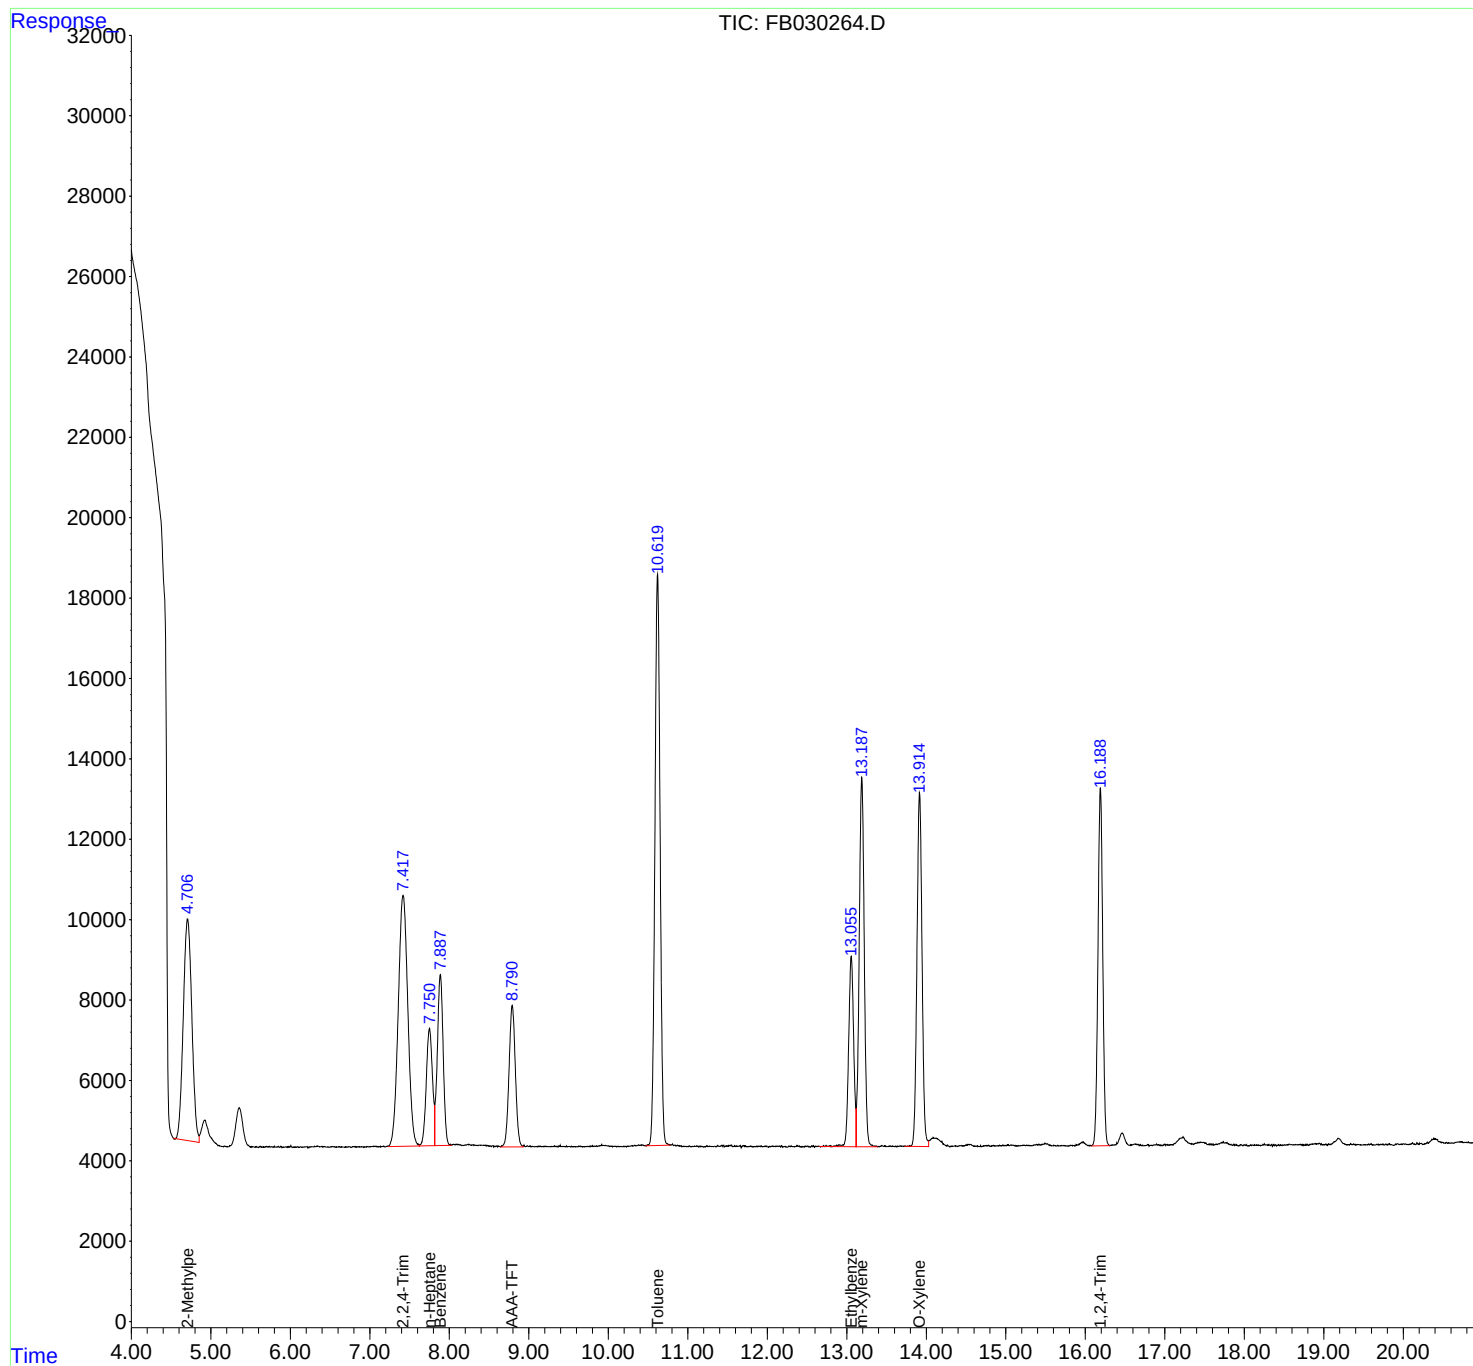


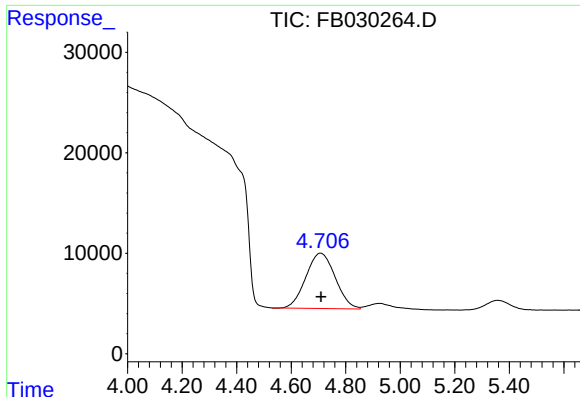

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 412162
Conc: 24.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0814S3

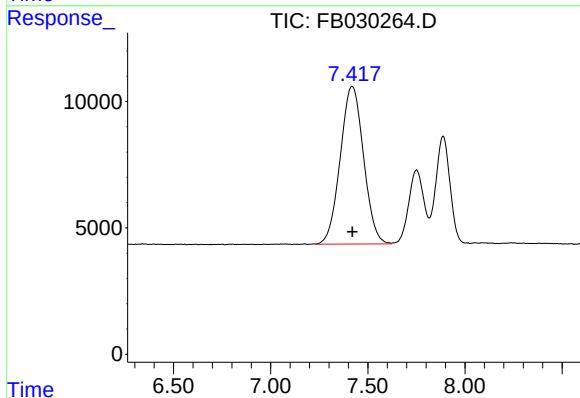


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.002 min
Response: 520020
Conc: 28.02 ng/ml

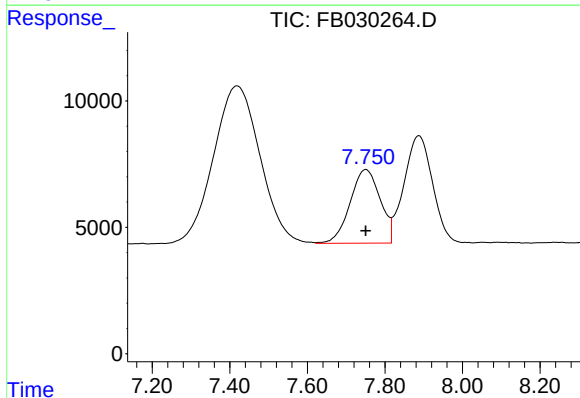


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.001 min
Response: 157300
Conc: 8.18 ng/ml

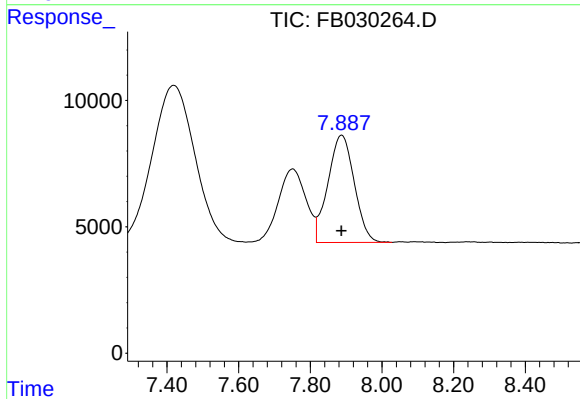

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 216787
Conc: 9.22 ng/ml

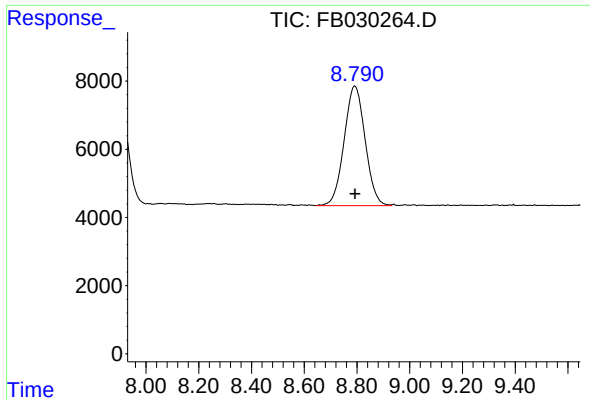

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.001 min
Response: 193886
Conc: 15.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0814S3

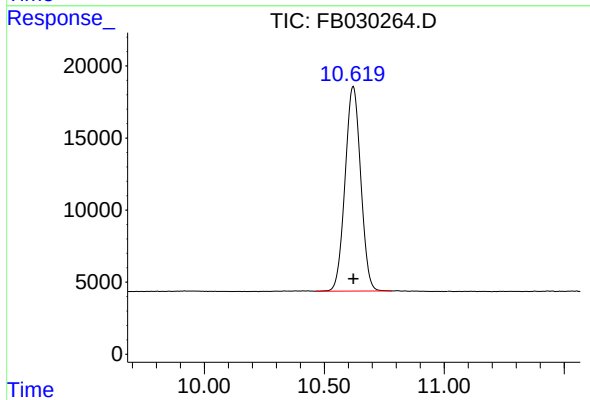


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 644183
Conc: 28.11 ng/ml

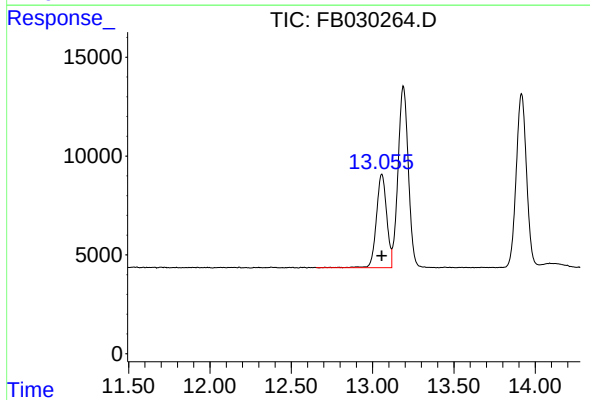


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 207570
Conc: 9.67 ng/ml

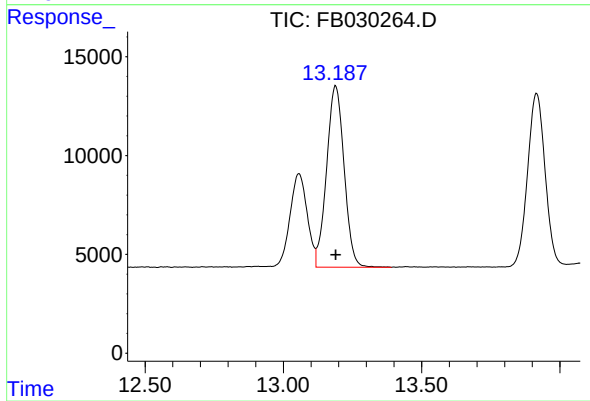

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 404096
Conc: 19.21 ng/ml

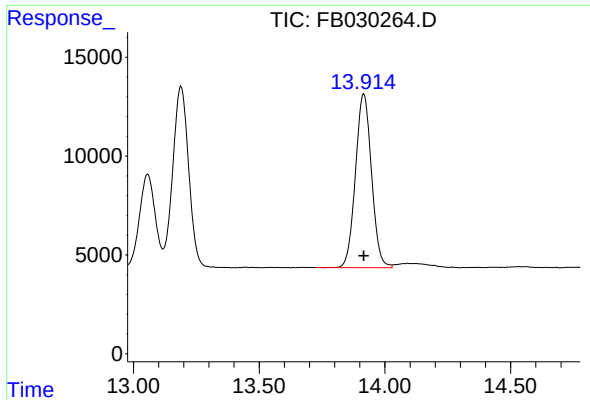

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 389502
Conc: 18.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0814S3

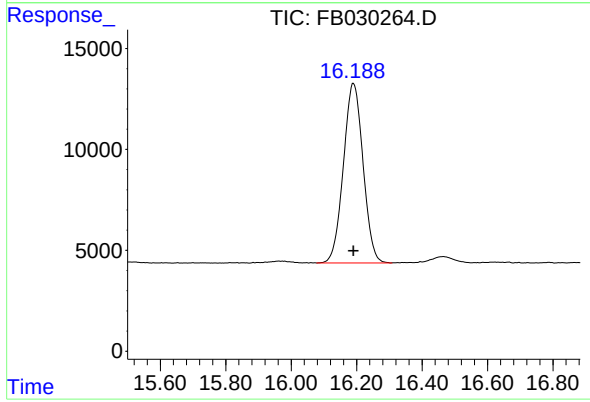

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 371017
Conc: 18.96 ng/ml