

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081519\
 Data File : FB022023.D
 Signal(s) : FID2B.CH
 Acq On : 15 Aug 2019 13:18
 Operator : DD/AJ
 Sample : BSF0815S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 15 13:46:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
 Quant Title :
 QLast Update : Thu Aug 15 11:19:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	241051	18.670 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	781926	28.858 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	811074	30.398 ng/ml
3) t n-Heptane	7.950	242802	9.941 ng/ml
4) t Benzene	8.085	269690	9.353 ng/ml
6) t Toluene	10.832	578305	29.136 ng/ml
7) t Ethylbenzene	13.277	197511	9.794 ng/ml
8) t m-Xylene	13.410	421464	19.468 ng/ml
9) t O-Xylene	14.139	443094	19.785 ng/ml
10) t 1,2,4-Trimethylbenzene	16.419	458584	19.519 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081519\
Data File : FB022023.D
Signal(s) : FID2B.CH
Acq On : 15 Aug 2019 13:18
Operator : DD/AJ
Sample : BSF081551
Misc : 5.01/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 15 13:46:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
Quant Title :
QLast Update : Thu Aug 15 11:19:59 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

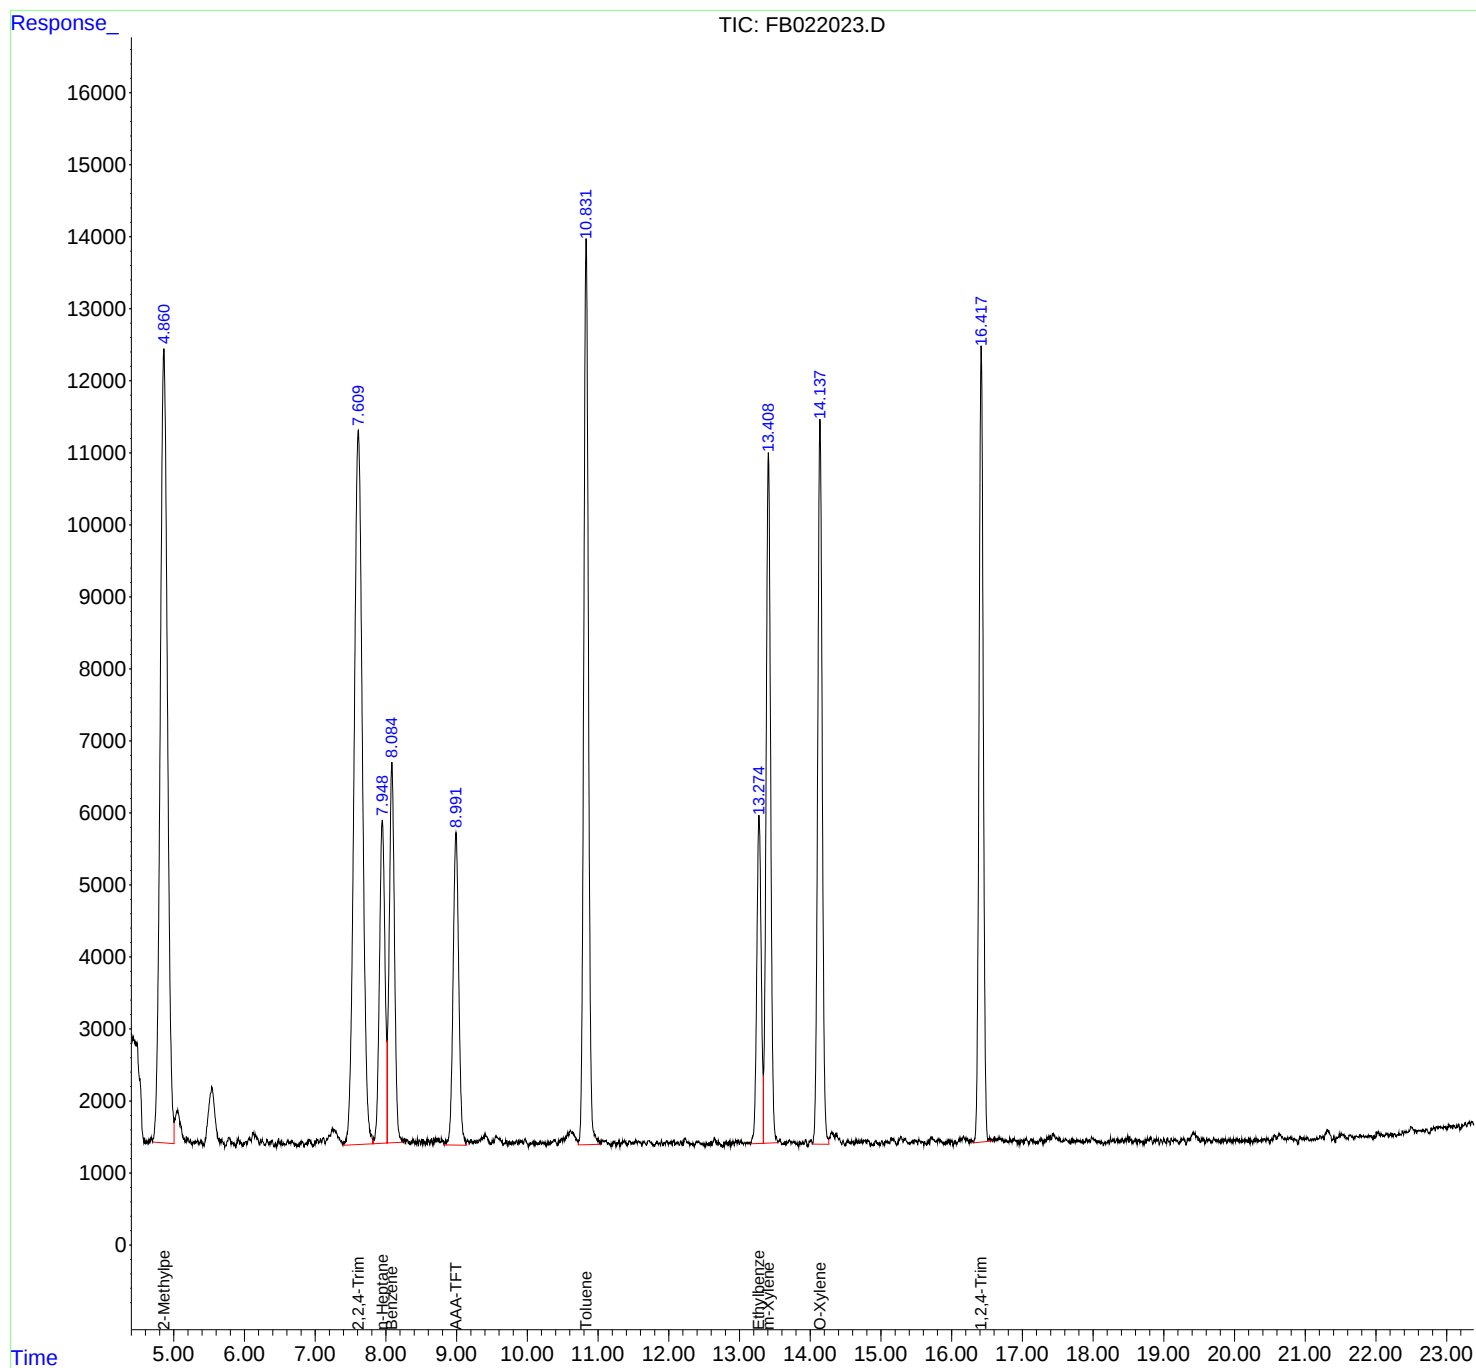

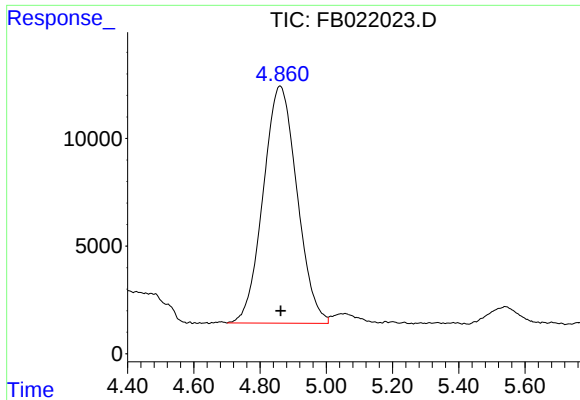


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 781926
Conc: 28.86 ng/ml

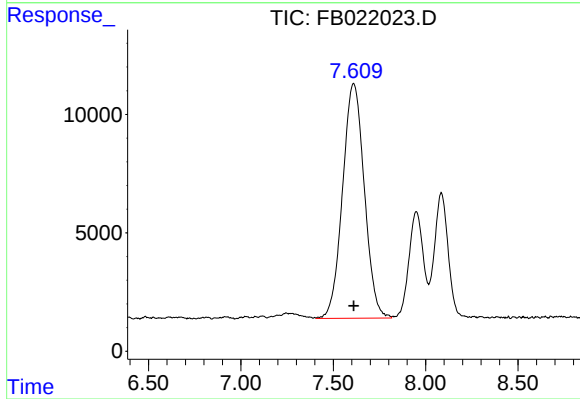


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: -0.001 min
Response: 811074
Conc: 30.40 ng/ml

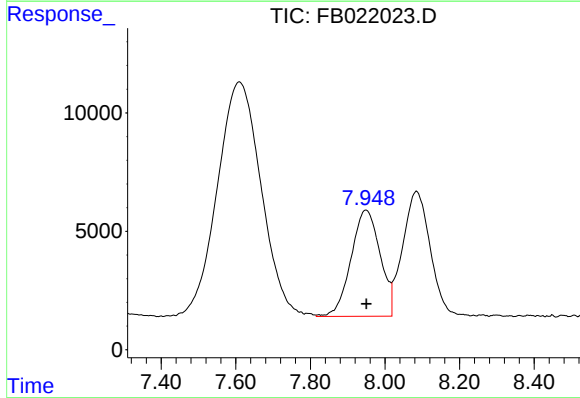


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.001 min
Response: 242802
Conc: 9.94 ng/ml

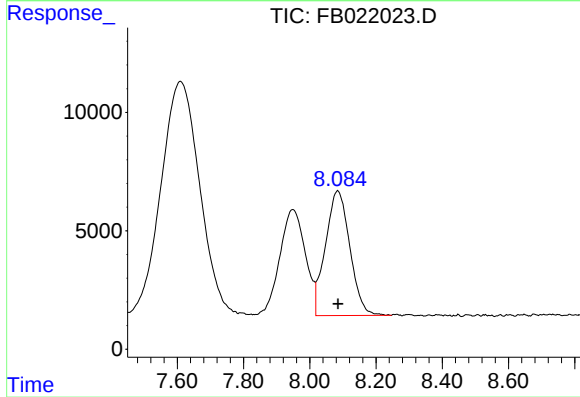


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 269690
Conc: 9.35 ng/ml

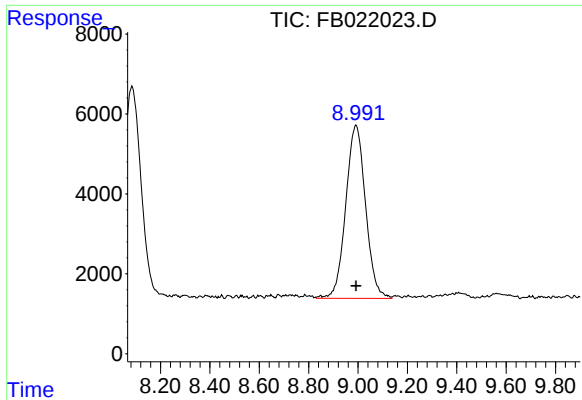


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 241051
Conc: 18.67 ng/ml

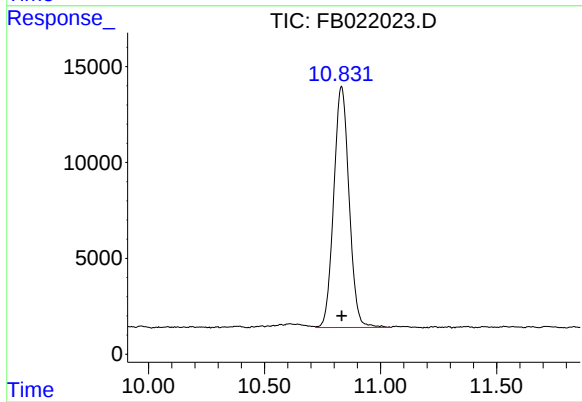


#6 Toluene

R.T.: 10.832 min
Delta R.T.: 0.000 min
Response: 578305
Conc: 29.14 ng/ml

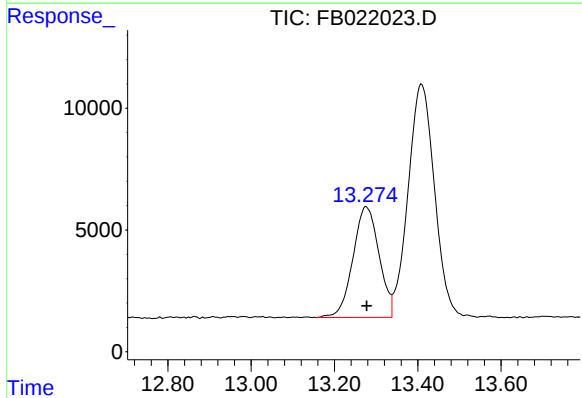


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: 0.000 min
Response: 197511
Conc: 9.79 ng/ml

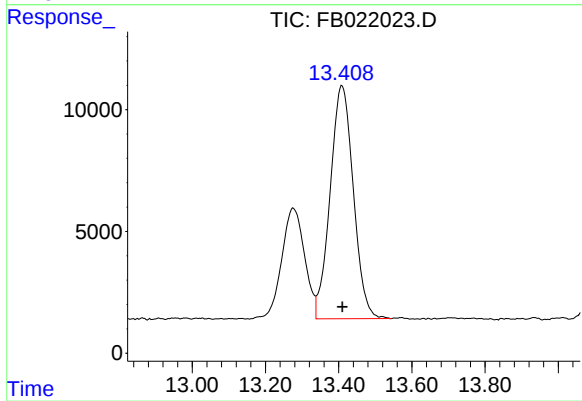

#8 m-Xylene

R.T.: 13.410 min
Delta R.T.: 0.000 min
Response: 421464
Conc: 19.47 ng/ml

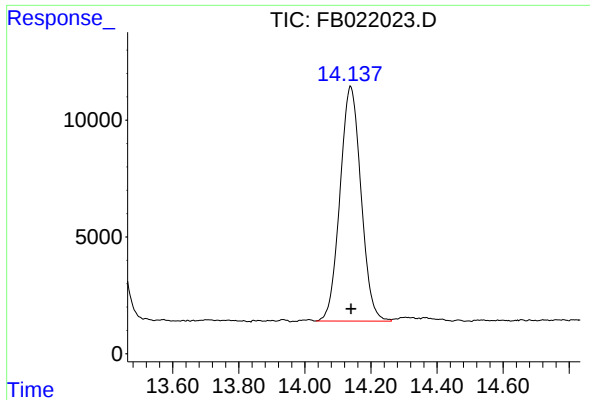


#9 O-Xylene

R.T.: 14.139 min

Delta R.T.: 0.000 min

Response: 443094

Conc: 19.79 ng/ml

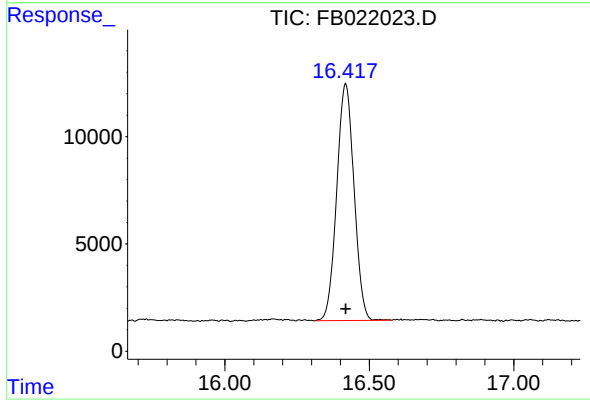

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min

Delta R.T.: 0.000 min

Response: 458584

Conc: 19.52 ng/ml