

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081522\
 Data File : FB027979.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2022 1:43
 Operator : AJ/MA
 Sample : N4211-02MSD
 Misc : 5.08G/5.00 ML DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 16 06:35:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	207752	17.926 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	400757	22.153 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	481042	24.530 ng/ml
3) t n-Heptane	7.749	147040	7.632 ng/ml
4) t Benzene	7.886	224457	9.654 ng/ml
6) t Toluene	10.620	609602	27.800 ng/ml
7) t Ethylbenzene	13.057	191700	9.303 ng/ml
8) t m-Xylene	13.189	374410	18.297 ng/ml
9) t O-Xylene	13.916	370771	18.717 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	342803	17.579 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081522\
Data File : FB027979.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2022 1:43
Operator : AJ/MA
Sample : N4211-02MSD
Misc : 5.08G/5.00 ML DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 16 06:35:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

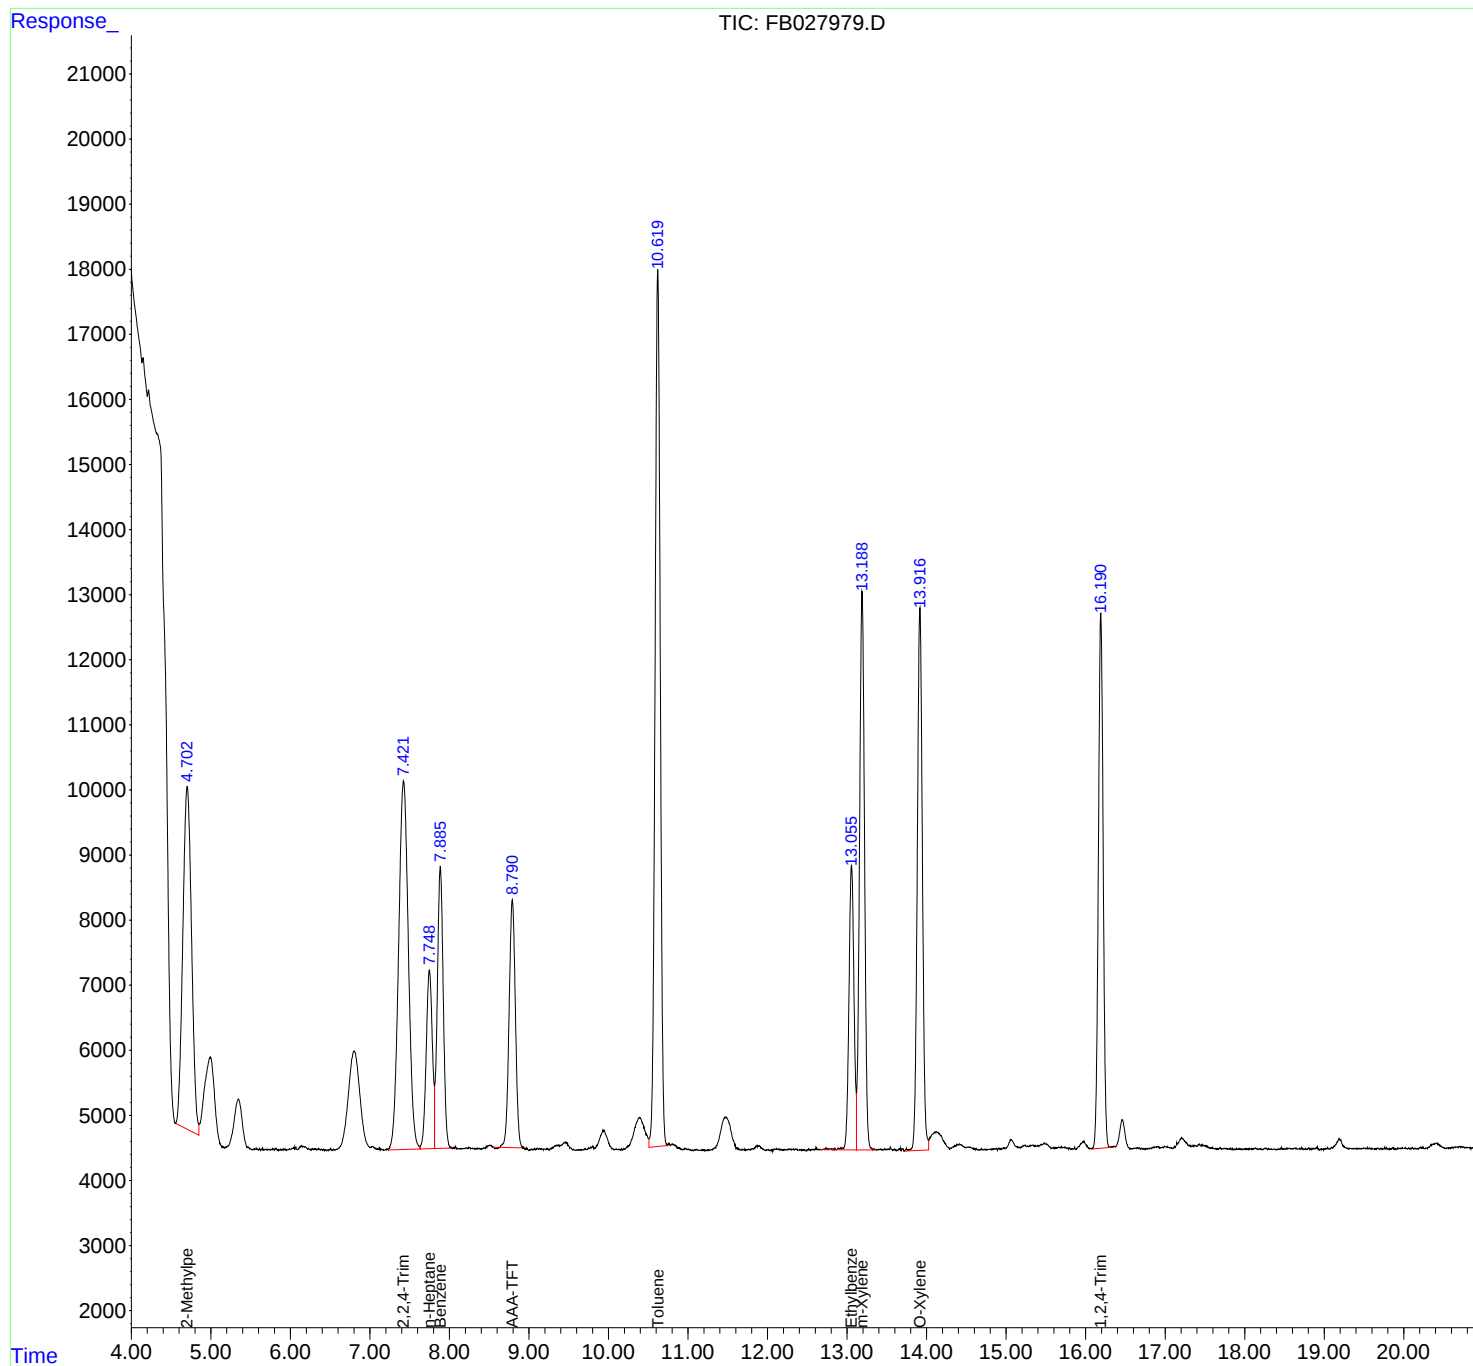


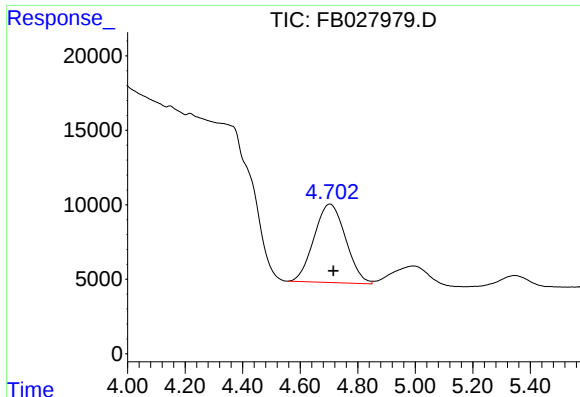

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.012 min
Response: 400757
Conc: 22.15 ng/ml

Instrument :
FID_B
ClientSampleId :

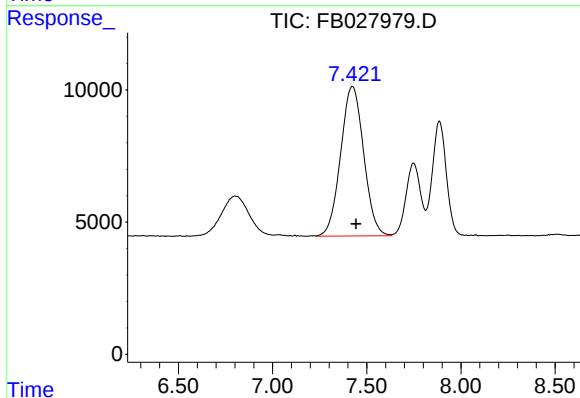


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.019 min
Response: 481042
Conc: 24.53 ng/ml

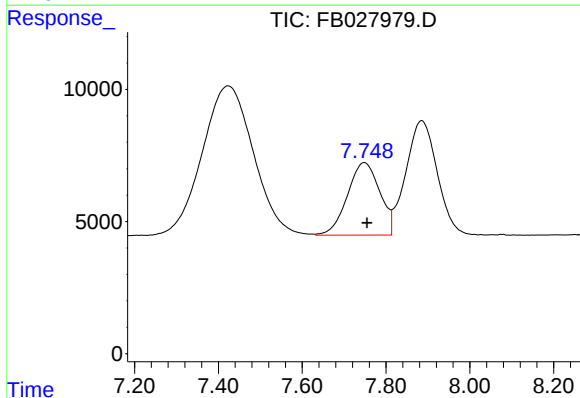


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.006 min
Response: 147040
Conc: 7.63 ng/ml

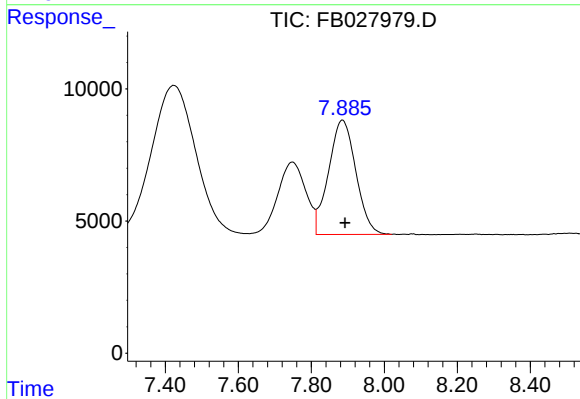

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.006 min
Response: 224457
Conc: 9.65 ng/ml

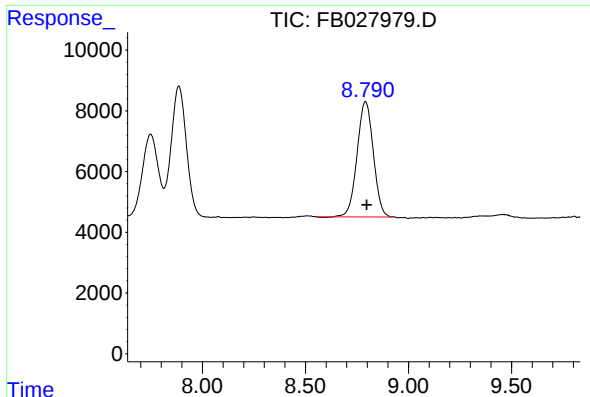

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.007 min
Response: 207752
Conc: 17.93 ng/ml

Instrument :
FID_B
ClientSampleId :

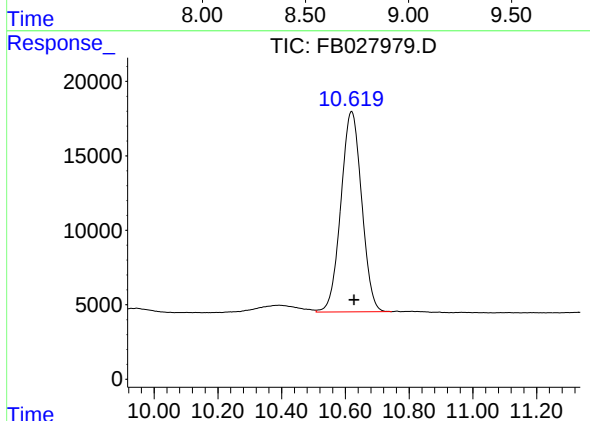


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.007 min
Response: 609602
Conc: 27.80 ng/ml

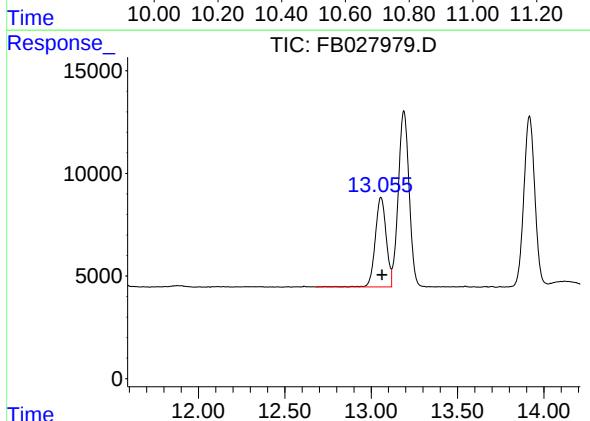


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: -0.008 min
Response: 191700
Conc: 9.30 ng/ml

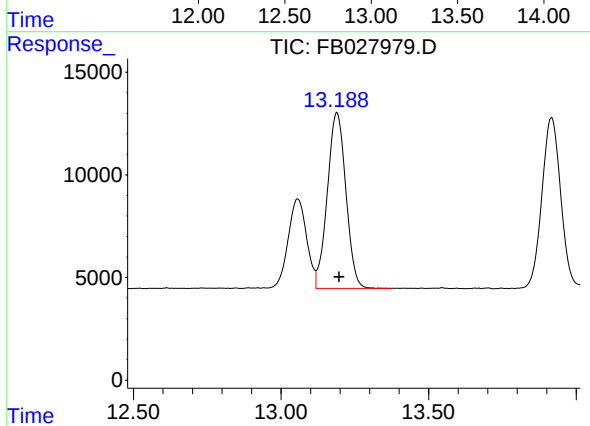

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.008 min
Response: 374410
Conc: 18.30 ng/ml

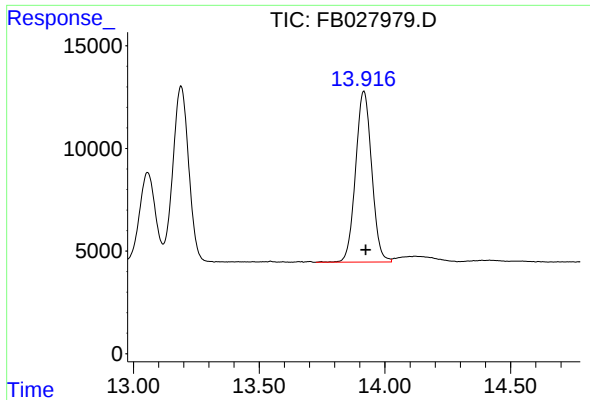

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.008 min
Response: 370771
Conc: 18.72 ng/ml

Instrument :
FID_B
ClientSampleId :

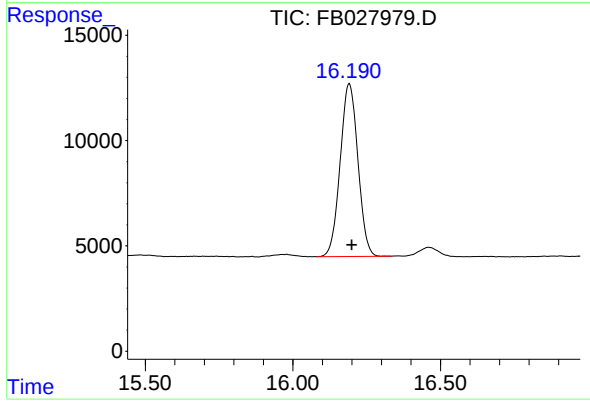

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.008 min
Response: 342803
Conc: 17.58 ng/ml