

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081522\
Data File : FB027961.D
Signal(s) : FID2B.CH
Acq On : 15 Aug 2022 13:24
Operator : AJ/MA
Sample : VBF0815S1 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0815S2

Integration File: Calibration.e
Quant Time: Aug 16 04:00:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	215873	18.627 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081522\
Data File : FB027961.D
Signal(s) : FID2B.CH
Acq On : 15 Aug 2022 13:24
Operator : AJ/MA
Sample : VBF0815S1 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0815S2

Integration File: Calibration.e
Quant Time: Aug 16 04:00:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

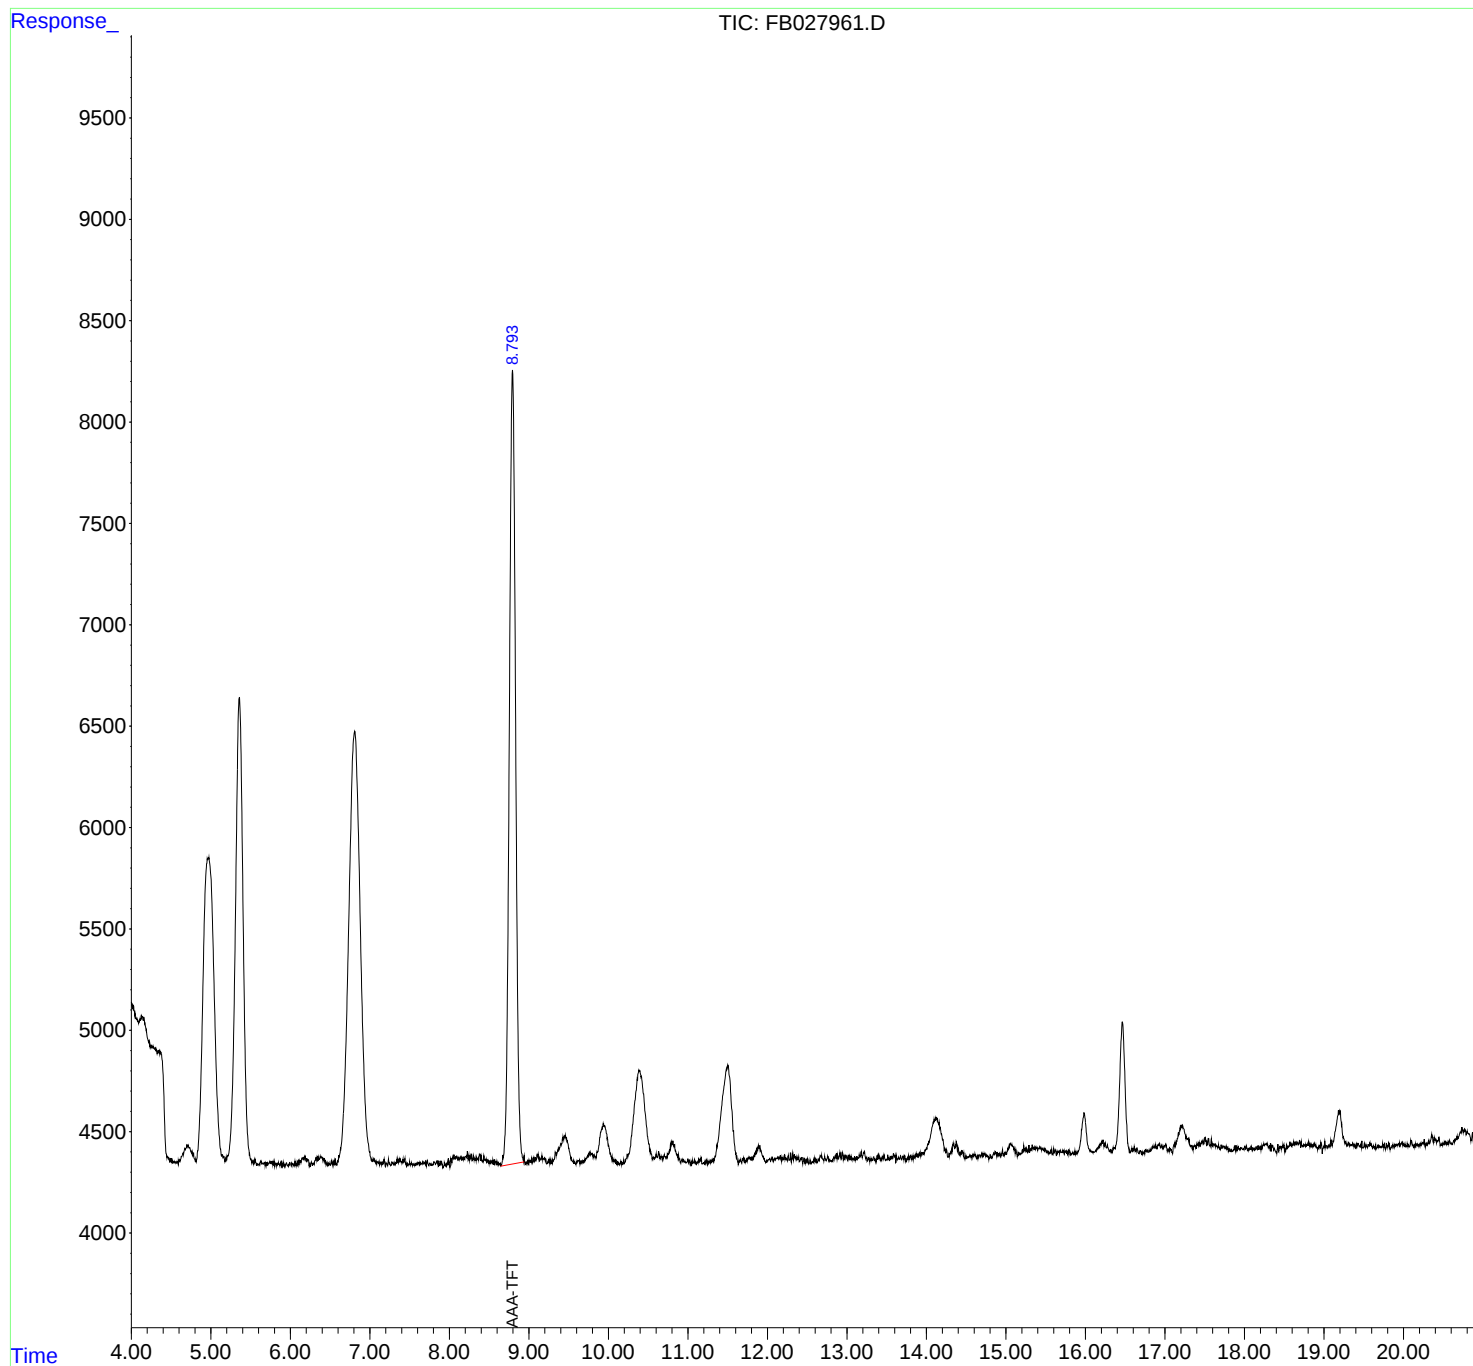

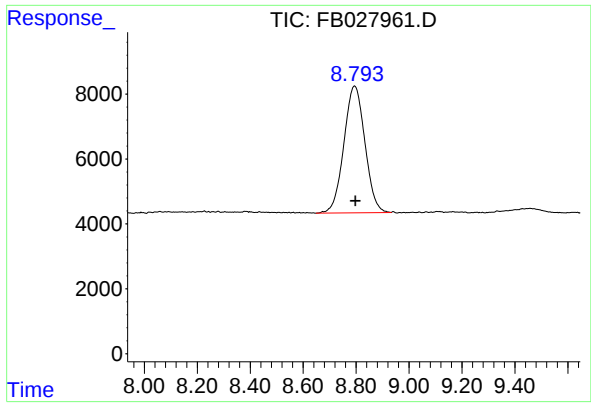

#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 215873
Conc: 18.63 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0815S2