

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081522\
 Data File : FB027962.D
 Signal(s) : FID2B.CH
 Acq On : 15 Aug 2022 14:01
 Operator : AJ/MA
 Sample : BSF0815S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0815S1

Integration File: Calibration.e
 Quant Time: Aug 16 04:01:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	206730	17.838 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	426205	23.559 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	473955	24.169 ng/ml
3) t n-Heptane	7.754	139829	7.258 ng/ml
4) t Benzene	7.890	182970	7.869 ng/ml
6) t Toluene	10.623	520471	23.735 ng/ml
7) t Ethylbenzene	13.061	166718	8.090 ng/ml
8) t m-Xylene	13.192	330439	16.148 ng/ml
9) t O-Xylene	13.919	320793	16.194 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	319115	16.364 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081522\
Data File : FB027962.D
Signal(s) : FID2B.CH
Acq On : 15 Aug 2022 14:01
Operator : AJ/MA
Sample : BSF0815S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0815S1

Integration File: Calibration.e
Quant Time: Aug 16 04:01:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

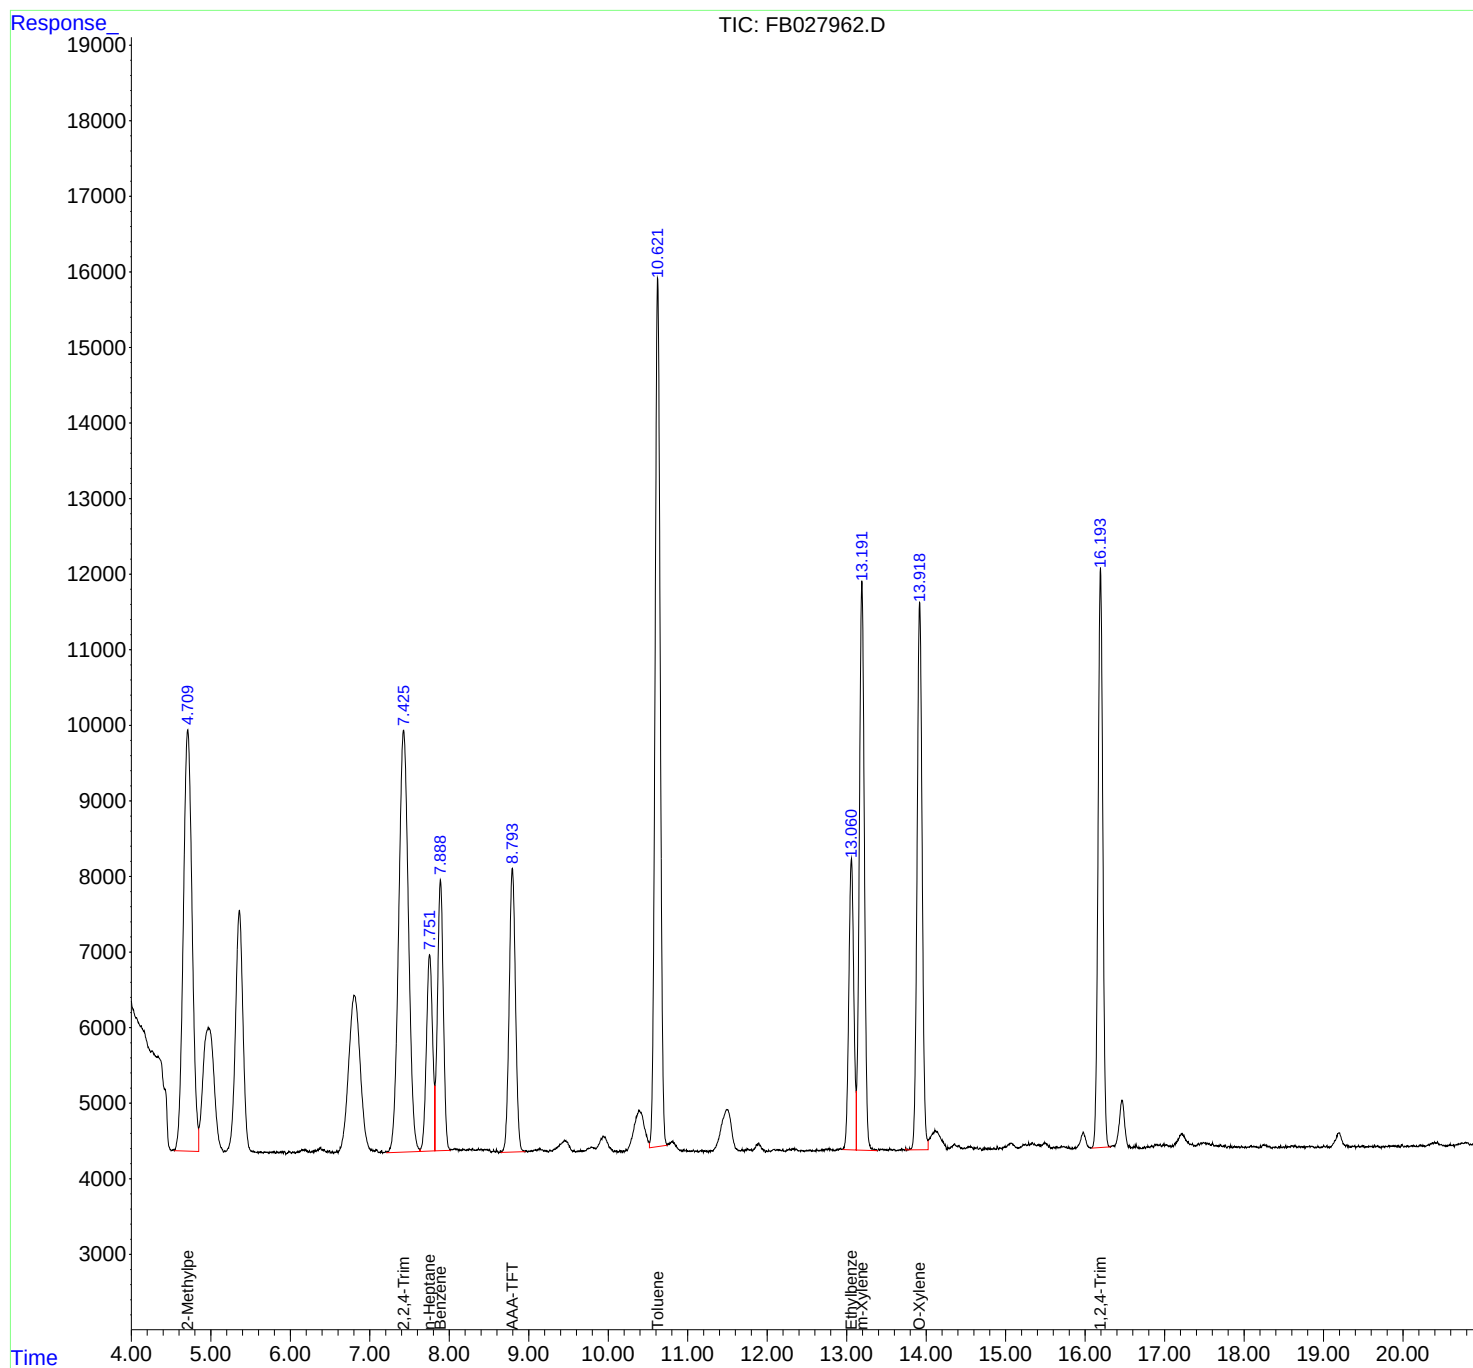


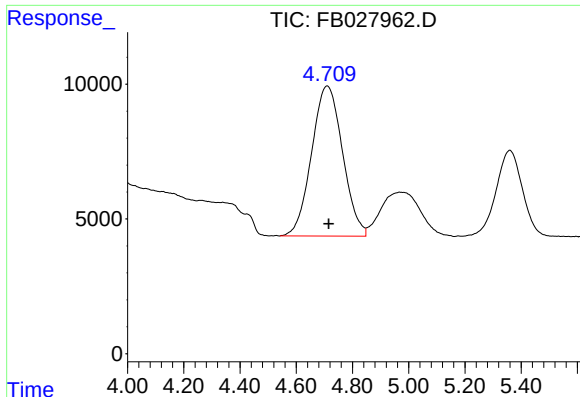

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: -0.004 min
Response: 426205
Conc: 23.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0815S1

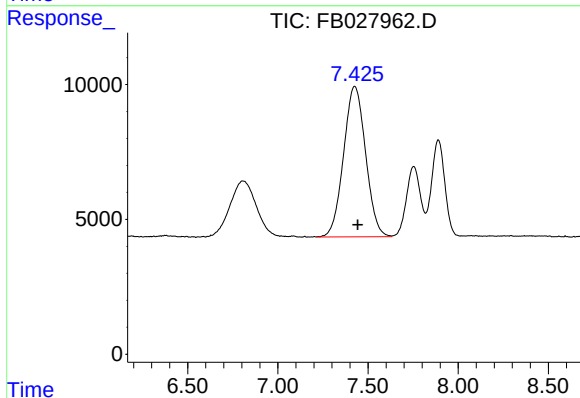


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: -0.016 min
Response: 473955
Conc: 24.17 ng/ml

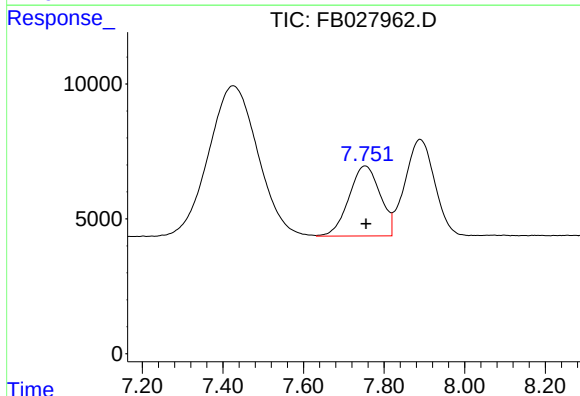


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.002 min
Response: 139829
Conc: 7.26 ng/ml

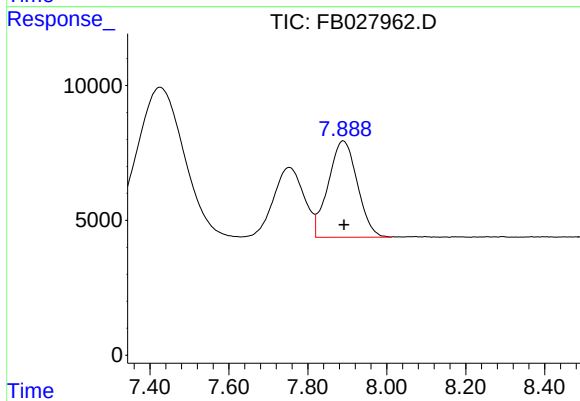

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 182970
Conc: 7.87 ng/ml

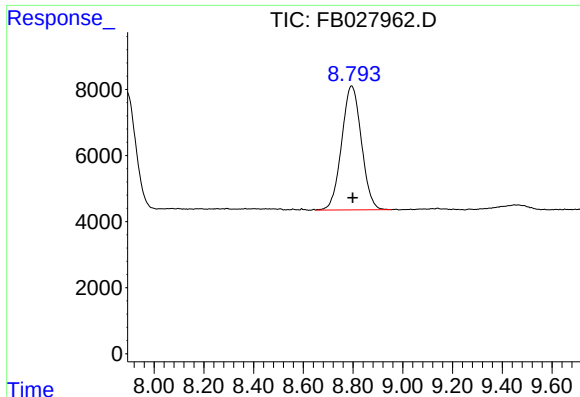

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 206730
Conc: 17.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0815S1

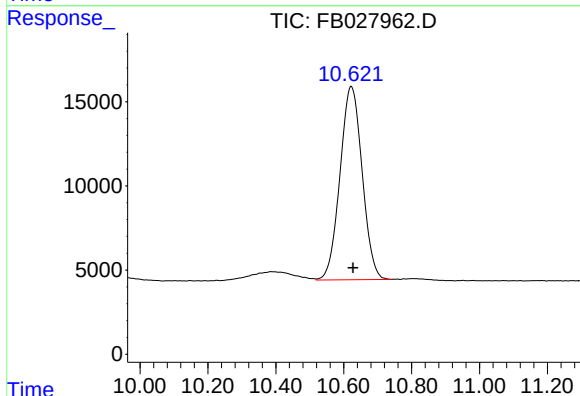


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.004 min
Response: 520471
Conc: 23.74 ng/ml

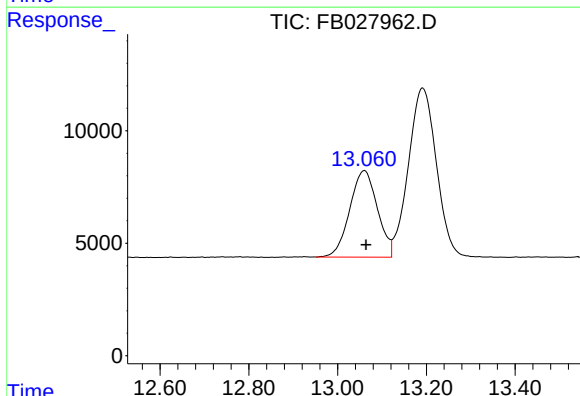


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.003 min
Response: 166718
Conc: 8.09 ng/ml

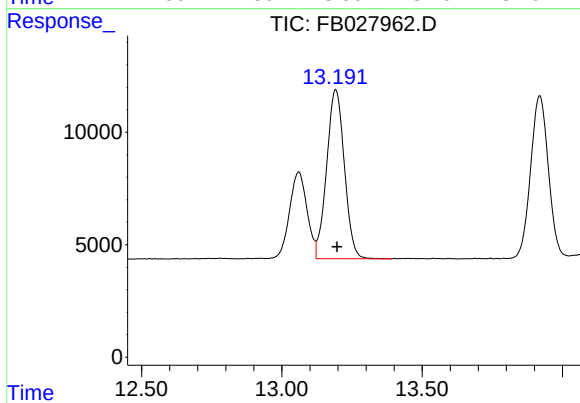

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.005 min
Response: 330439
Conc: 16.15 ng/ml

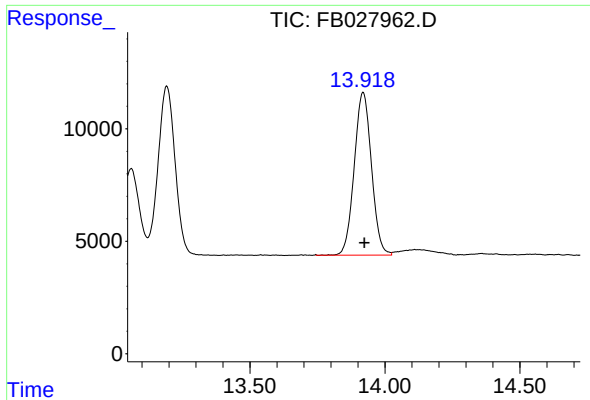

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.005 min
Response: 320793
Conc: 16.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0815S1

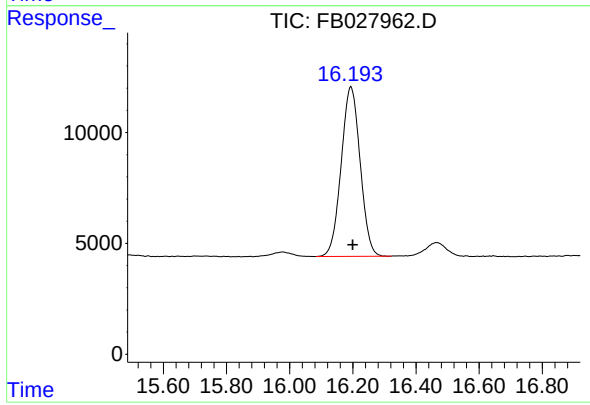

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.005 min
Response: 319115
Conc: 16.36 ng/ml