

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081522\
 Data File : FB027978.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2022 1:07
 Operator : AJ/MA
 Sample : N4211-02MS
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WC-2MS

Integration File: Calibration.e
 Quant Time: Aug 16 06:35:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	210801	18.189 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	329675	18.223 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	432511	22.055 ng/ml
3) t n-Heptane	7.748	119654	6.211 ng/ml
4) t Benzene	7.885	183401	7.888 ng/ml
6) t Toluene	10.620	503117	22.944 ng/ml
7) t Ethylbenzene	13.058	161745	7.849 ng/ml
8) t m-Xylene	13.190	317344	15.508 ng/ml
9) t O-Xylene	13.917	316581	15.982 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	315256	16.166 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081522\
Data File : FB027978.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2022 1:07
Operator : AJ/MA
Sample : N4211-02MS
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WC-2MS

Integration File: Calibration.e
Quant Time: Aug 16 06:35:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

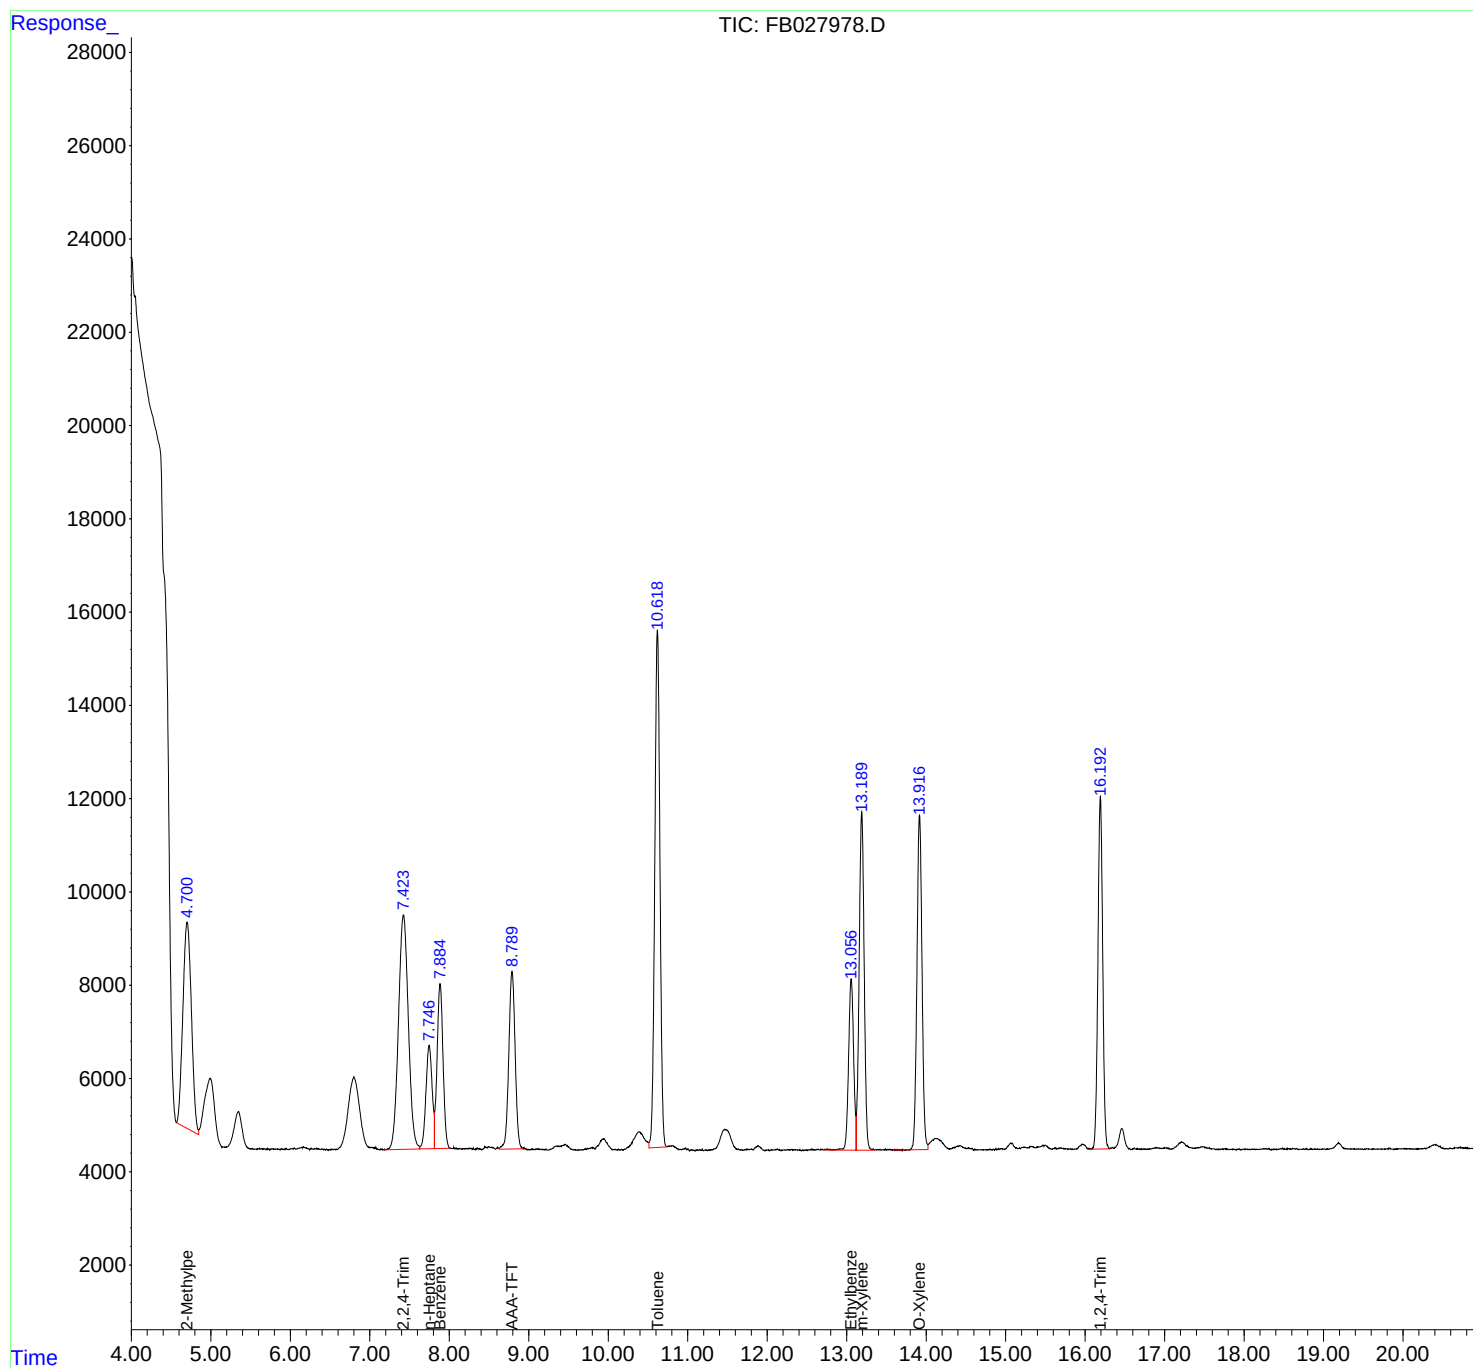


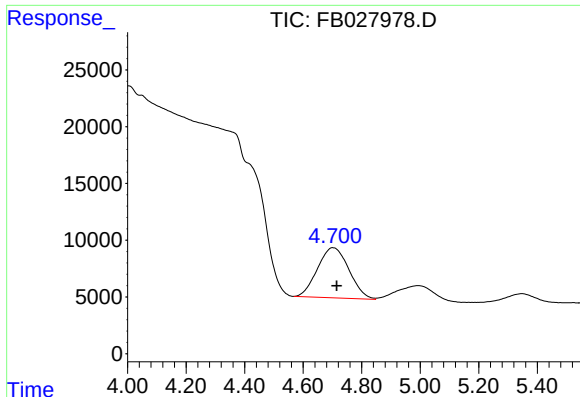

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.014 min
Response: 329675
Conc: 18.22 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-2MS

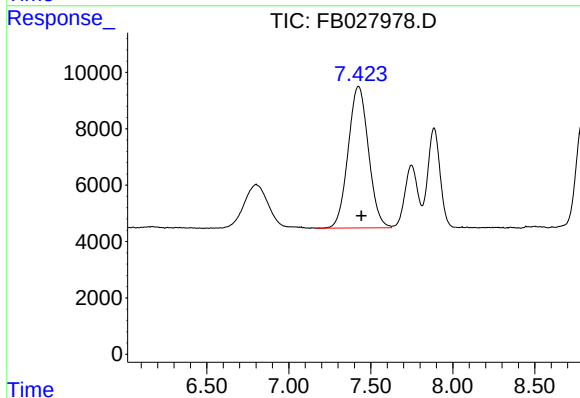


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.018 min
Response: 432511
Conc: 22.06 ng/ml

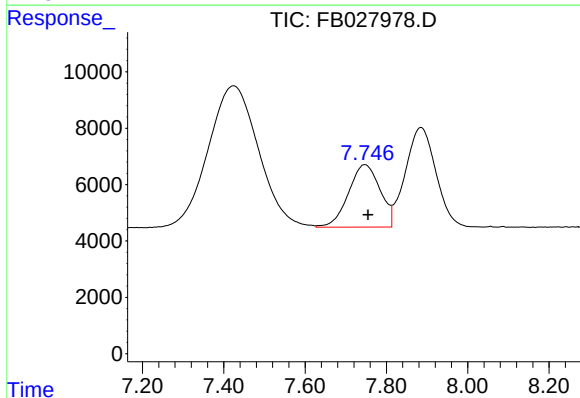


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.007 min
Response: 119654
Conc: 6.21 ng/ml

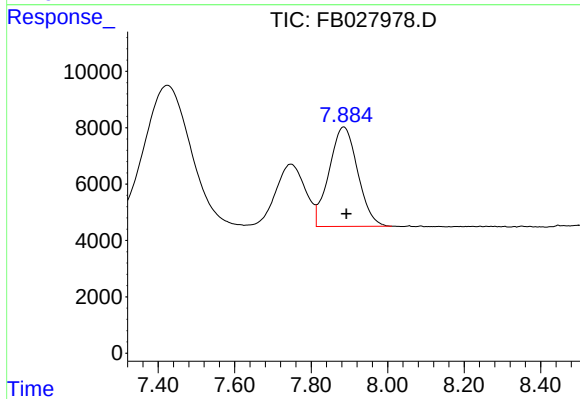

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.007 min
Response: 183401
Conc: 7.89 ng/ml

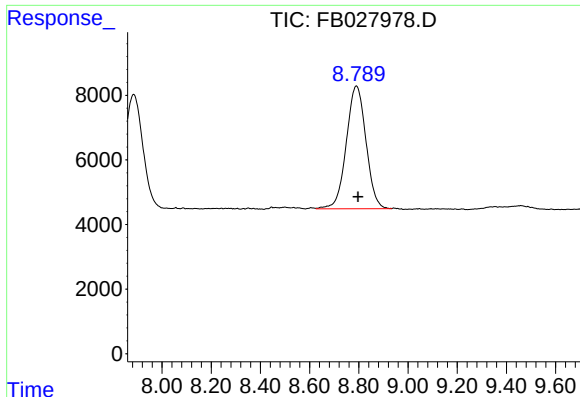

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.007 min
Response: 210801
Conc: 18.19 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-2MS

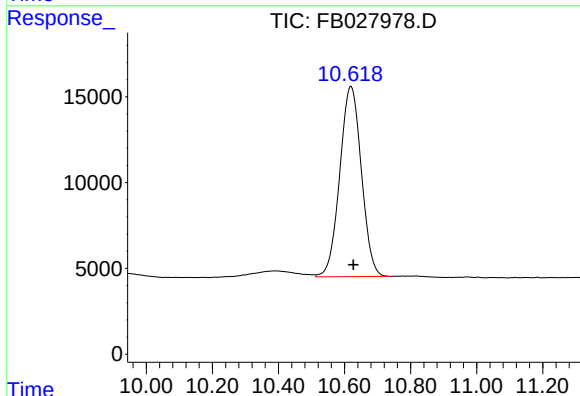


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.007 min
Response: 503117
Conc: 22.94 ng/ml

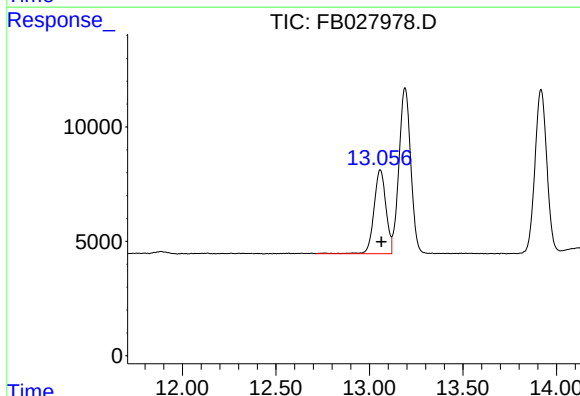


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.007 min
Response: 161745
Conc: 7.85 ng/ml

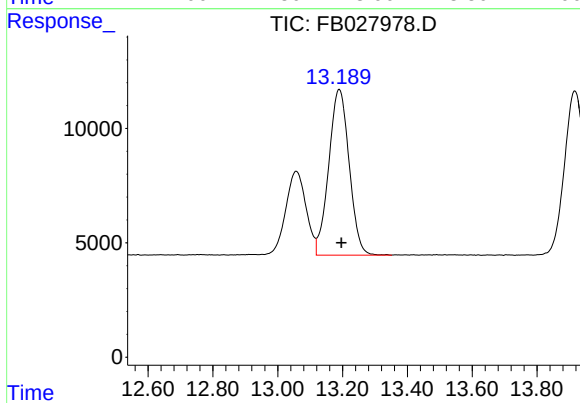

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.007 min
Response: 317344
Conc: 15.51 ng/ml

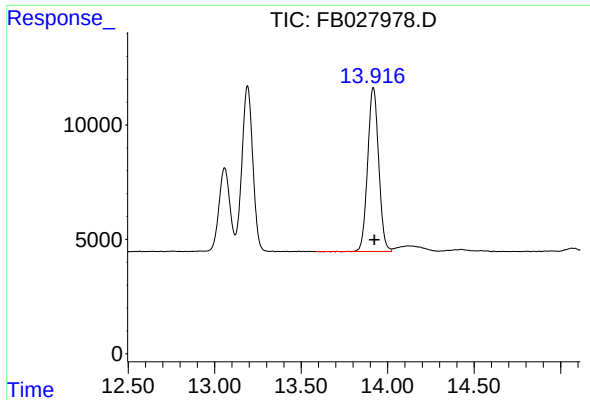

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.007 min
Response: 316581
Conc: 15.98 ng/ml

Instrument :
FID_B
ClientSampleId :
WC-2MS

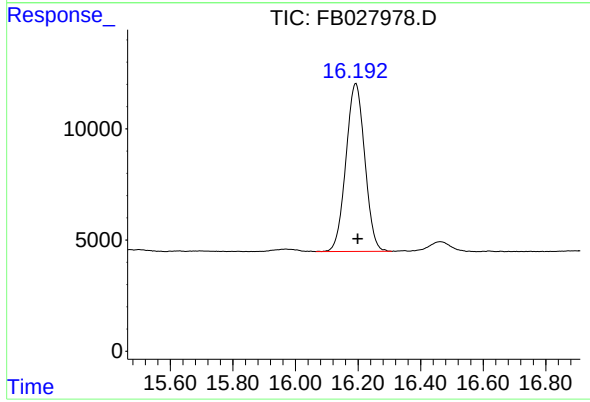

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: -0.006 min
Response: 315256
Conc: 16.17 ng/ml