

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
 Data File : FB022025.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2019 8:58
 Operator : DD/AJ
 Sample : VBF0816S1
 Misc : 5.02/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 17 00:25:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
 Quant Title :
 QLast Update : Thu Aug 15 11:19:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	244679	18.951 ng/ml
Target Compounds				
2) t	2,2,4-Trimethylpentane	7.613	2419	0.091 ng/ml
3) t	n-Heptane	7.962	2247	0.092 ng/ml
6) t	Toluene	10.841	2713	0.137 ng/ml
7) t	Ethylbenzene	13.279	1424	0.071 ng/ml
8) t	m-Xylene	13.415	1715	0.079 ng/ml
9) t	O-Xylene	14.113	2109	0.094 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
Data File : FB022025.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2019 8:58
Operator : DD/AJ
Sample : VBF0816S1
Misc : 5.02/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 00:25:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
Quant Title :
QLast Update : Thu Aug 15 11:19:59 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

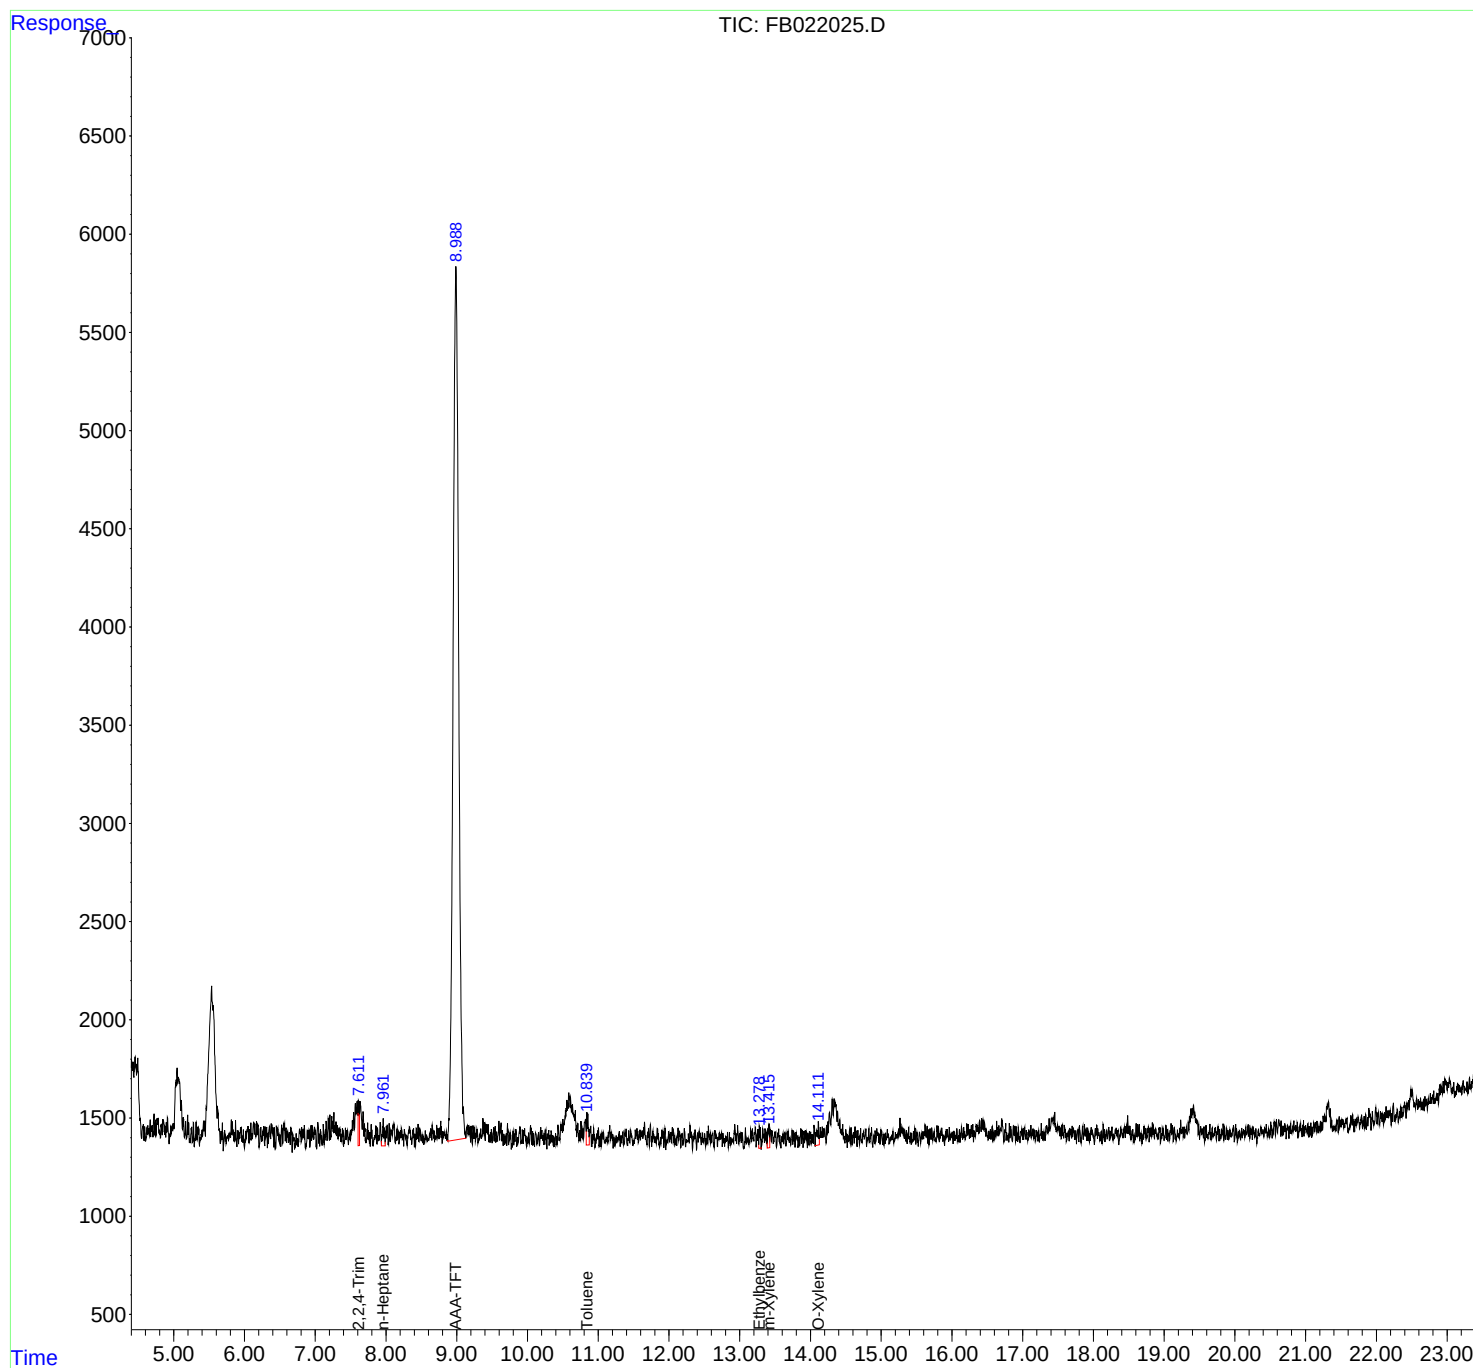

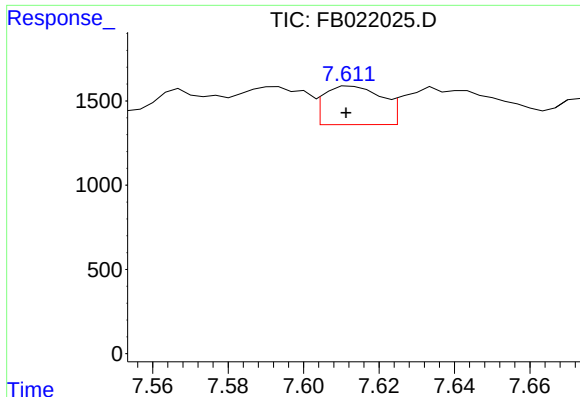


#2 2,2,4-Trimethylpentane

R.T.: 7.613 min
Delta R.T.: 0.002 min
Response: 2419
Conc: 0.09 ng/ml

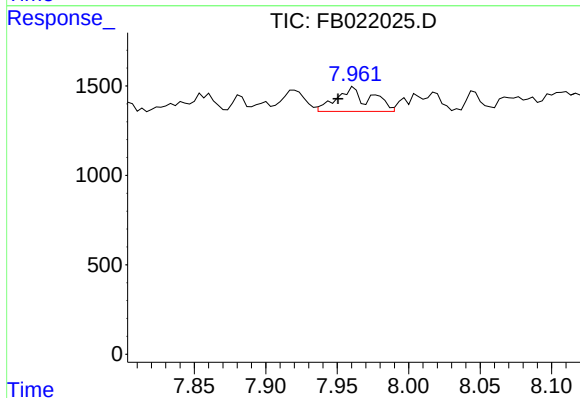


#3 n-Heptane

R.T.: 7.962 min
Delta R.T.: 0.011 min
Response: 2247
Conc: 0.09 ng/ml

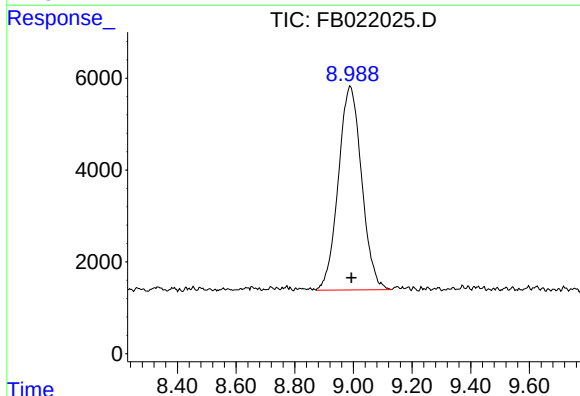


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.003 min
Response: 244679
Conc: 18.95 ng/ml

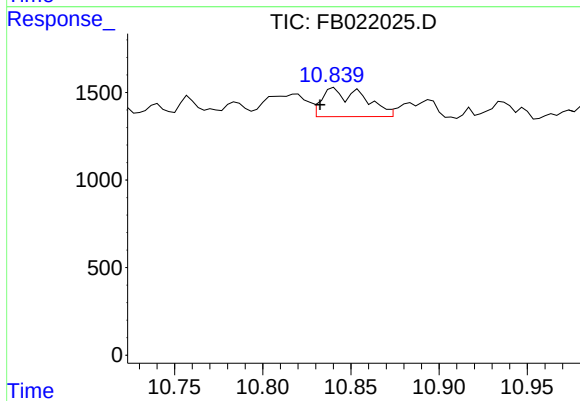


#6 Toluene

R.T.: 10.841 min
Delta R.T.: 0.008 min
Response: 2713
Conc: 0.14 ng/ml

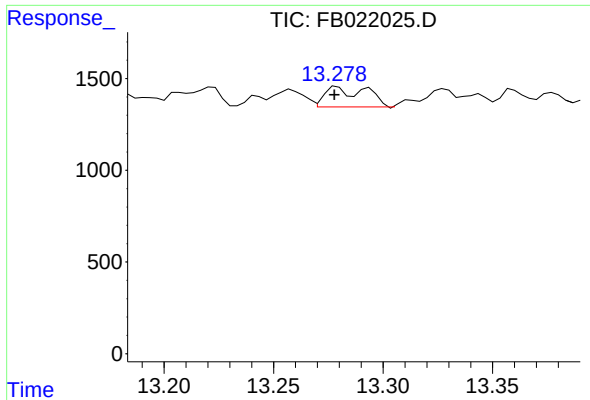


#7 Ethylbenzene

R.T.: 13.279 min
Delta R.T.: 0.002 min
Response: 1424
Conc: 0.07 ng/ml

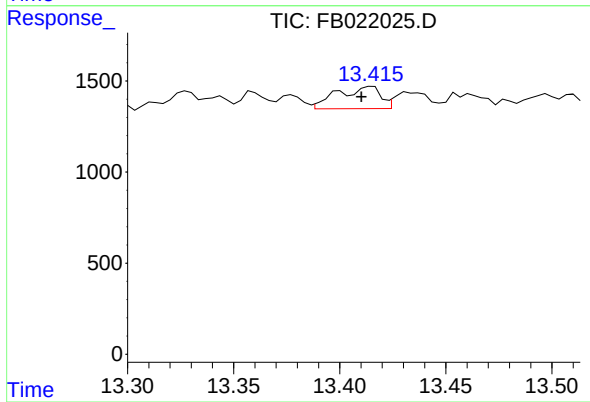

#8 m-Xylene

R.T.: 13.415 min
Delta R.T.: 0.005 min
Response: 1715
Conc: 0.08 ng/ml

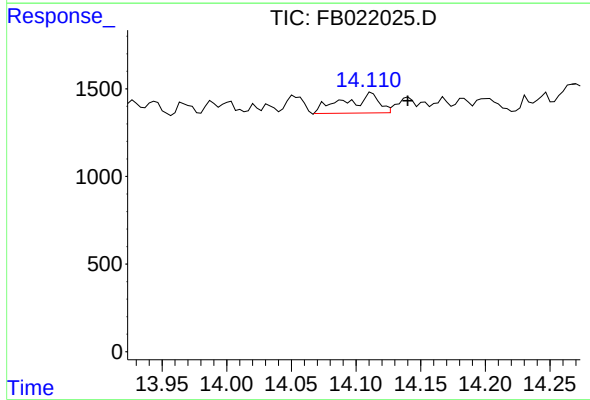

#9 O-Xylene

R.T.: 14.113 min
Delta R.T.: -0.027 min
Response: 2109
Conc: 0.09 ng/ml