

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
 Data File : FB022026.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2019 9:28
 Operator : DD/AJ
 Sample : BSF0816S1
 Misc : 5.01/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 17 00:25:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
 Quant Title :
 QLast Update : Thu Aug 15 11:19:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.990	241122	18.675 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.862	671198	24.771 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	675194	25.305 ng/ml
3) t	n-Heptane	7.949	208767	8.548 ng/ml
4) t	Benzene	8.084	259698	9.006 ng/ml
6) t	Toluene	10.830	581320	29.288 ng/ml
7) t	Ethylbenzene	13.276	207528	10.291 ng/ml
8) t	m-Xylene	13.408	442096	20.421 ng/ml
9) t	O-Xylene	14.138	455321	20.331 ng/ml
10) t	1,2,4-Trimethylbenzene	16.416	459132	19.543 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
Data File : FB022026.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2019 9:28
Operator : DD/AJ
Sample : BSF0816S1
Misc : 5.01/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 00:25:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
Quant Title :
QLast Update : Thu Aug 15 11:19:59 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

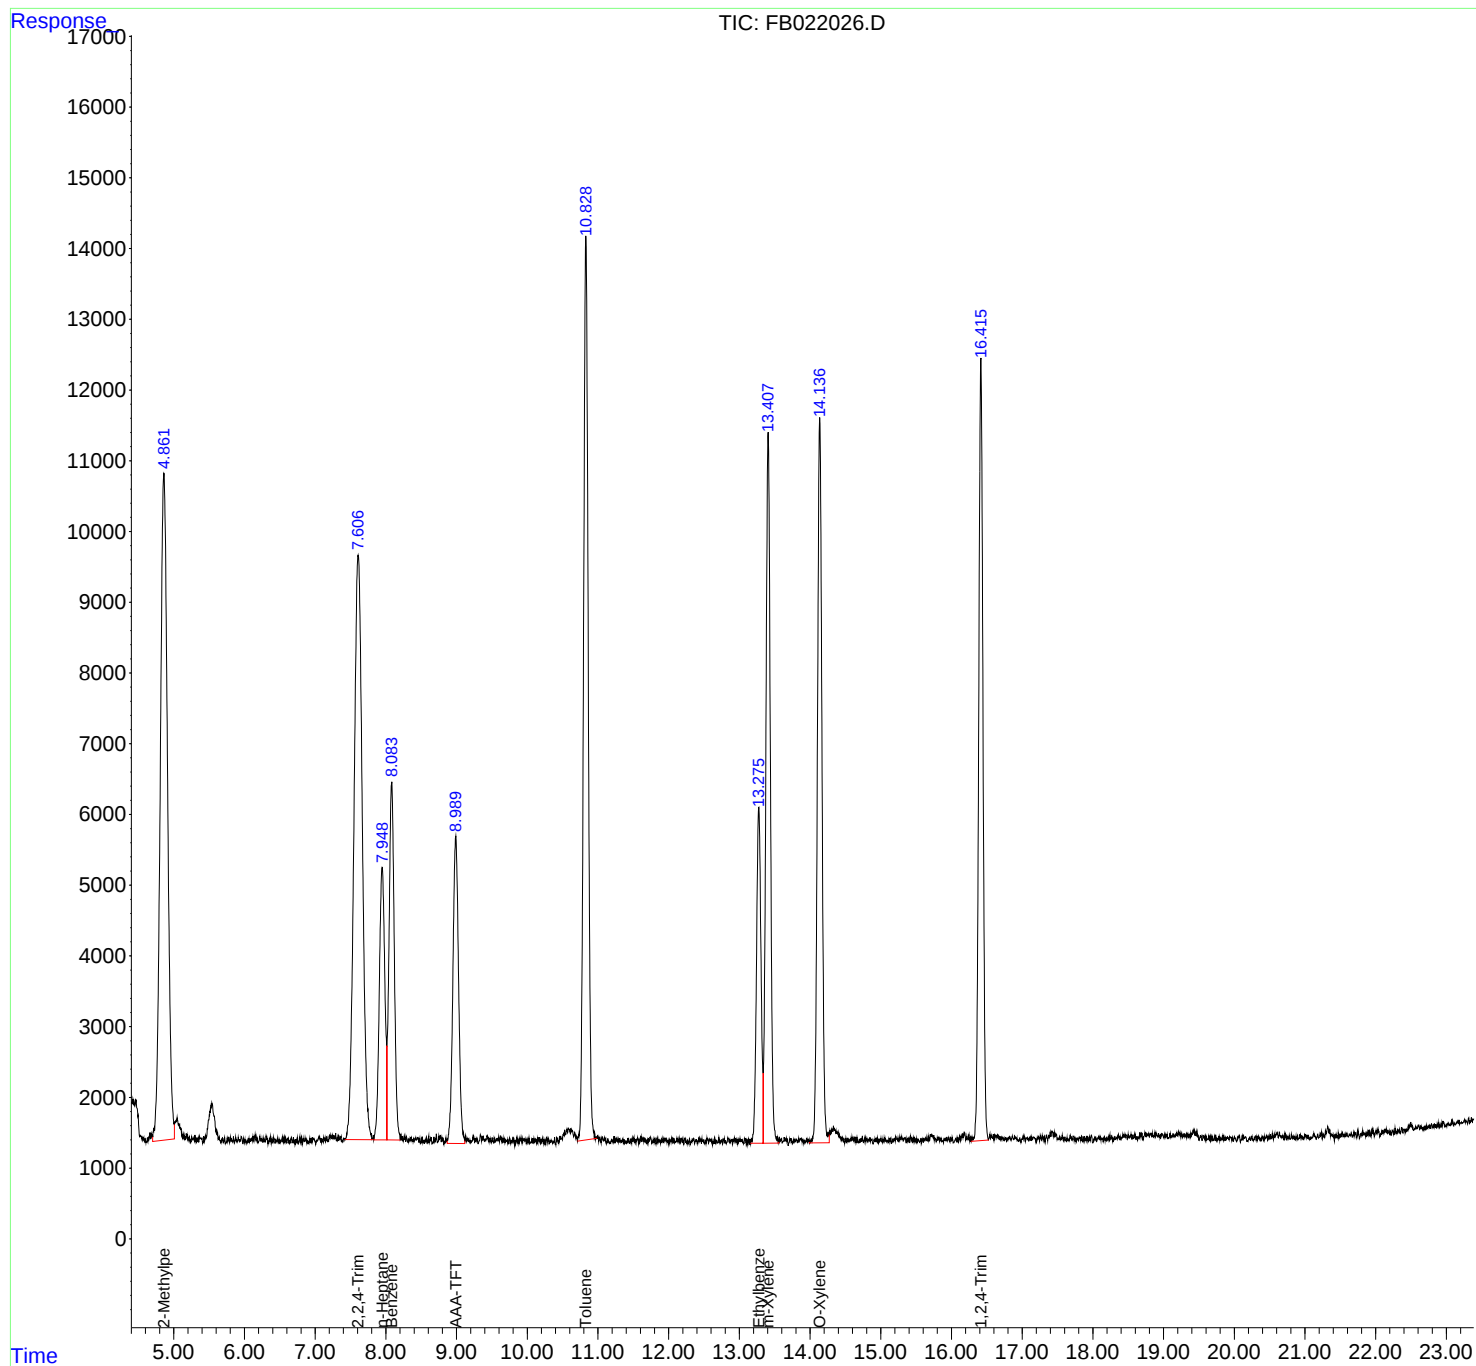

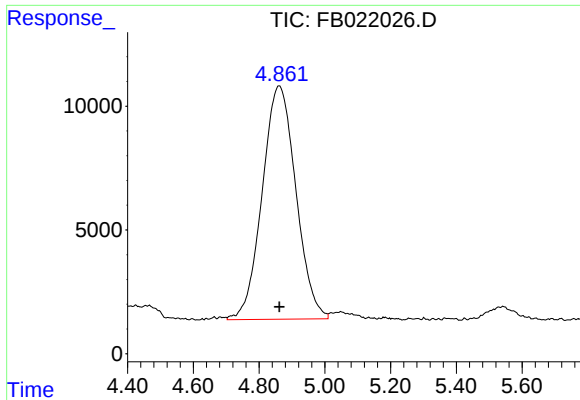


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 671198
Conc: 24.77 ng/ml

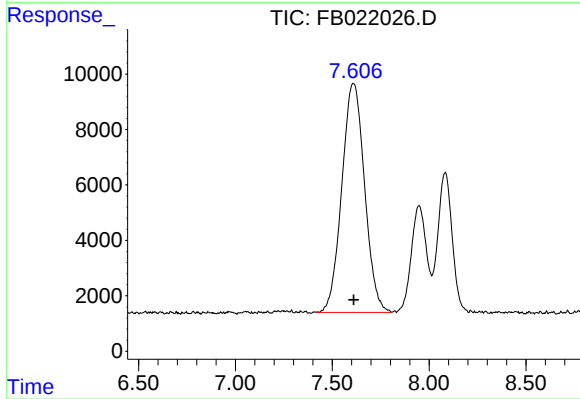


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: -0.003 min
Response: 675194
Conc: 25.31 ng/ml

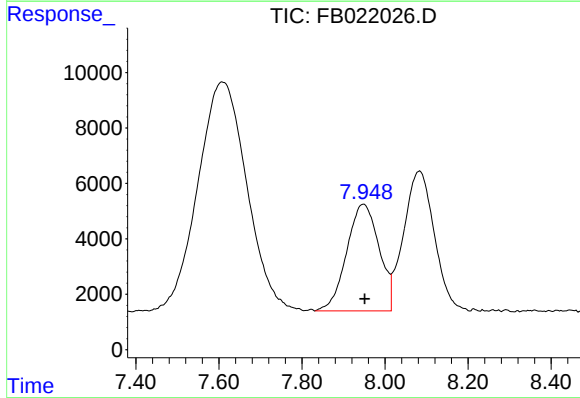


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.002 min
Response: 208767
Conc: 8.55 ng/ml

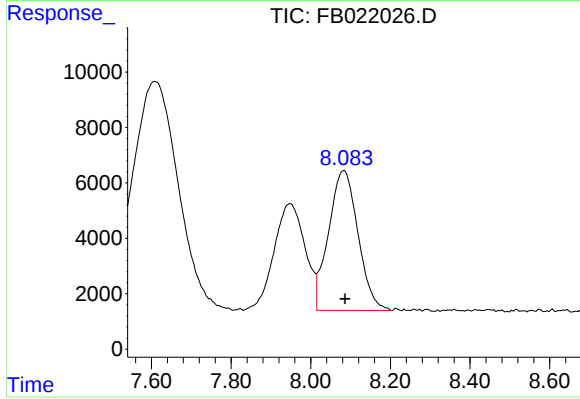


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.002 min
Response: 259698
Conc: 9.01 ng/ml

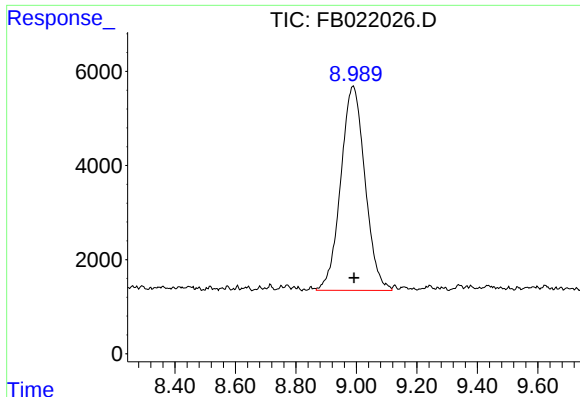


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.003 min
Response: 241122
Conc: 18.68 ng/ml

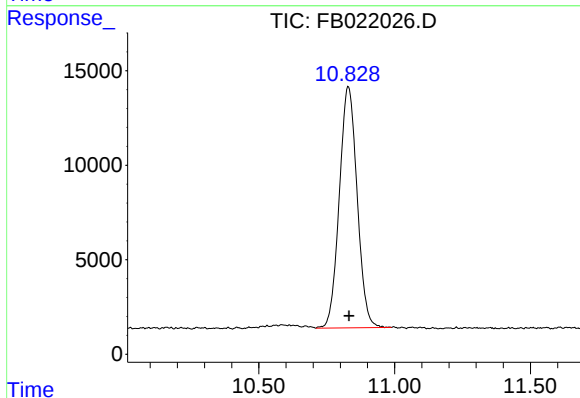


#6 Toluene

R.T.: 10.830 min
Delta R.T.: -0.003 min
Response: 581320
Conc: 29.29 ng/ml

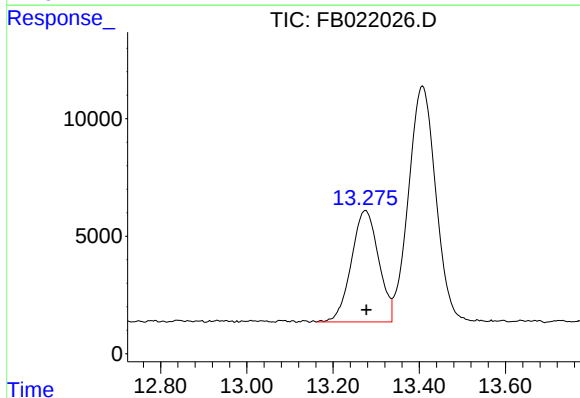


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.002 min
Response: 207528
Conc: 10.29 ng/ml

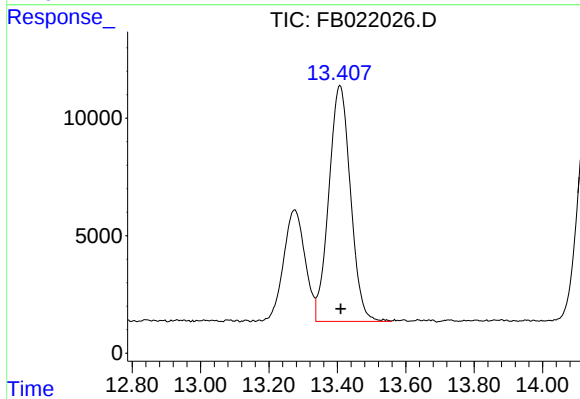


#8 m-Xylene

R.T.: 13.408 min
Delta R.T.: -0.002 min
Response: 442096
Conc: 20.42 ng/ml

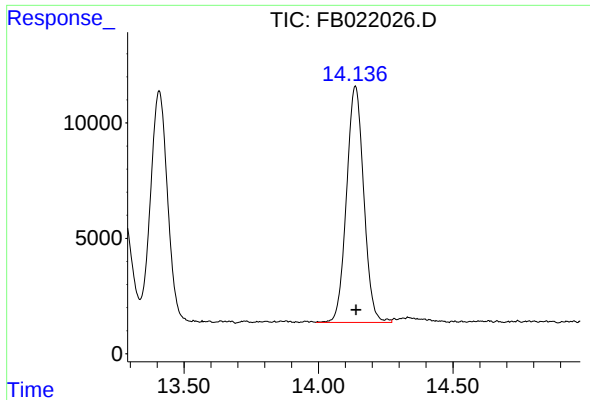

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.002 min
Response: 455321
Conc: 20.33 ng/ml

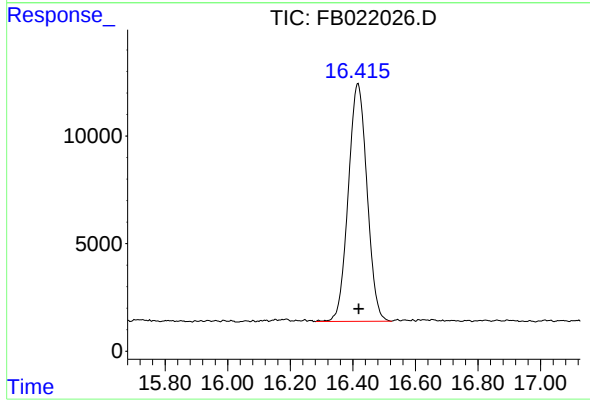

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: -0.002 min
Response: 459132
Conc: 19.54 ng/ml