

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
 Data File : FB022032.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2019 13:54
 Operator : DD/AJ
 Sample : K3616-16MSD
 Misc : 5.06/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 17 00:27:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
 Quant Title :
 QLast Update : Thu Aug 15 11:19:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.994	259193	20.075 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.866	576718	21.284 ng/ml
2) t	2,2,4-Trimethylpentane	7.614	491687	18.428 ng/ml
3) t	n-Heptane	7.952	119795	4.905 ng/ml
4) t	Benzene	8.089	267861	9.289 ng/ml
6) t	Toluene	10.835	530683	26.737 ng/ml
7) t	Ethylbenzene	13.280	165498	8.207 ng/ml
8) t	m-Xylene	13.412	341918	15.793 ng/ml
9) t	O-Xylene	14.142	363536	16.233 ng/ml
10) t	1,2,4-Trimethylbenzene	16.420	326999	13.919 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
Data File : FB022032.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2019 13:54
Operator : DD/AJ
Sample : K3616-16MSD
Misc : 5.06/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 00:27:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
Quant Title :
QLast Update : Thu Aug 15 11:19:59 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

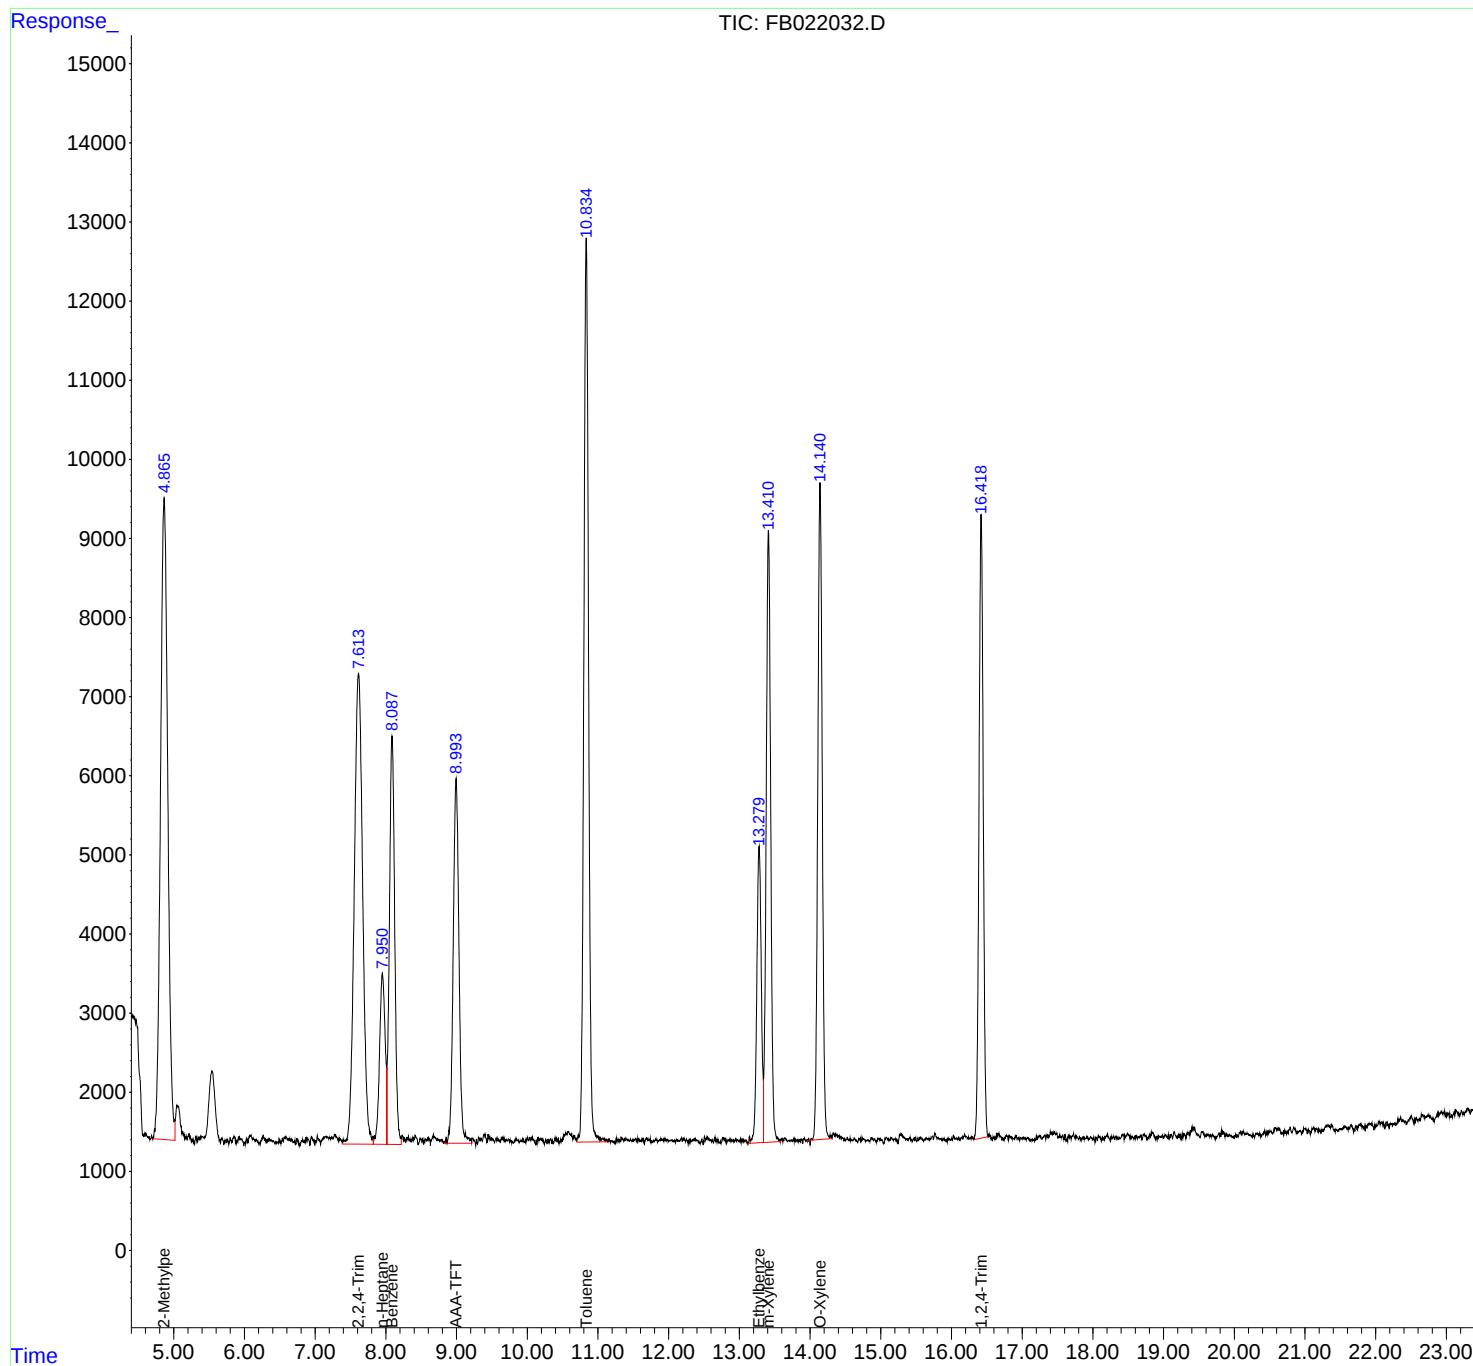

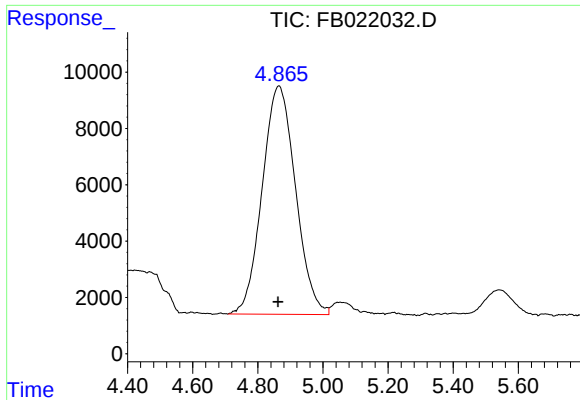


#1 2-Methylpentane

R.T.: 4.866 min
Delta R.T.: 0.004 min
Response: 576718
Conc: 21.28 ng/ml

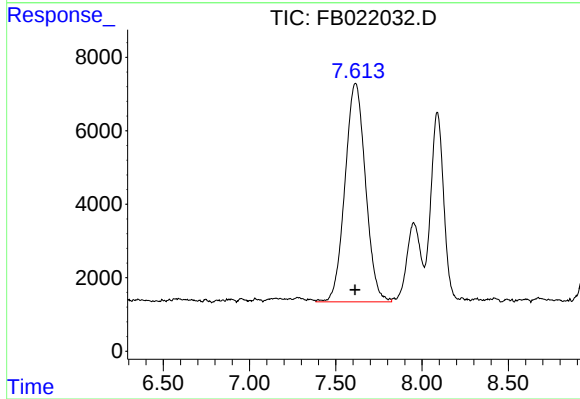


#2 2,2,4-Trimethylpentane

R.T.: 7.614 min
Delta R.T.: 0.003 min
Response: 491687
Conc: 18.43 ng/ml

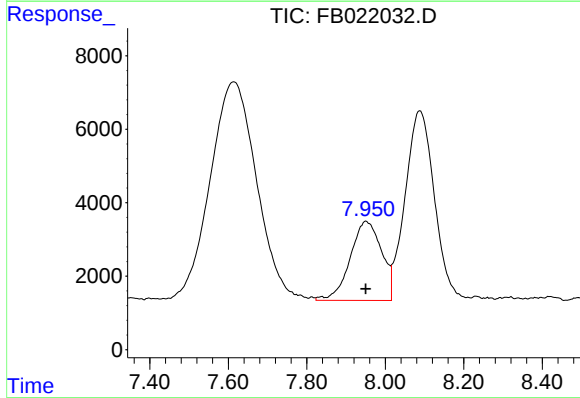


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.001 min
Response: 119795
Conc: 4.90 ng/ml

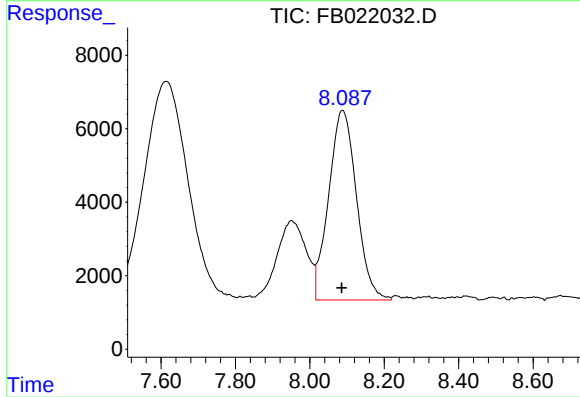


#4 Benzene

R.T.: 8.089 min
Delta R.T.: 0.003 min
Response: 267861
Conc: 9.29 ng/ml

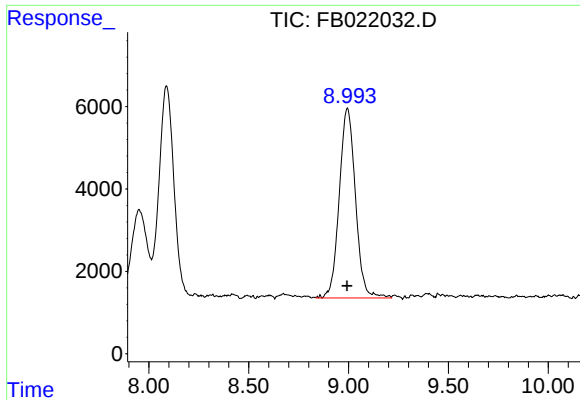


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 259193
Conc: 20.07 ng/ml

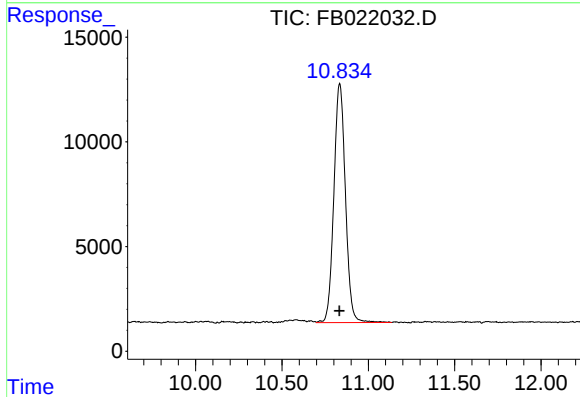


#6 Toluene

R.T.: 10.835 min
Delta R.T.: 0.002 min
Response: 530683
Conc: 26.74 ng/ml

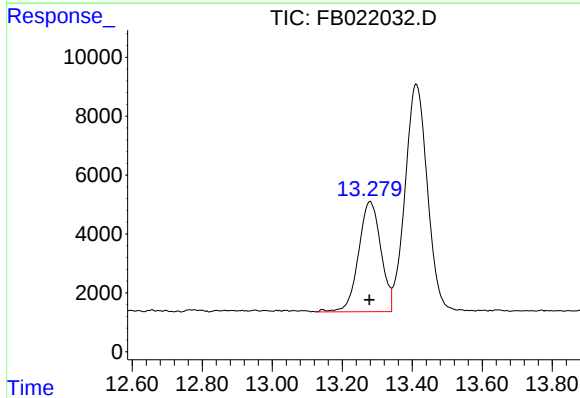


#7 Ethylbenzene

R.T.: 13.280 min
Delta R.T.: 0.002 min
Response: 165498
Conc: 8.21 ng/ml

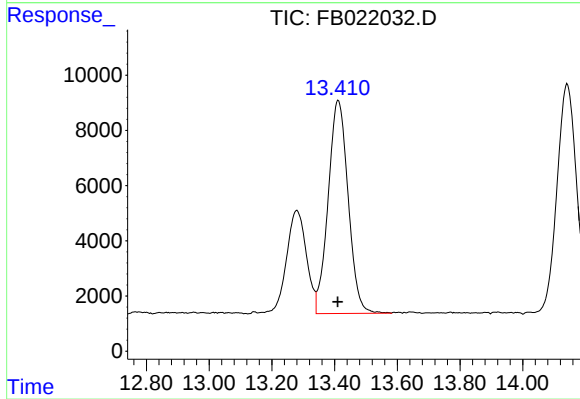


#8 m-Xylene

R.T.: 13.412 min
Delta R.T.: 0.002 min
Response: 341918
Conc: 15.79 ng/ml

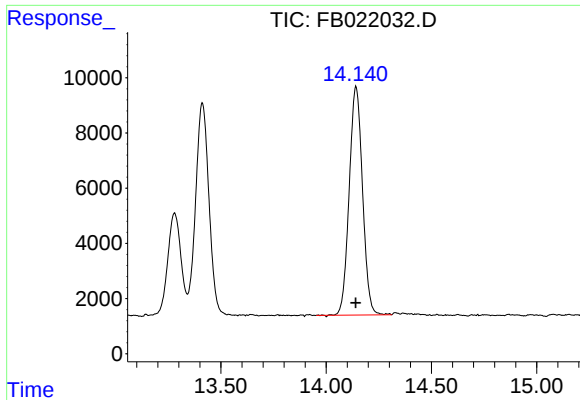

#9 O-Xylene

R.T.: 14.142 min
Delta R.T.: 0.002 min
Response: 363536
Conc: 16.23 ng/ml

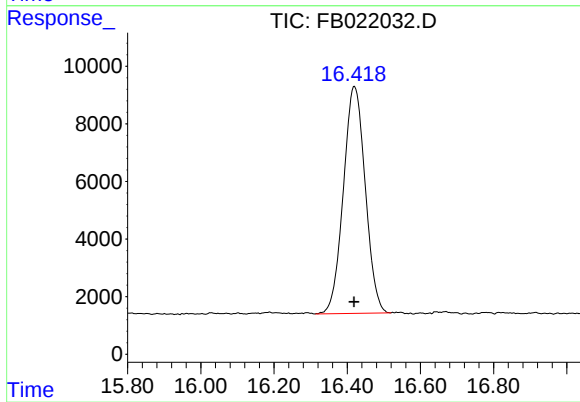

#10 1,2,4-Trimethylbenzene

R.T.: 16.420 min
Delta R.T.: 0.002 min
Response: 326999
Conc: 13.92 ng/ml