

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
 Data File : FB022033.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2019 14:25
 Operator : DD/AJ
 Sample : K4383-01
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 17 00:27:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
 Quant Title :
 QLast Update : Thu Aug 15 11:19:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.994	259896	20.129 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.855	3886	0.143 ng/ml
2) t	2,2,4-Trimethylpentane	7.608	6168	0.231 ng/ml
3) t	n-Heptane	7.954	4736	0.194 ng/ml
4) t	Benzene	8.055	4001	0.139 ng/ml
6) t	Toluene	10.852	4911	0.247 ng/ml
7) t	Ethylbenzene	13.272	6013	0.298 ng/ml
8) t	m-Xylene	13.413	6215	0.287 ng/ml
9) t	O-Xylene	14.154	11604	0.518 ng/ml
10) t	1,2,4-Trimethylbenzene	16.421	8947	0.381 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
Data File : FB022033.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2019 14:25
Operator : DD/AJ
Sample : K4383-01
Misc : 5.05/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 00:27:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
Quant Title :
QLast Update : Thu Aug 15 11:19:59 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

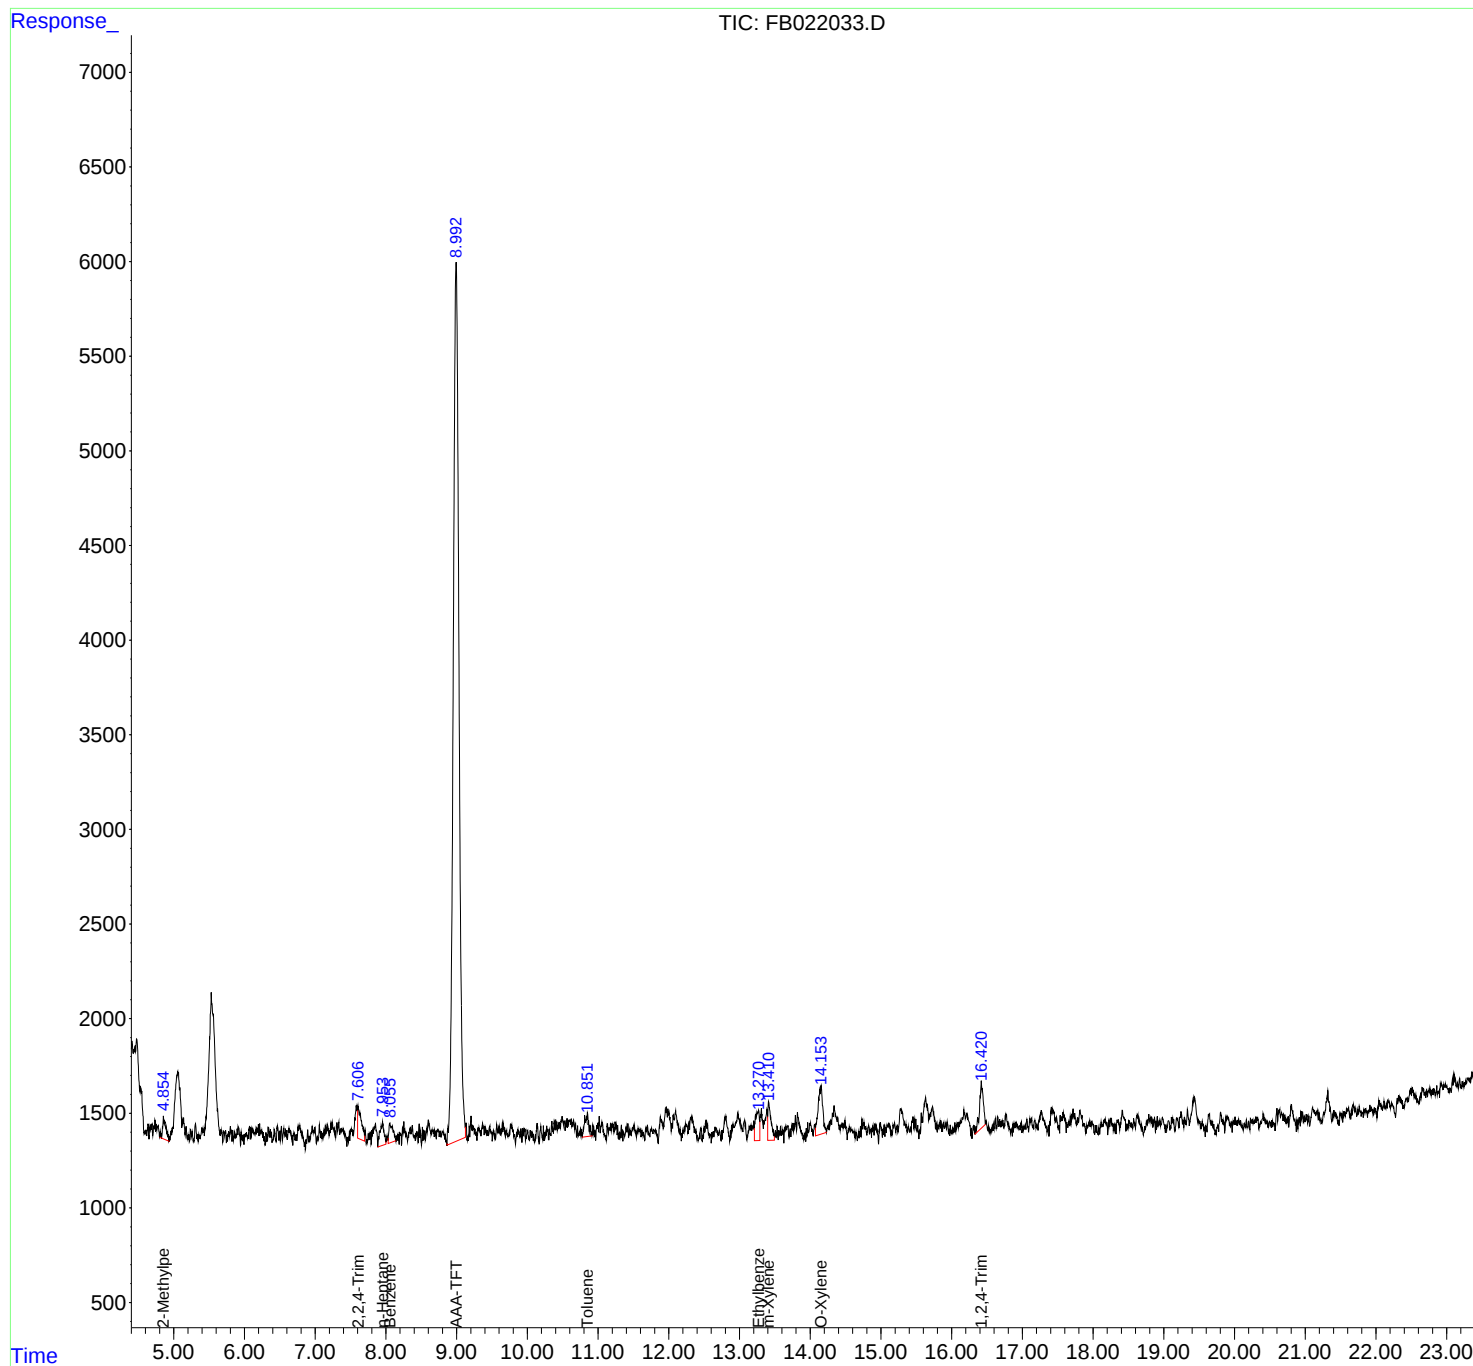

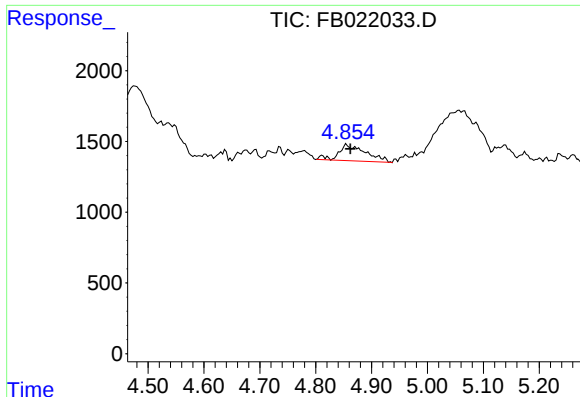


#1 2-Methylpentane

R.T.: 4.855 min
Delta R.T.: -0.007 min
Response: 3886
Conc: 0.14 ng/ml

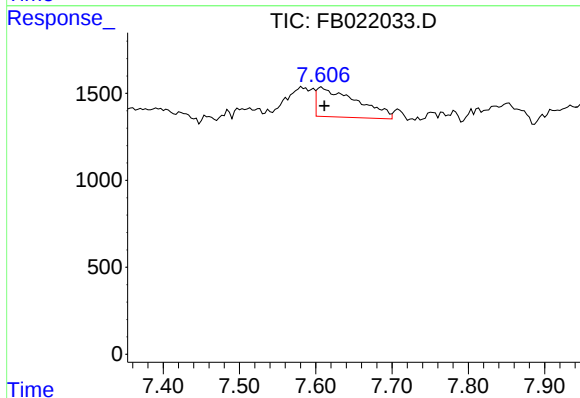


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: -0.003 min
Response: 6168
Conc: 0.23 ng/ml

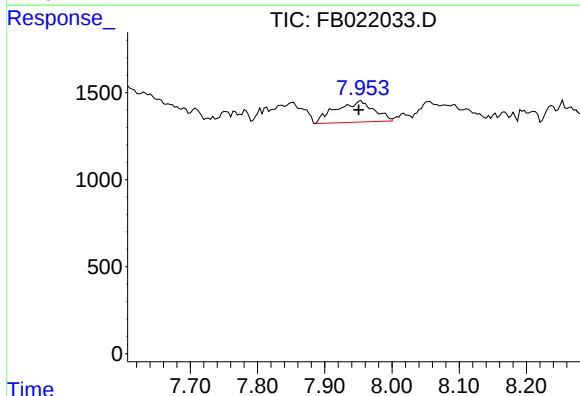


#3 n-Heptane

R.T.: 7.954 min
Delta R.T.: 0.003 min
Response: 4736
Conc: 0.19 ng/ml

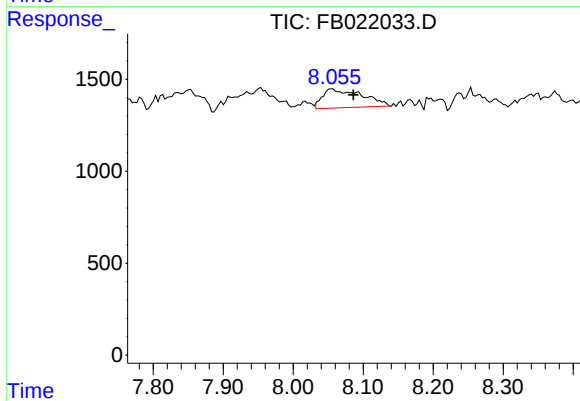


#4 Benzene

R.T.: 8.055 min
Delta R.T.: -0.030 min
Response: 4001
Conc: 0.14 ng/ml

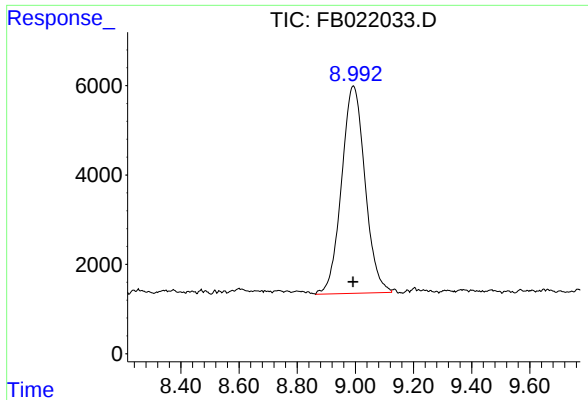


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 259896
Conc: 20.13 ng/ml

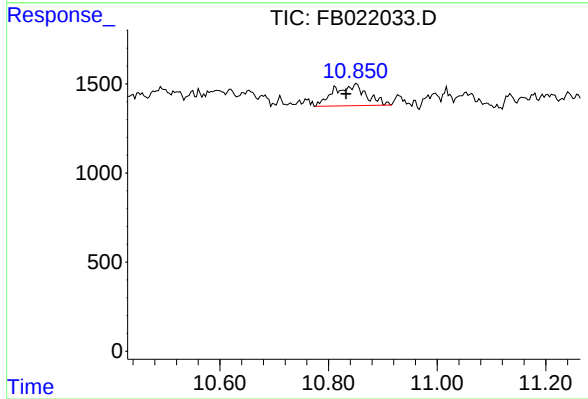


#6 Toluene

R.T.: 10.852 min
Delta R.T.: 0.020 min
Response: 4911
Conc: 0.25 ng/ml

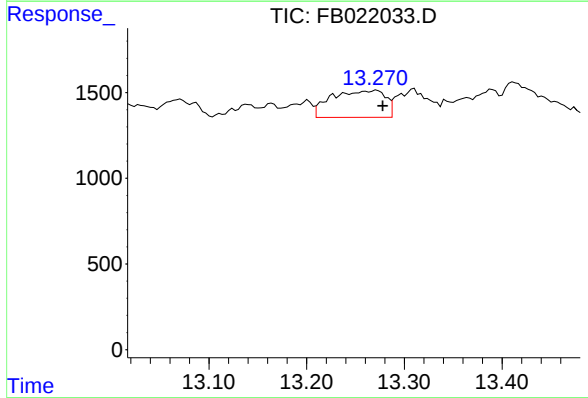


#7 Ethylbenzene

R.T.: 13.272 min
Delta R.T.: -0.006 min
Response: 6013
Conc: 0.30 ng/ml

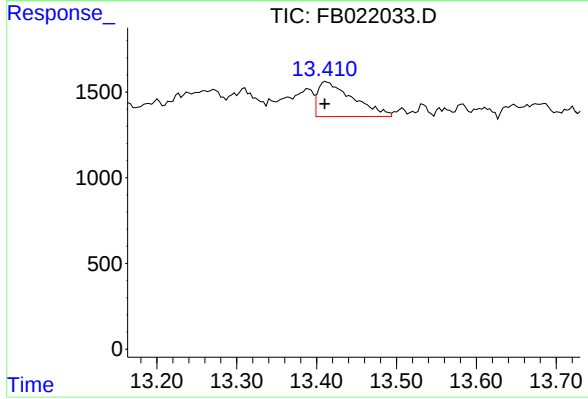


#8 m-Xylene

R.T.: 13.413 min
Delta R.T.: 0.002 min
Response: 6215
Conc: 0.29 ng/ml

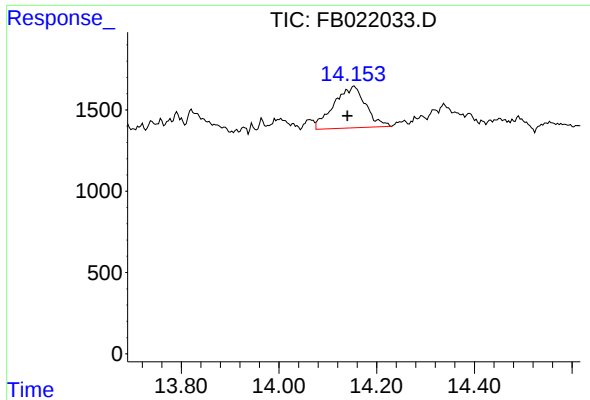

#9 O-Xylene

R.T.: 14.154 min
Delta R.T.: 0.014 min
Response: 11604
Conc: 0.52 ng/ml

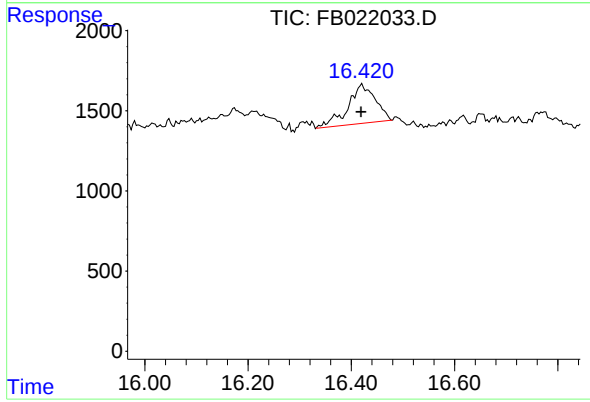

#10 1,2,4-Trimethylbenzene

R.T.: 16.421 min
Delta R.T.: 0.002 min
Response: 8947
Conc: 0.38 ng/ml