

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
 Data File : FB022037.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2019 16:28
 Operator : DD/AJ
 Sample : K4372-02
 Misc : 5.05/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 17 00:29:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
 Quant Title :
 QLast Update : Thu Aug 15 11:19:59 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	164239	12.720 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.862	2691	0.099 ng/ml
2) t	2,2,4-Trimethylpentane	7.643	3132	0.117 ng/ml
3) t	n-Heptane	7.922	1915	0.078 ng/ml
4) t	Benzene	8.088	4311	0.150 ng/ml
6) t	Toluene	10.835	38818	1.956 ng/ml
7) t	Ethylbenzene	13.276	107649	5.338 ng/ml
8) t	m-Xylene	13.407	116694	5.390 ng/ml
9) t	O-Xylene	14.142	103820	4.636 ng/ml
10) t	1,2,4-Trimethylbenzene	16.425	26216	1.116 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
Data File : FB022037.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2019 16:28
Operator : DD/AJ
Sample : K4372-02
Misc : 5.05/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 00:29:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
Quant Title :
QLast Update : Thu Aug 15 11:19:59 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

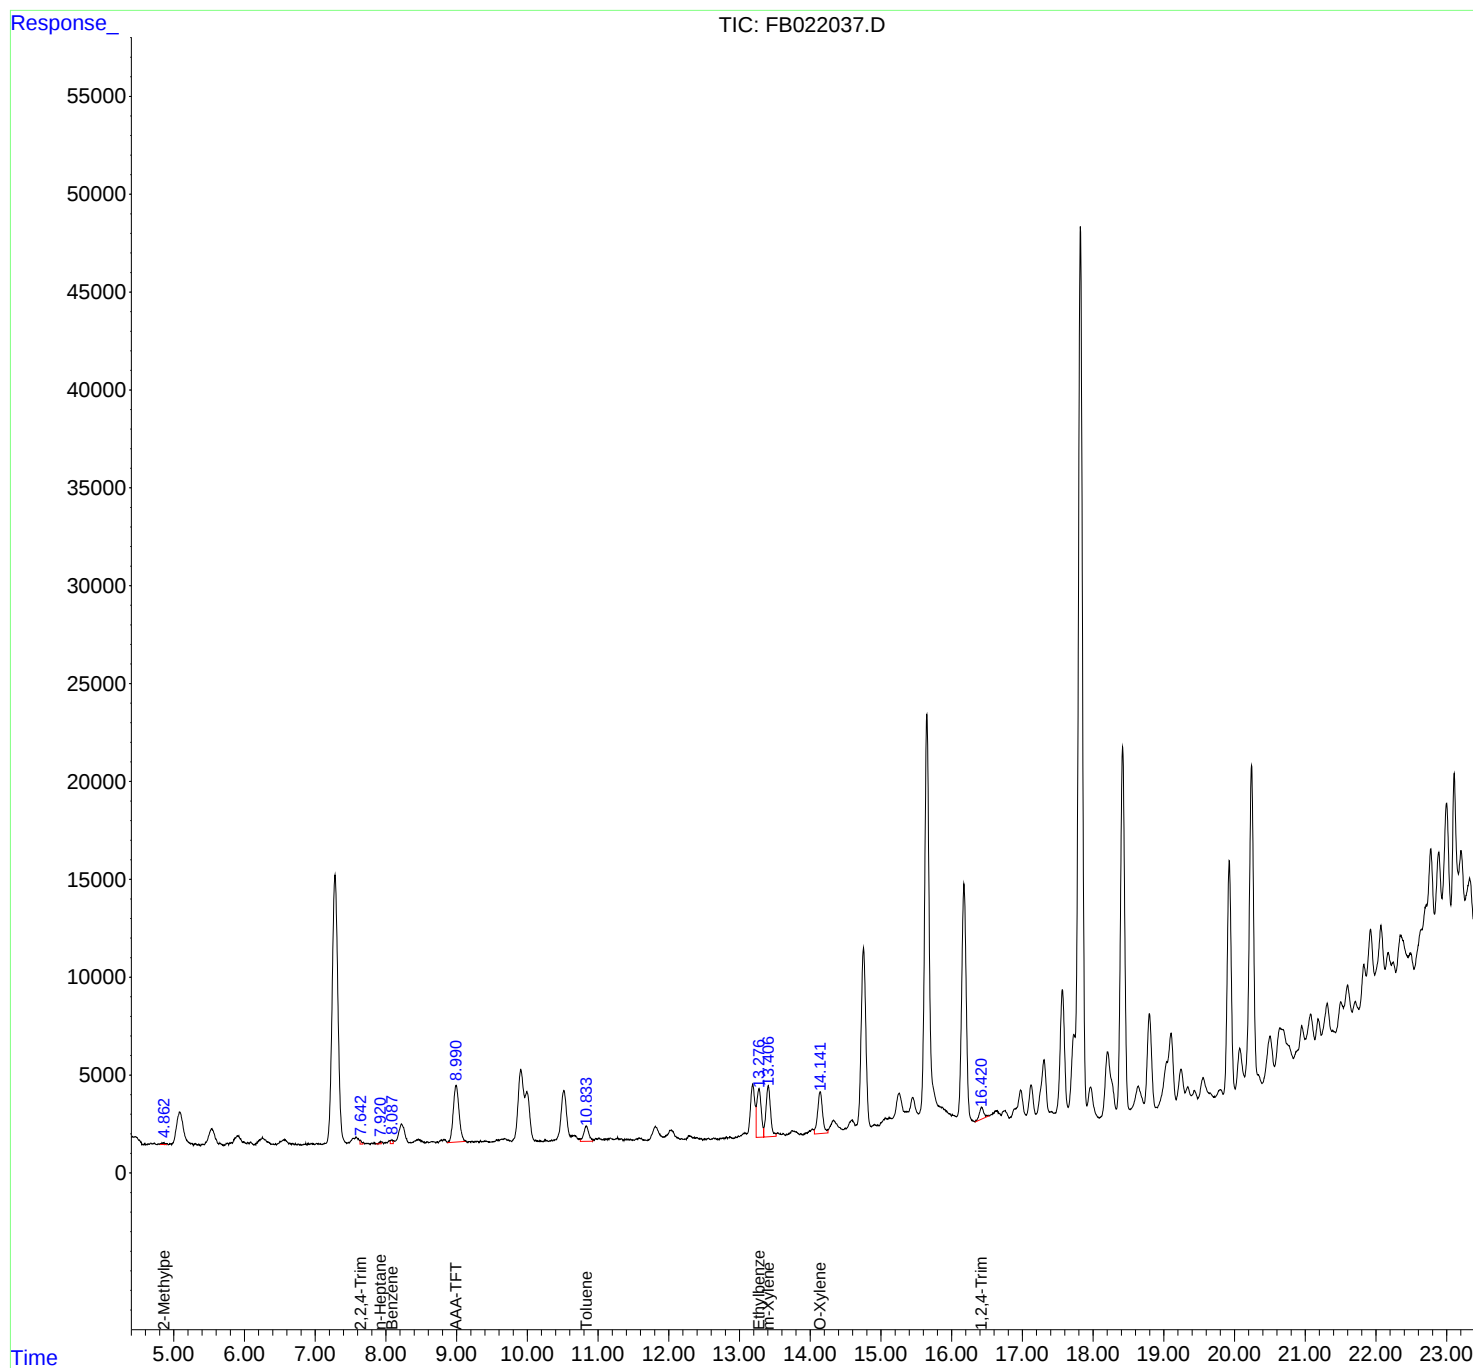

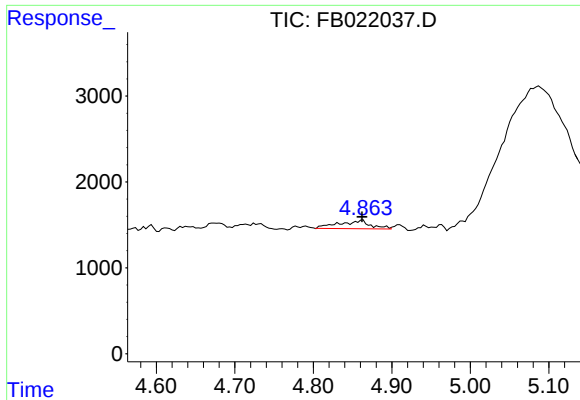


#1 2-Methylpentane

R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 2691
Conc: 0.10 ng/ml

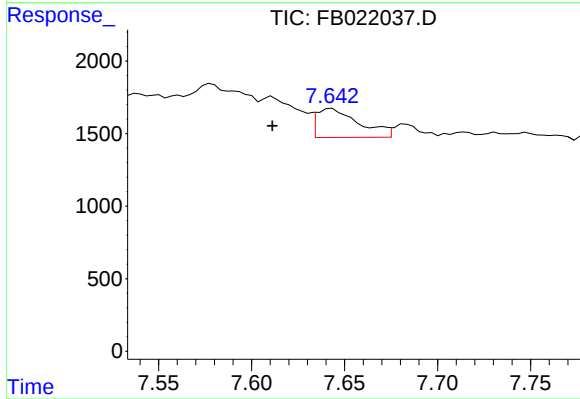


#2 2,2,4-Trimethylpentane

R.T.: 7.643 min
Delta R.T.: 0.032 min
Response: 3132
Conc: 0.12 ng/ml

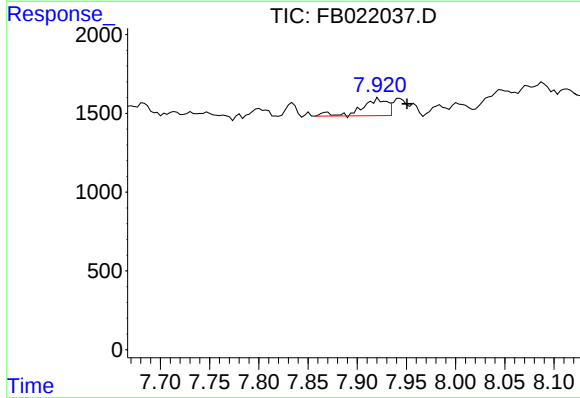


#3 n-Heptane

R.T.: 7.922 min
Delta R.T.: -0.029 min
Response: 1915
Conc: 0.08 ng/ml

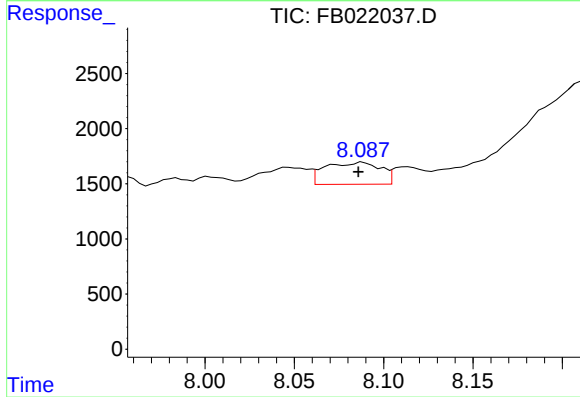


#4 Benzene

R.T.: 8.088 min
Delta R.T.: 0.003 min
Response: 4311
Conc: 0.15 ng/ml

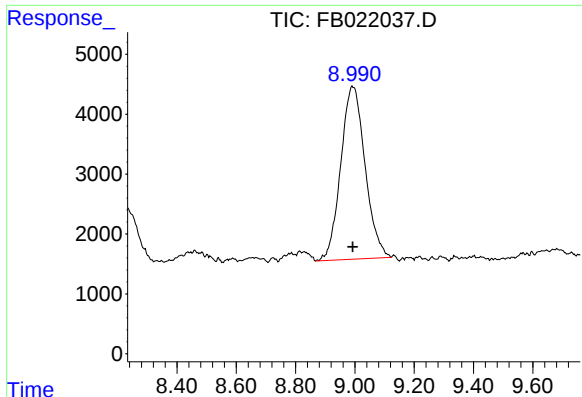


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 164239
Conc: 12.72 ng/ml

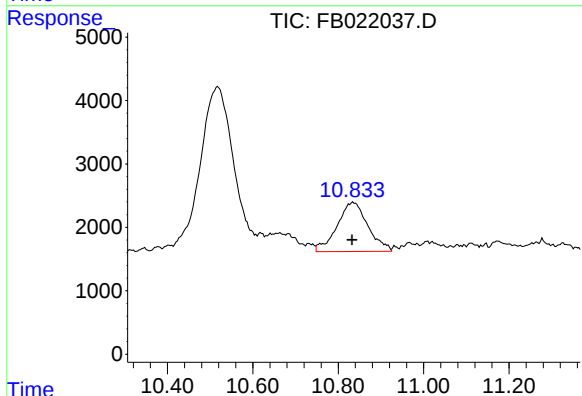


#6 Toluene

R.T.: 10.835 min
Delta R.T.: 0.003 min
Response: 38818
Conc: 1.96 ng/ml

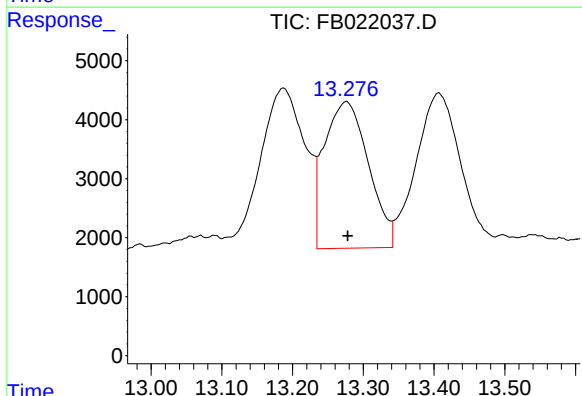


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.001 min
Response: 107649
Conc: 5.34 ng/ml

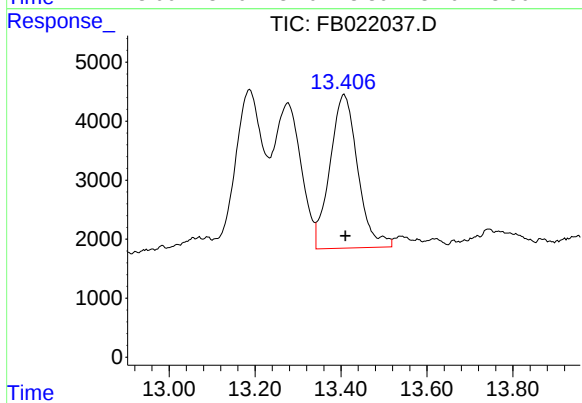


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: -0.003 min
Response: 116694
Conc: 5.39 ng/ml

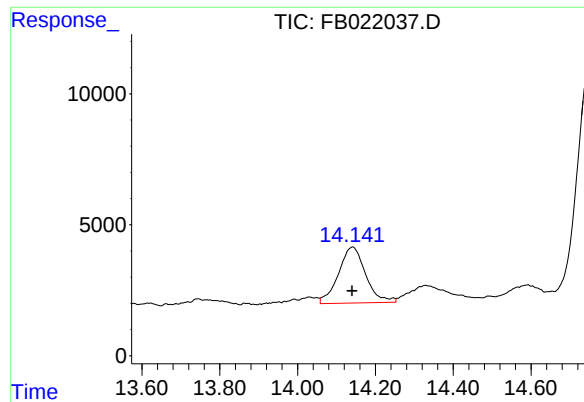

#9 O-Xylene

R.T.: 14.142 min
Delta R.T.: 0.002 min
Response: 103820
Conc: 4.64 ng/ml

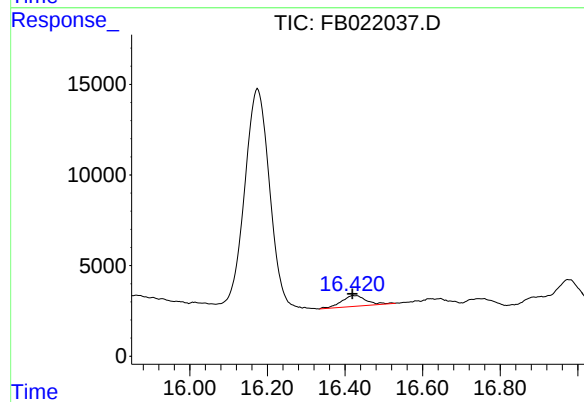

#10 1,2,4-Trimethylbenzene

R.T.: 16.425 min
Delta R.T.: 0.006 min
Response: 26216
Conc: 1.12 ng/ml