

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
Data File : FB022027.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2019 11:21
Operator : DD/AJ
Sample : K4090-10
Misc : 5.04/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 00:26:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
Quant Title :
QLast Update : Thu Aug 15 11:19:59 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	283957	21.993 ng/ml
Target Compounds			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081619\
Data File : FB022027.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2019 11:21
Operator : DD/AJ
Sample : K4090-10
Misc : 5.04/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 00:26:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081519.M
Quant Title :
QLast Update : Thu Aug 15 11:19:59 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

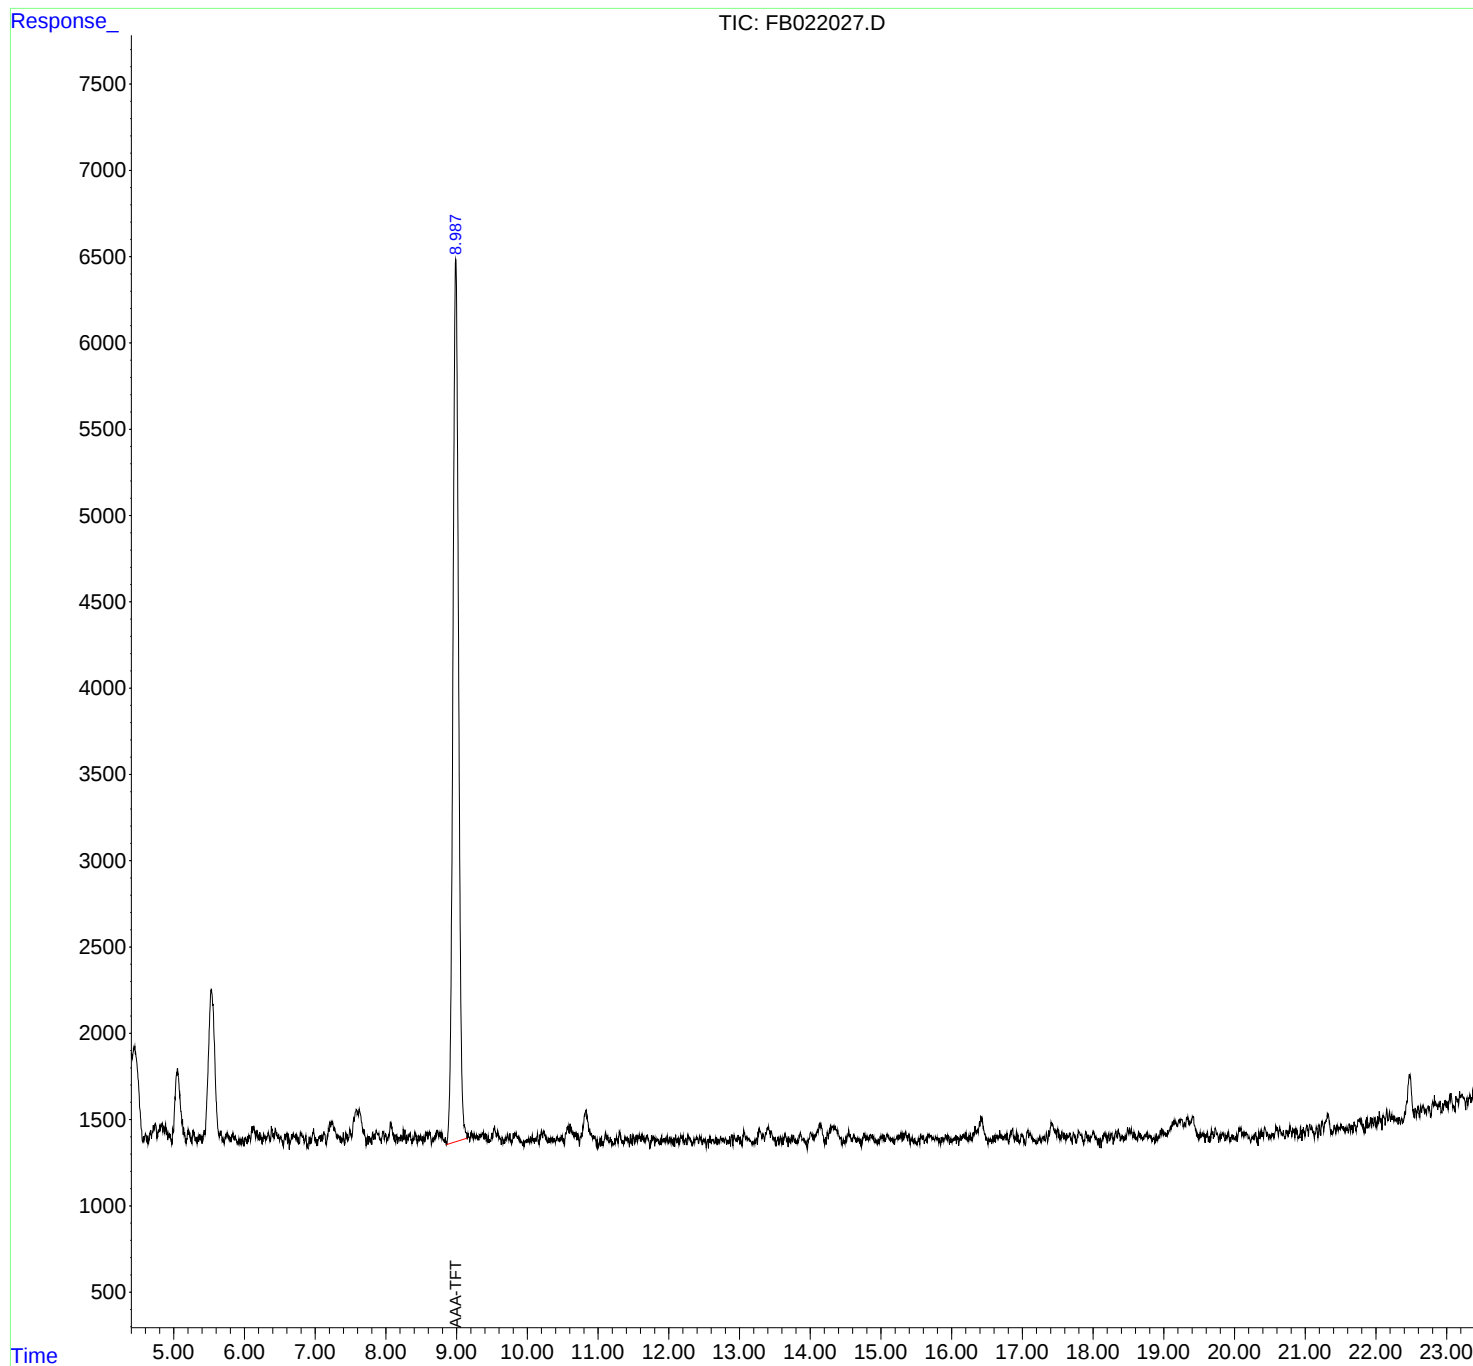

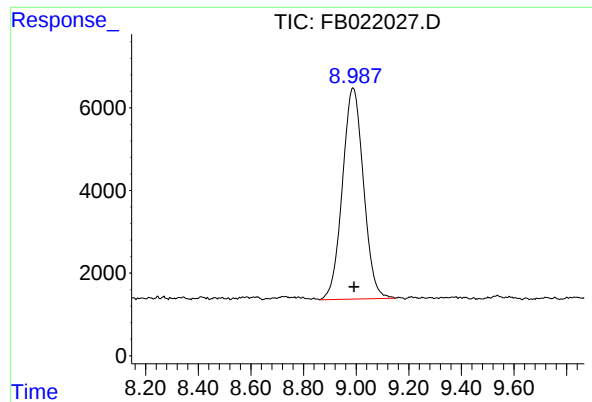

#5 AAA-TFT

R.T.: 8.989 min

Delta R.T.: -0.004 min

Response: 283957

Conc: 21.99 ng/ml