

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081621\
 Data File : FB026179.D
 Signal(s) : FID2B.CH
 Acq On : 16 Aug 2021 10:46
 Operator : AJ/MA
 Sample : BSF0816S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 17 02:48:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
 Quant Title :
 QLast Update : Fri Aug 13 22:11:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.834	261988	17.581 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.825	618069	27.377 ng/ml
2) t 2,2,4-Trimethylpentane	7.492	656664	29.870 ng/ml
3) t n-Heptane	7.809	253211	8.405 ng/ml
4) t Benzene	7.946	260030	8.229 ng/ml
6) t Toluene	10.646	757935	26.330 ng/ml
7) t Ethylbenzene	13.067	222248	9.206 ng/ml
8) t m-Xylene	13.200	441479	18.890 ng/ml
9) t O-Xylene	13.924	415348	19.964 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	444102	22.014 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081621\
Data File : FB026179.D
Signal(s) : FID2B.CH
Acq On : 16 Aug 2021 10:46
Operator : AJ/MA
Sample : BSF0816S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 02:48:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:11:30 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

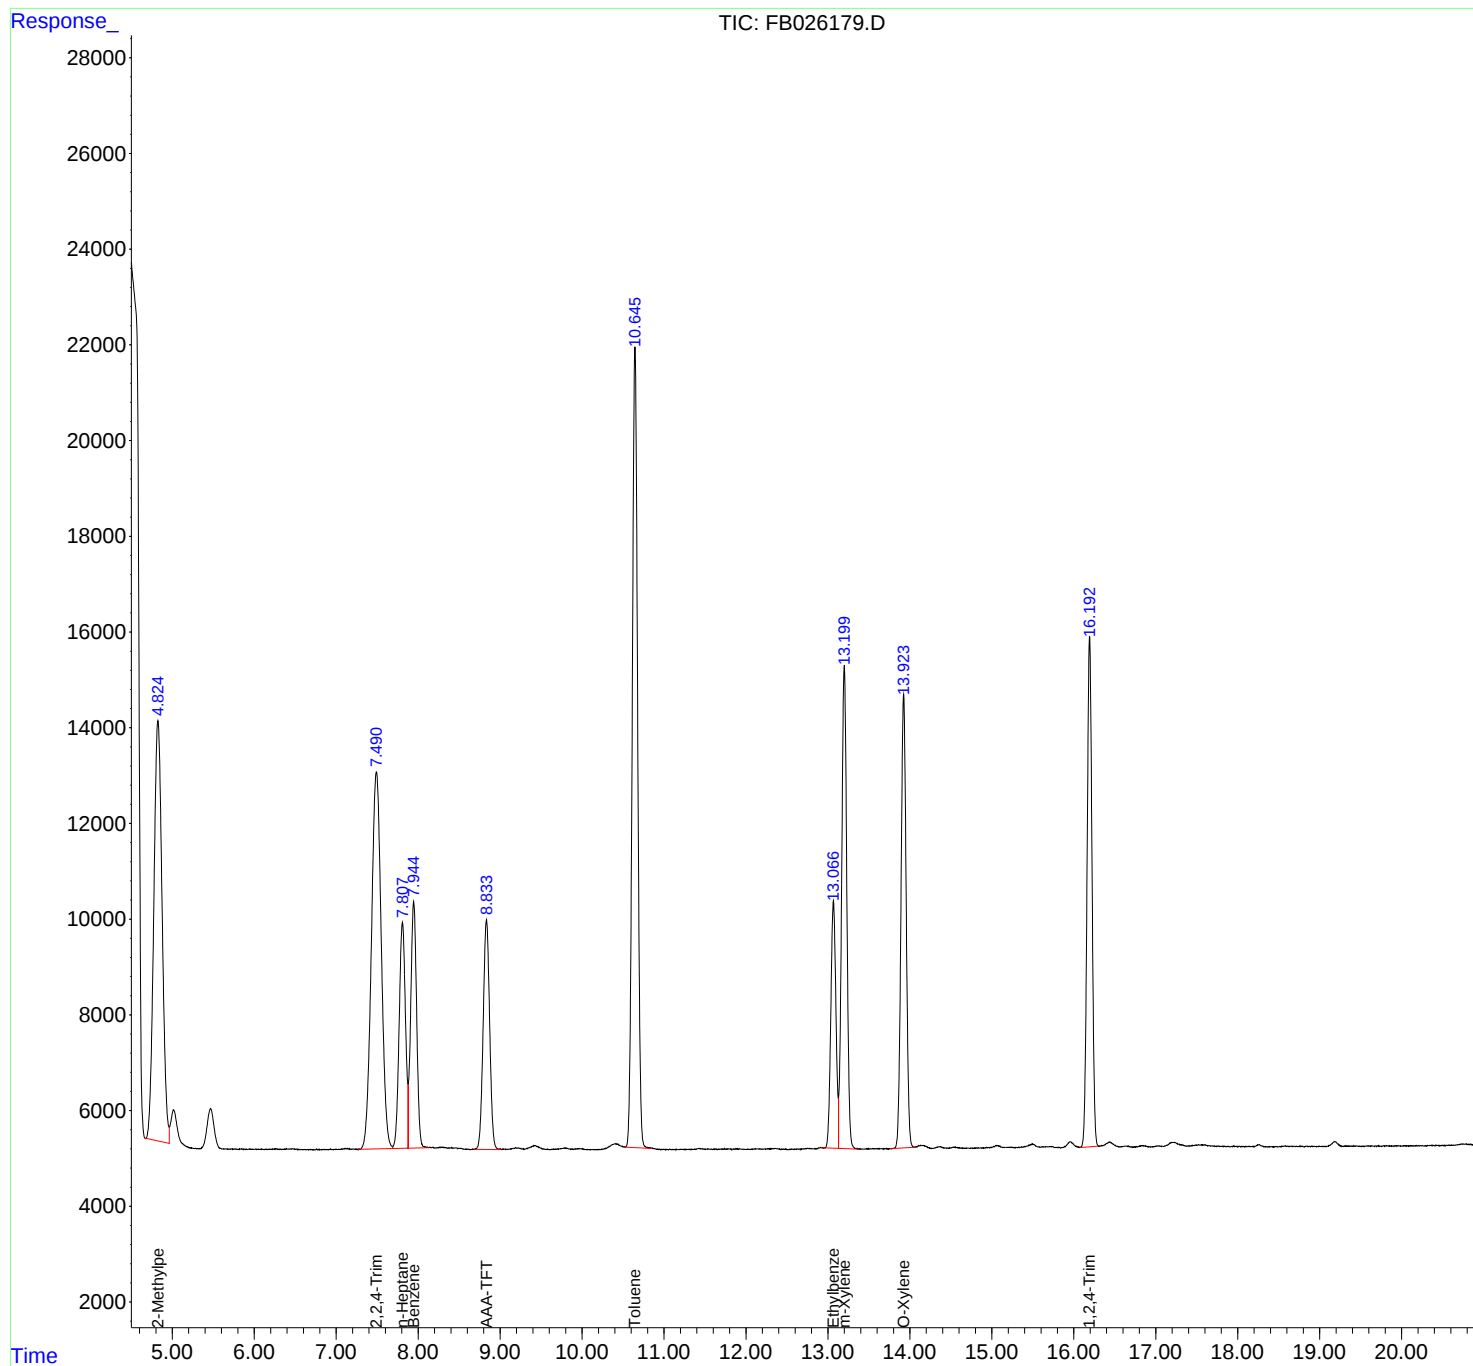

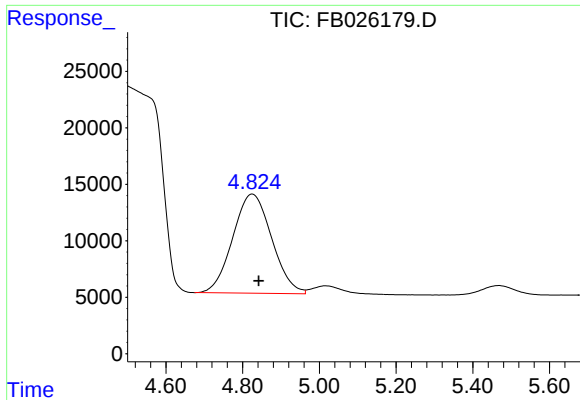


#1 2-Methylpentane

R.T.: 4.825 min
Delta R.T.: -0.017 min
Response: 618069
Conc: 27.38 ng/ml

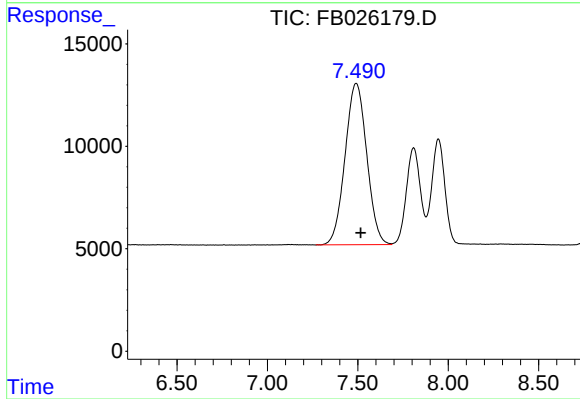


#2 2,2,4-Trimethylpentane

R.T.: 7.492 min
Delta R.T.: -0.024 min
Response: 656664
Conc: 29.87 ng/ml

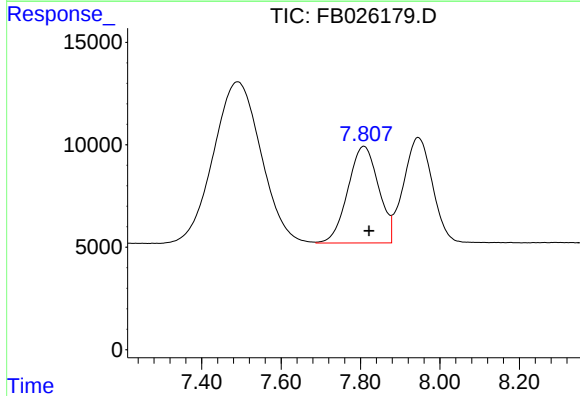


#3 n-Heptane

R.T.: 7.809 min
Delta R.T.: -0.013 min
Response: 253211
Conc: 8.41 ng/ml

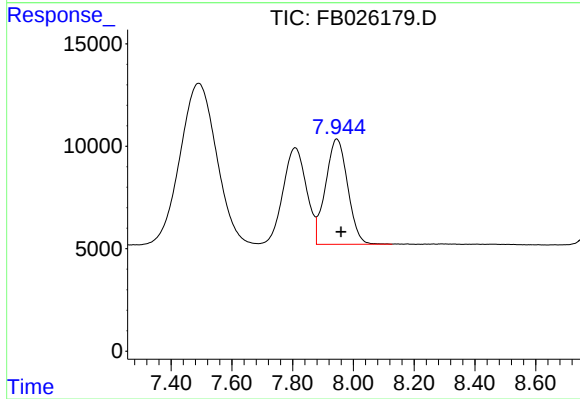


#4 Benzene

R.T.: 7.946 min
Delta R.T.: -0.015 min
Response: 260030
Conc: 8.23 ng/ml

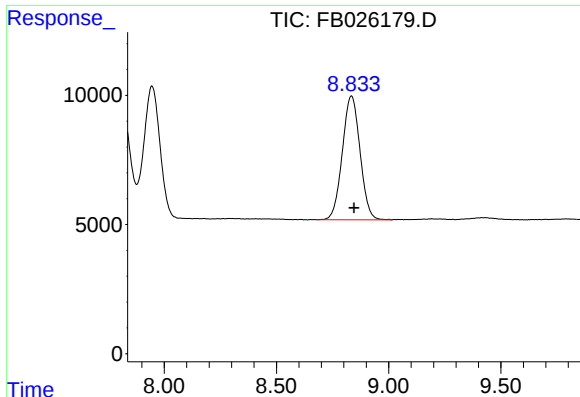


#5 AAA-TFT

R.T.: 8.834 min
Delta R.T.: -0.013 min
Response: 261988
Conc: 17.58 ng/ml

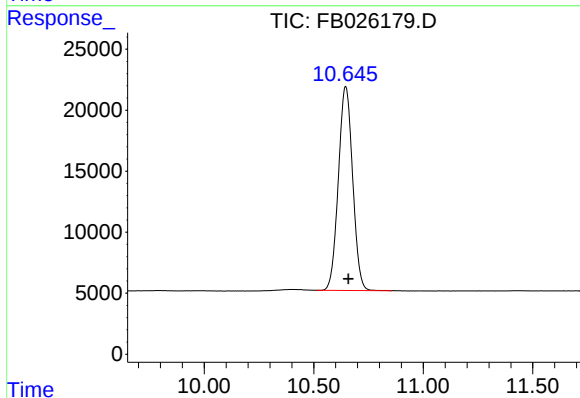


#6 Toluene

R.T.: 10.646 min
Delta R.T.: -0.012 min
Response: 757935
Conc: 26.33 ng/ml

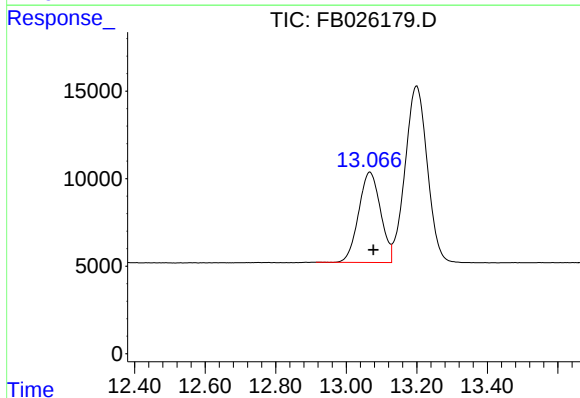


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.009 min
Response: 222248
Conc: 9.21 ng/ml

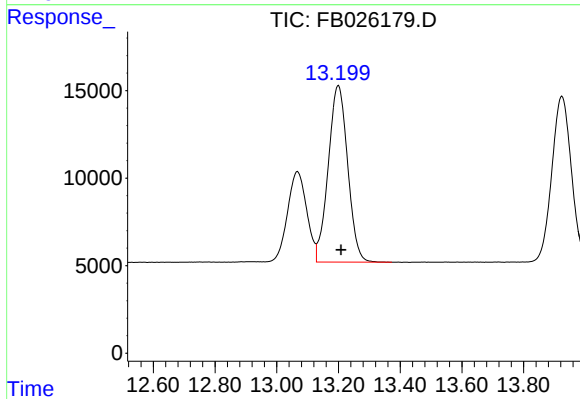

#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.010 min
Response: 441479
Conc: 18.89 ng/ml

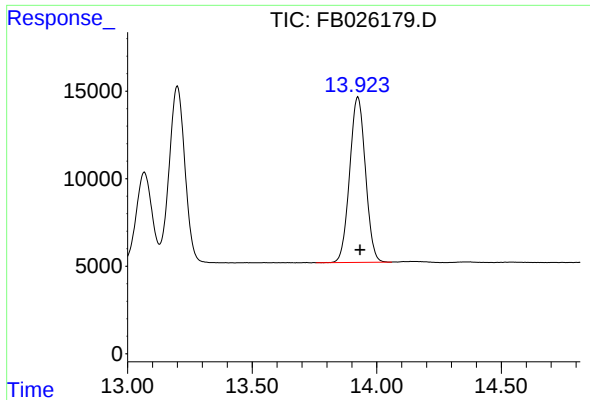


#9 O-Xylene

R.T.: 13.924 min

Delta R.T.: -0.009 min

Response: 415348

Conc: 19.96 ng/ml

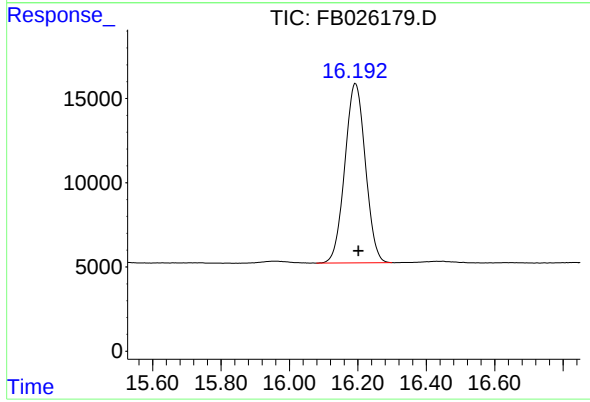

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min

Delta R.T.: -0.009 min

Response: 444102

Conc: 22.01 ng/ml