

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081718\
 Data File : FB017441.D
 Signal(s) : FID2B.CH
 Acq On : 17 Aug 2018 9:09
 Operator : MJ/SJ
 Sample : BSF0817S1
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 17 11:32:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080818.M
 Quant Title :
 QLast Update : Wed Aug 08 11:39:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	200705	21.421 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.964	448742	26.243 ng/ml
2) t 2,2,4-Trimethylpentane	7.730	458129	27.114 ng/ml
3) t n-Heptane	8.066	142721	8.859 ng/ml
4) t Benzene	8.206	184527	9.106 ng/ml
6) t Toluene	10.961	468807	28.441 ng/ml
7) t Ethylbenzene	13.410	156546	9.383 ng/ml
8) t m-Xylene	13.543	332479	17.736 ng/ml
9) t O-Xylene	14.275	353067	17.372 ng/ml
10) t 1,2,4-Trimethylbenzene	16.557	405542	18.108 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081718\
Data File : FB017441.D
Signal(s) : FID2B.CH
Acq On : 17 Aug 2018 9:09
Operator : MJ/SJ
Sample : BSF0817S1
Misc : 5.00g/5.00mL DI Water
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 11:32:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080818.M
Quant Title :
QLast Update : Wed Aug 08 11:39:03 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

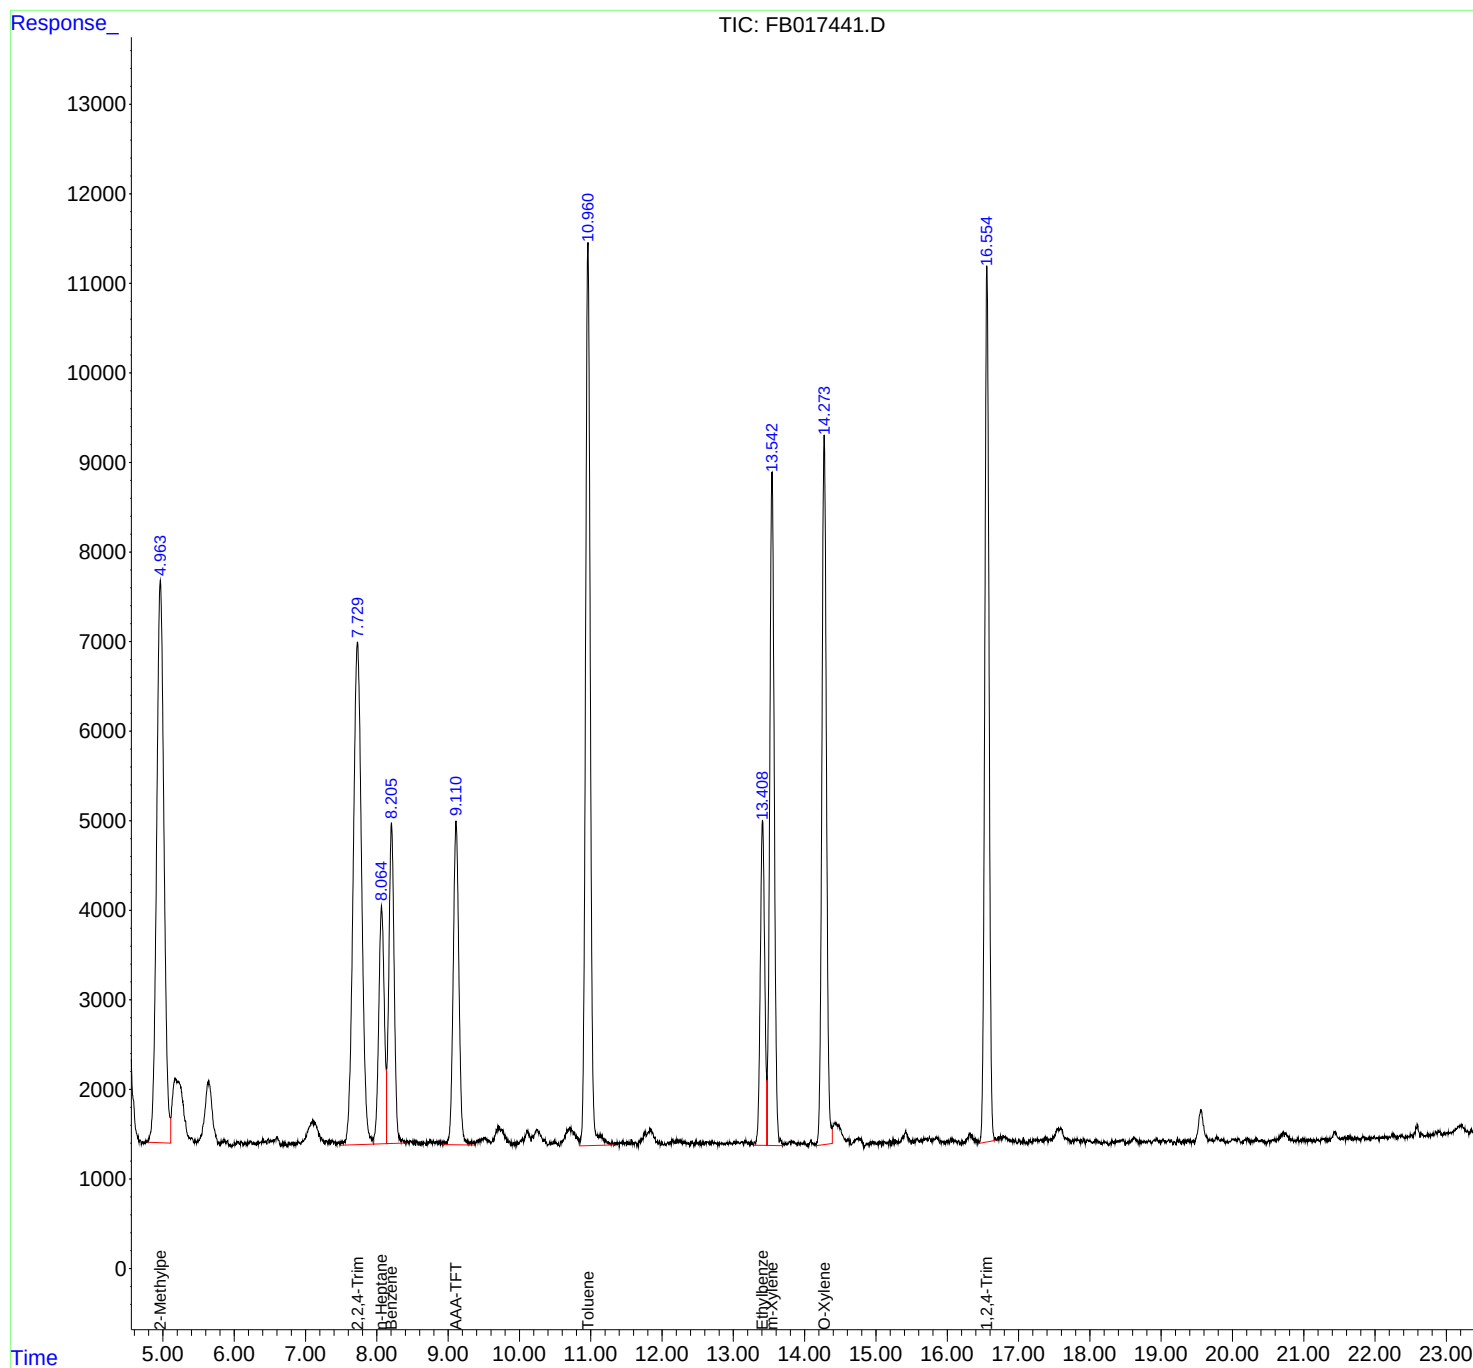

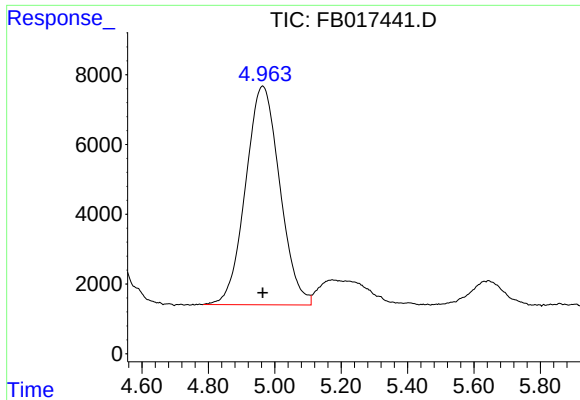


#1 2-Methylpentane

R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 448742
Conc: 26.24 ng/ml

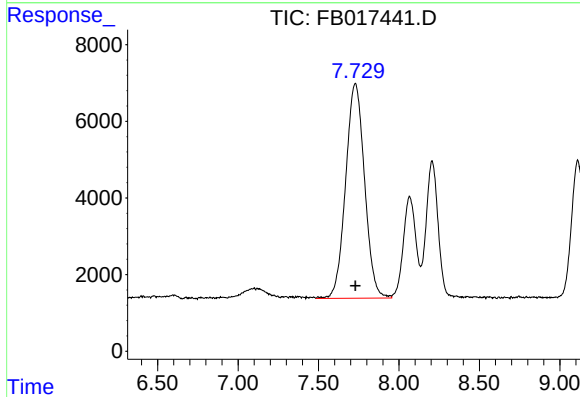


#2 2,2,4-Trimethylpentane

R.T.: 7.730 min
Delta R.T.: 0.000 min
Response: 458129
Conc: 27.11 ng/ml

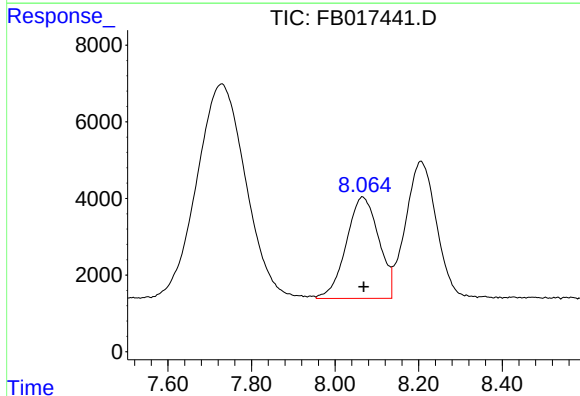


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 142721
Conc: 8.86 ng/ml

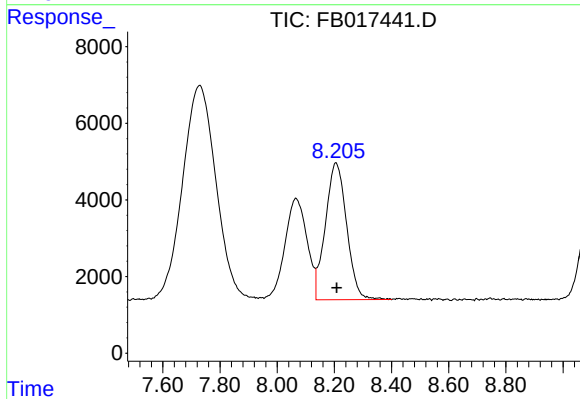


#4 Benzene

R.T.: 8.206 min
Delta R.T.: -0.002 min
Response: 184527
Conc: 9.11 ng/ml

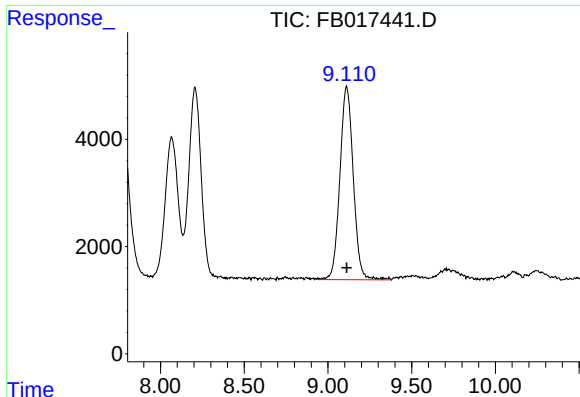


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: -0.001 min
Response: 200705
Conc: 21.42 ng/ml

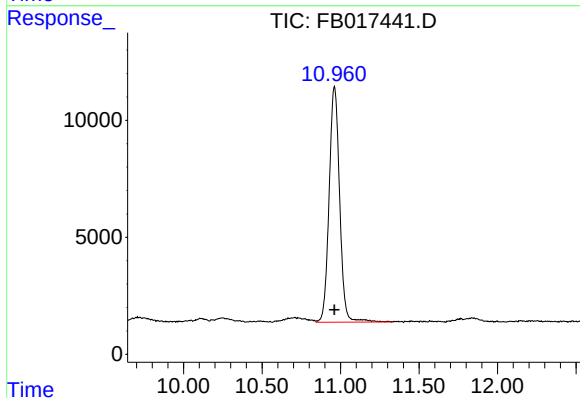


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.000 min
Response: 468807
Conc: 28.44 ng/ml

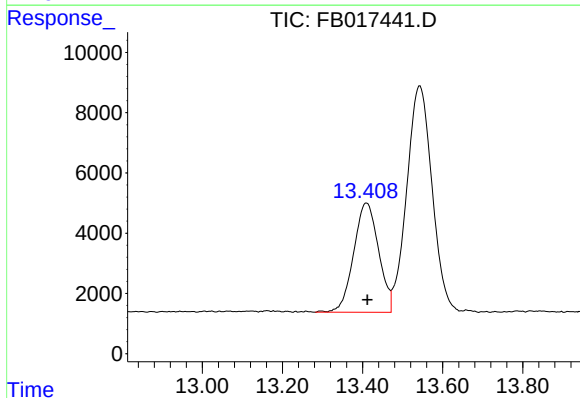


#7 Ethylbenzene

R.T.: 13.410 min
Delta R.T.: -0.002 min
Response: 156546
Conc: 9.38 ng/ml

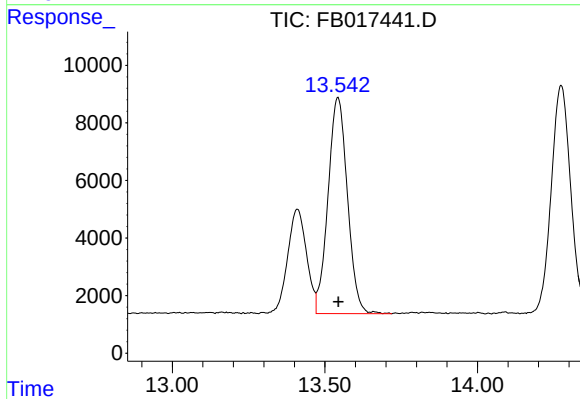


#8 m-Xylene

R.T.: 13.543 min
Delta R.T.: -0.001 min
Response: 332479
Conc: 17.74 ng/ml

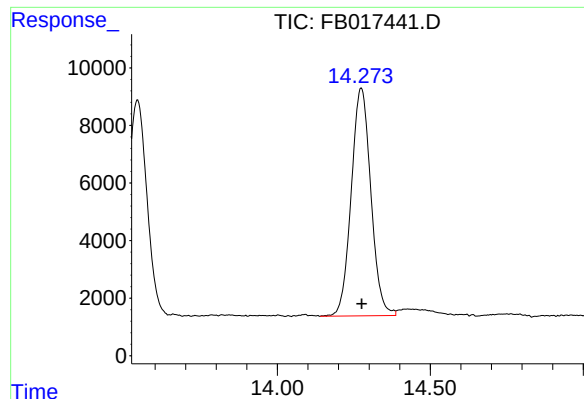

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: -0.002 min
Response: 353067
Conc: 17.37 ng/ml

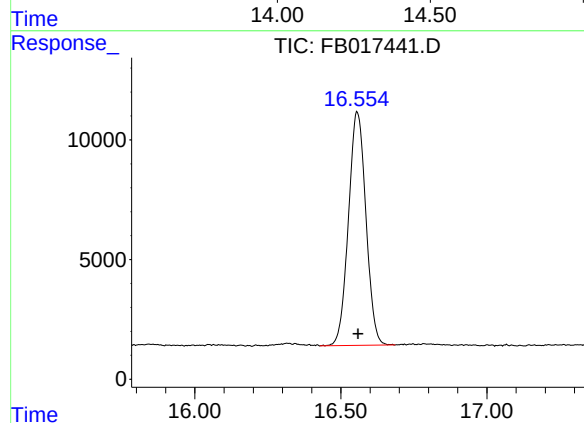

#10 1,2,4-Trimethylbenzene

R.T.: 16.557 min
Delta R.T.: -0.002 min
Response: 405542
Conc: 18.11 ng/ml