

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081718\
 Data File : FB017443.D
 Signal(s) : FID2B.CH
 Acq On : 17 Aug 2018 10:09
 Operator : MJ/SJ
 Sample : J4521-08MS
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 17 11:32:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080818.M
 Quant Title :
 QLast Update : Wed Aug 08 11:39:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.112	197317	21.060 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.963	474937	27.775 ng/ml
2) t 2,2,4-Trimethylpentane	7.725	475648	28.151 ng/ml
3) t n-Heptane	8.066	149157	9.259 ng/ml
4) t Benzene	8.207	189360	9.344 ng/ml
6) t Toluene	10.961	469378	28.476 ng/ml
7) t Ethylbenzene	13.410	156695	9.392 ng/ml
8) t m-Xylene	13.544	324440	17.307 ng/ml
9) t O-Xylene	14.275	338663	16.663 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	398992	17.816 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081718\
Data File : FB017443.D
Signal(s) : FID2B.CH
Acq On : 17 Aug 2018 10:09
Operator : MJ/SJ
Sample : J4521-08MS
Misc : 5.01g/5.00mL DI Water
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 17 11:32:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080818.M
Quant Title :
QLast Update : Wed Aug 08 11:39:03 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

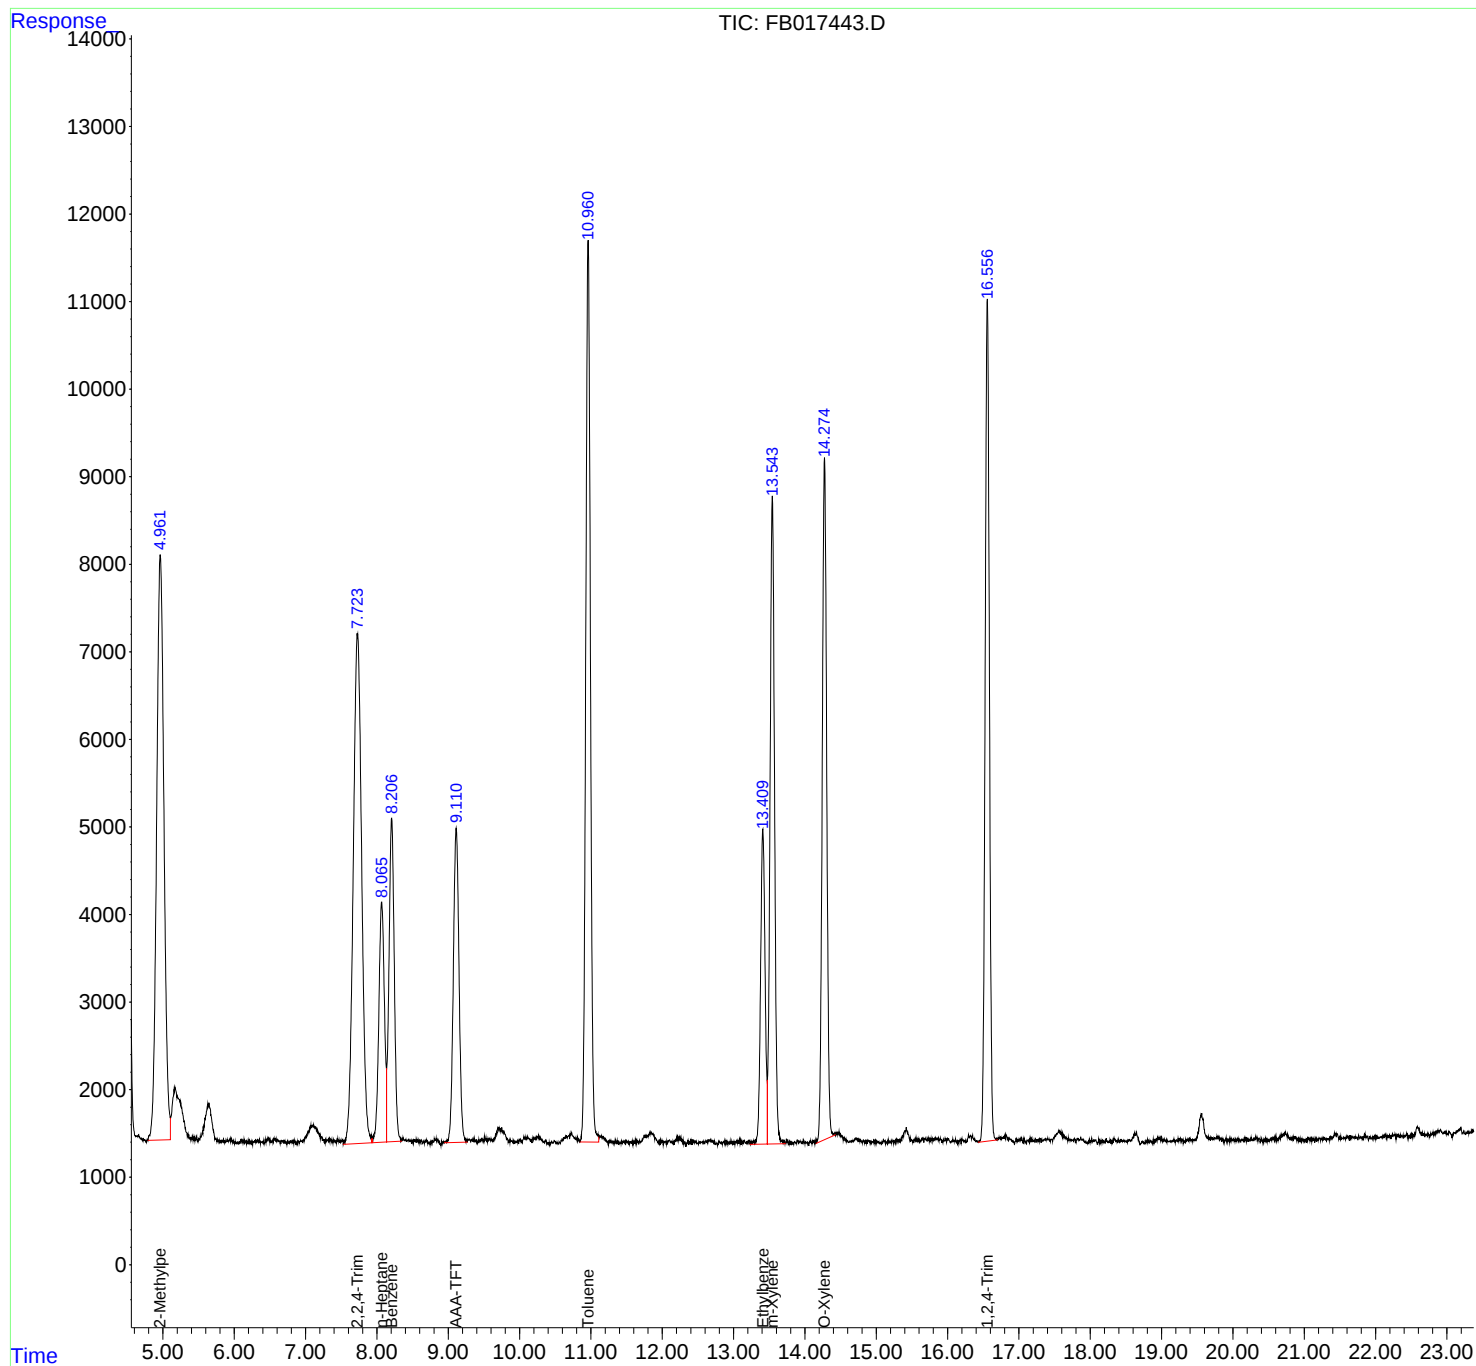

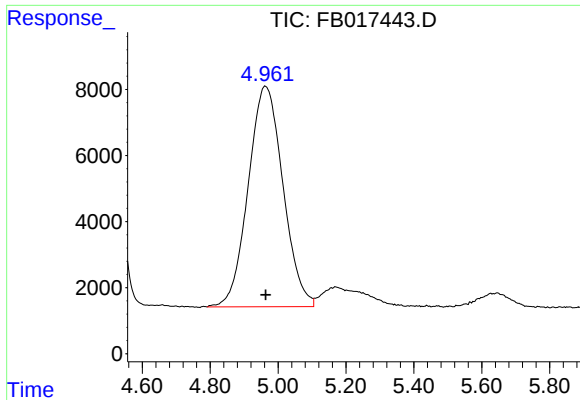


#1 2-Methylpentane

R.T.: 4.963 min
Delta R.T.: -0.001 min
Response: 474937
Conc: 27.77 ng/ml

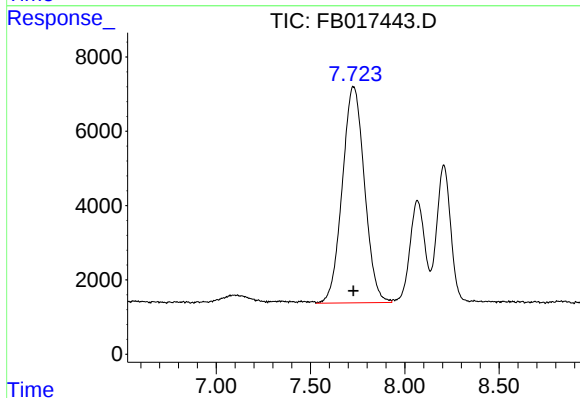


#2 2,2,4-Trimethylpentane

R.T.: 7.725 min
Delta R.T.: -0.003 min
Response: 475648
Conc: 28.15 ng/ml

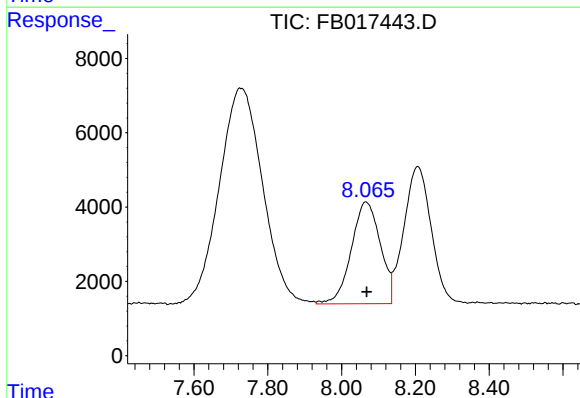


#3 n-Heptane

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 149157
Conc: 9.26 ng/ml

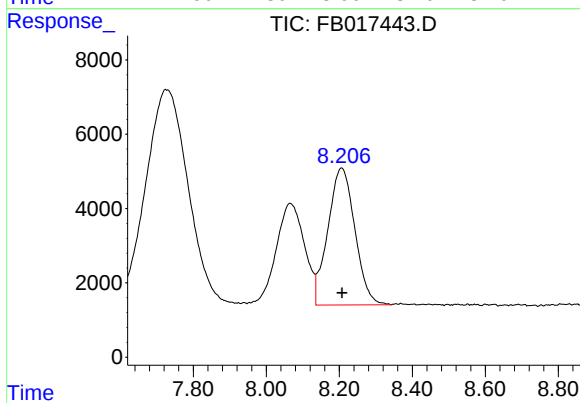


#4 Benzene

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 189360
Conc: 9.34 ng/ml

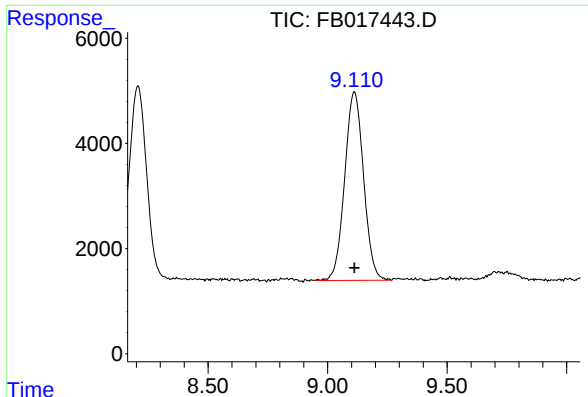


#5 AAA-TFT

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 197317
Conc: 21.06 ng/ml

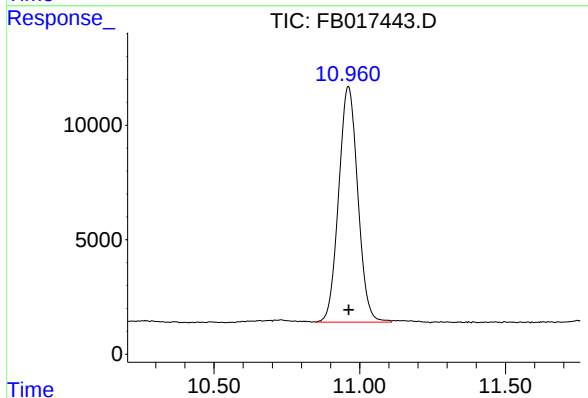


#6 Toluene

R.T.: 10.961 min
Delta R.T.: 0.000 min
Response: 469378
Conc: 28.48 ng/ml

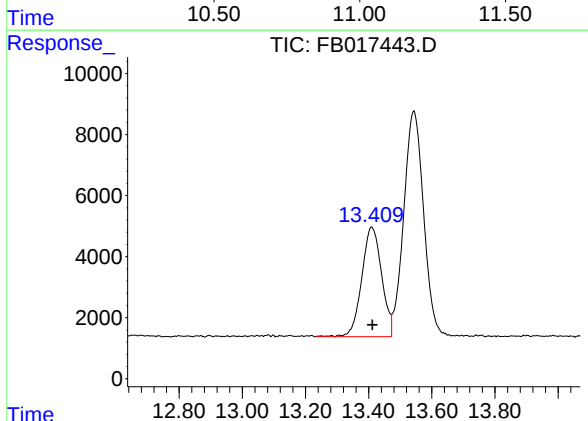


#7 Ethylbenzene

R.T.: 13.410 min
Delta R.T.: -0.002 min
Response: 156695
Conc: 9.39 ng/ml

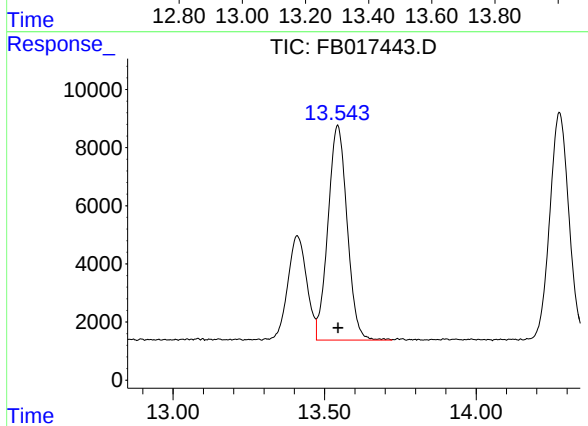


#8 m-Xylene

R.T.: 13.544 min
Delta R.T.: 0.000 min
Response: 324440
Conc: 17.31 ng/ml

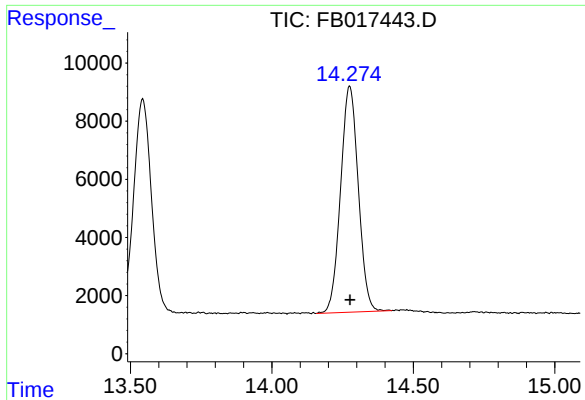

#9 O-Xylene

R.T.: 14.275 min
Delta R.T.: -0.001 min
Response: 338663
Conc: 16.66 ng/ml

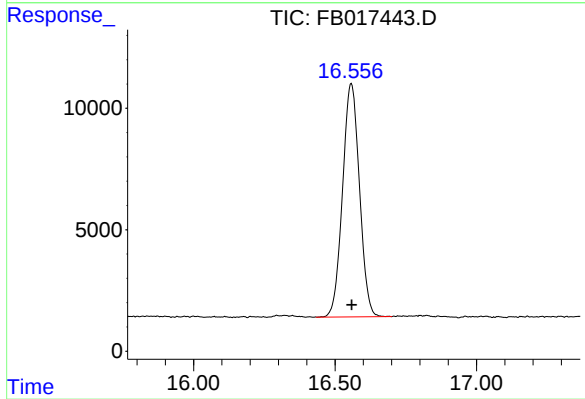

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: -0.001 min
Response: 398992
Conc: 17.82 ng/ml