

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081720\
 Data File : FB024759.D
 Signal(s) : FID2B.CH
 Acq On : 17 Aug 2020 16:49
 Operator : DD/AJ
 Sample : L3500-02MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 18 00:39:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
 Quant Title :
 QLast Update : Mon Aug 10 12:11:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	483021	23.392 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	704551	29.277 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	797247	28.761 ng/ml
3) t n-Heptane	7.759	248880	9.153 ng/ml
4) t Benzene	7.894	354406	10.099 ng/ml
6) t Toluene	10.632	1034563	30.034 ng/ml
7) t Ethylbenzene	13.072	318010	9.934 ng/ml
8) t m-Xylene	13.204	623641	19.986 ng/ml
9) t O-Xylene	13.932	611750	20.228 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	505380	20.578 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081720\
Data File : FB024759.D
Signal(s) : FID2B.CH
Acq On : 17 Aug 2020 16:49
Operator : DD/AJ
Sample : L3500-02MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 18 00:39:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

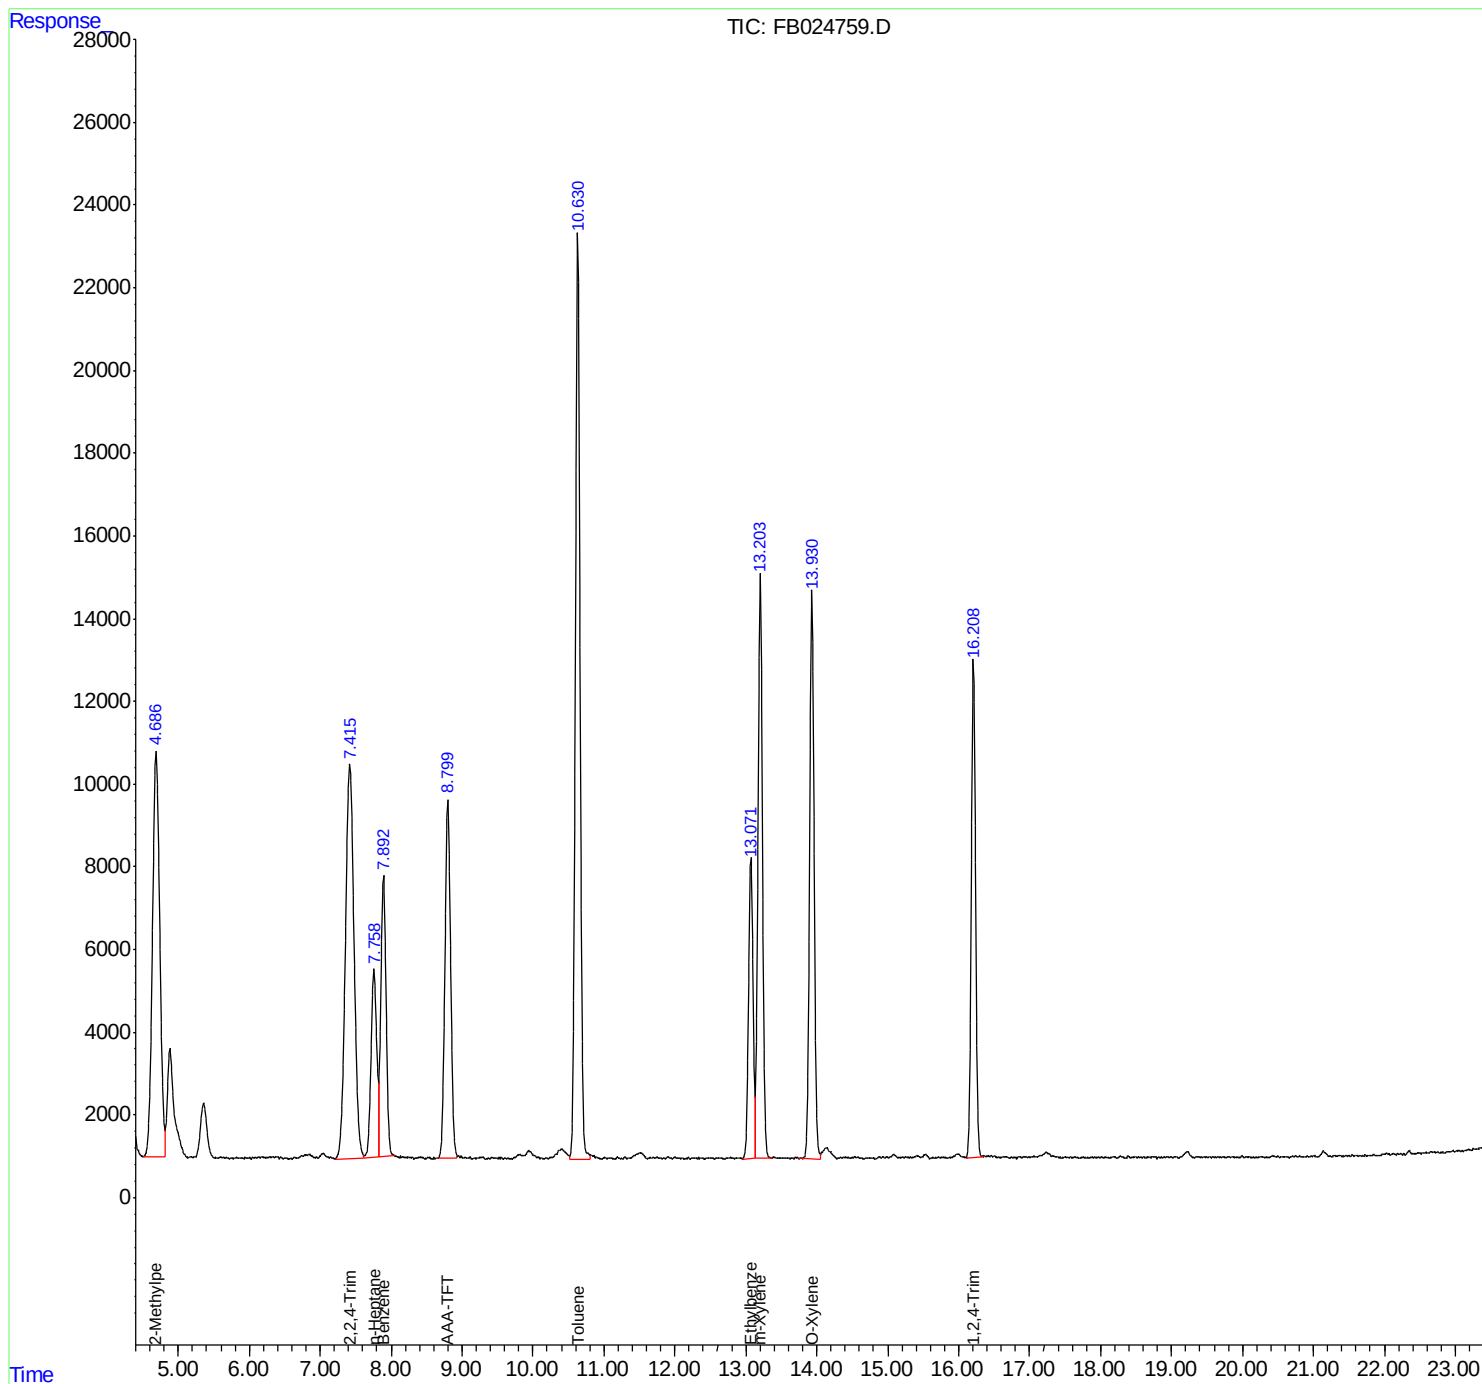

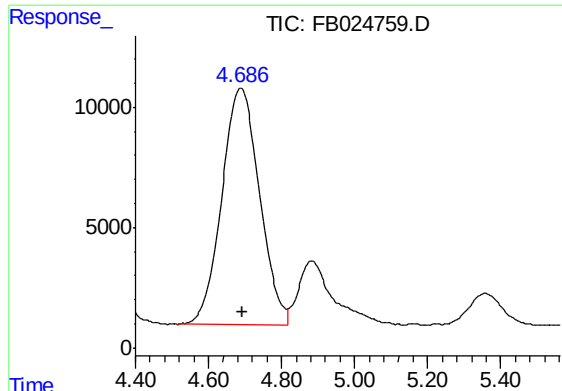


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 704551
Conc: 29.28 ng/ml

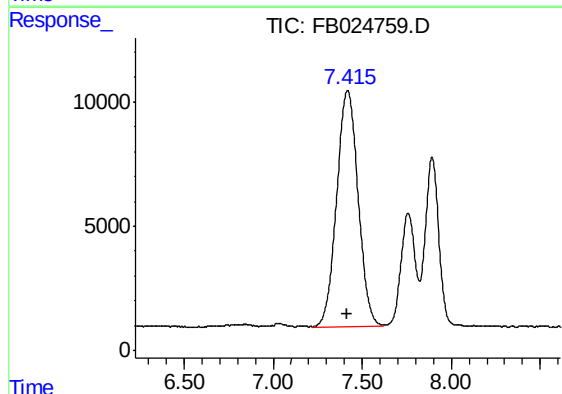


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 797247
Conc: 28.76 ng/ml

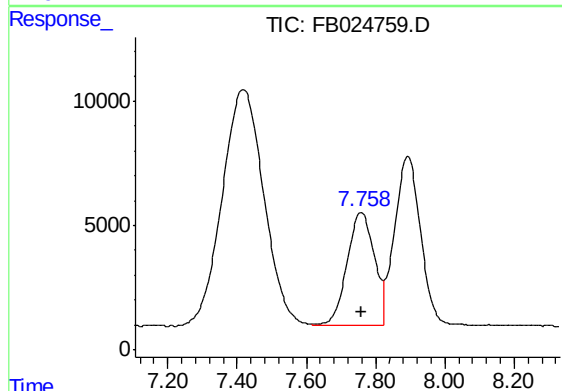


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.001 min
Response: 248880
Conc: 9.15 ng/ml

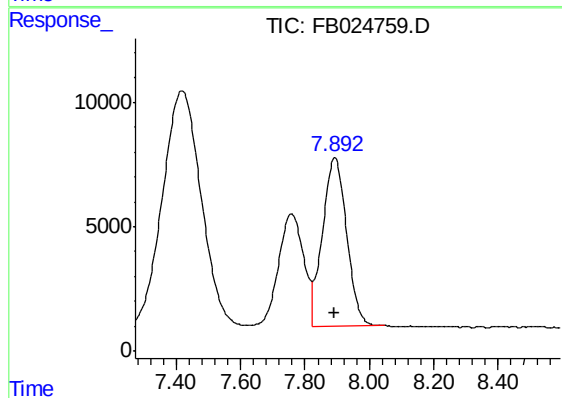


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.001 min
Response: 354406
Conc: 10.10 ng/ml

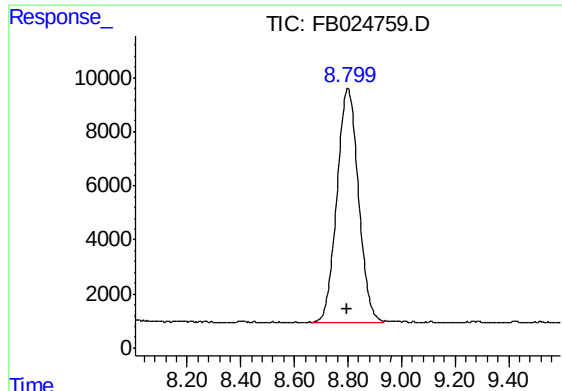


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.001 min
Response: 483021
Conc: 23.39 ng/ml

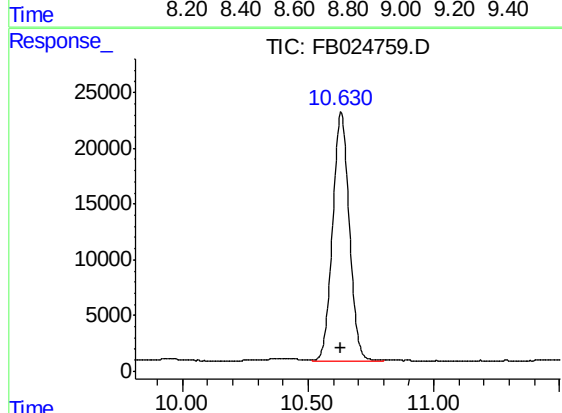


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.002 min
Response: 1034563
Conc: 30.03 ng/ml

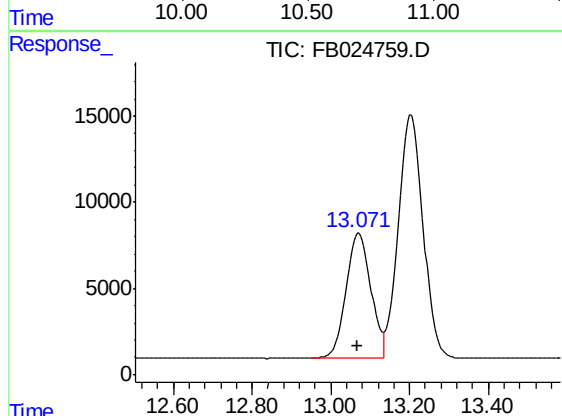


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.003 min
Response: 318010
Conc: 9.93 ng/ml

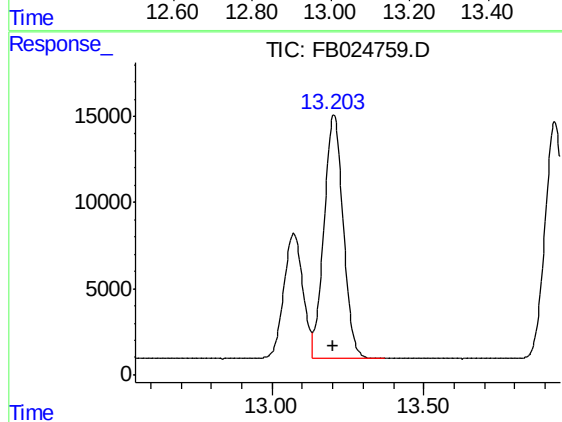


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.002 min
Response: 623641
Conc: 19.99 ng/ml

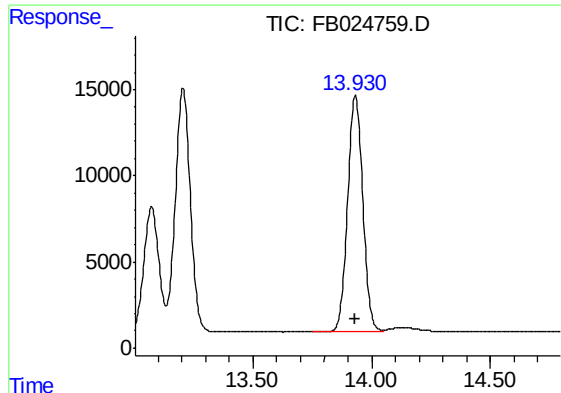

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.002 min
Response: 611750
Conc: 20.23 ng/ml

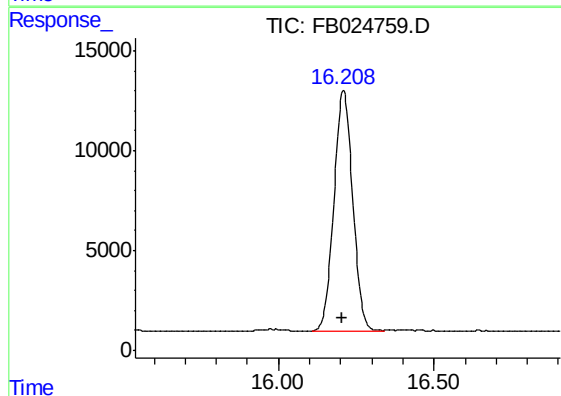

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.003 min
Response: 505380
Conc: 20.58 ng/ml