

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081721\
 Data File : FB026208.D
 Signal(s) : FID2B.CH
 Acq On : 17 Aug 2021 13:02
 Operator : AJ/MA
 Sample : BSF0817S1
 Misc : 5.02G\5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0817S1

Integration File: SAMPLE.e
 Quant Time: Aug 18 04:34:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
 Quant Title :
 QLast Update : Fri Aug 13 22:11:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.835	288917	19.388 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.824	678790	30.067 ng/ml
2) t 2,2,4-Trimethylpentane	7.493	704036	32.025 ng/ml
3) t n-Heptane	7.809	281551	9.346 ng/ml
4) t Benzene	7.947	294914	9.333 ng/ml
6) t Toluene	10.648	834674	28.996 ng/ml
7) t Ethylbenzene	13.069	239819	9.934 ng/ml
8) t m-Xylene	13.201	464782	19.887 ng/ml
9) t O-Xylene	13.926	425169	20.436 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	433981	21.512 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081721\
Data File : FB026208.D
Signal(s) : FID2B.CH
Acq On : 17 Aug 2021 13:02
Operator : AJ/MA
Sample : BSF0817S1
Misc : 5.02G\5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0817S1

Integration File: SAMPLE.e
Quant Time: Aug 18 04:34:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081321.M
Quant Title :
QLast Update : Fri Aug 13 22:11:30 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

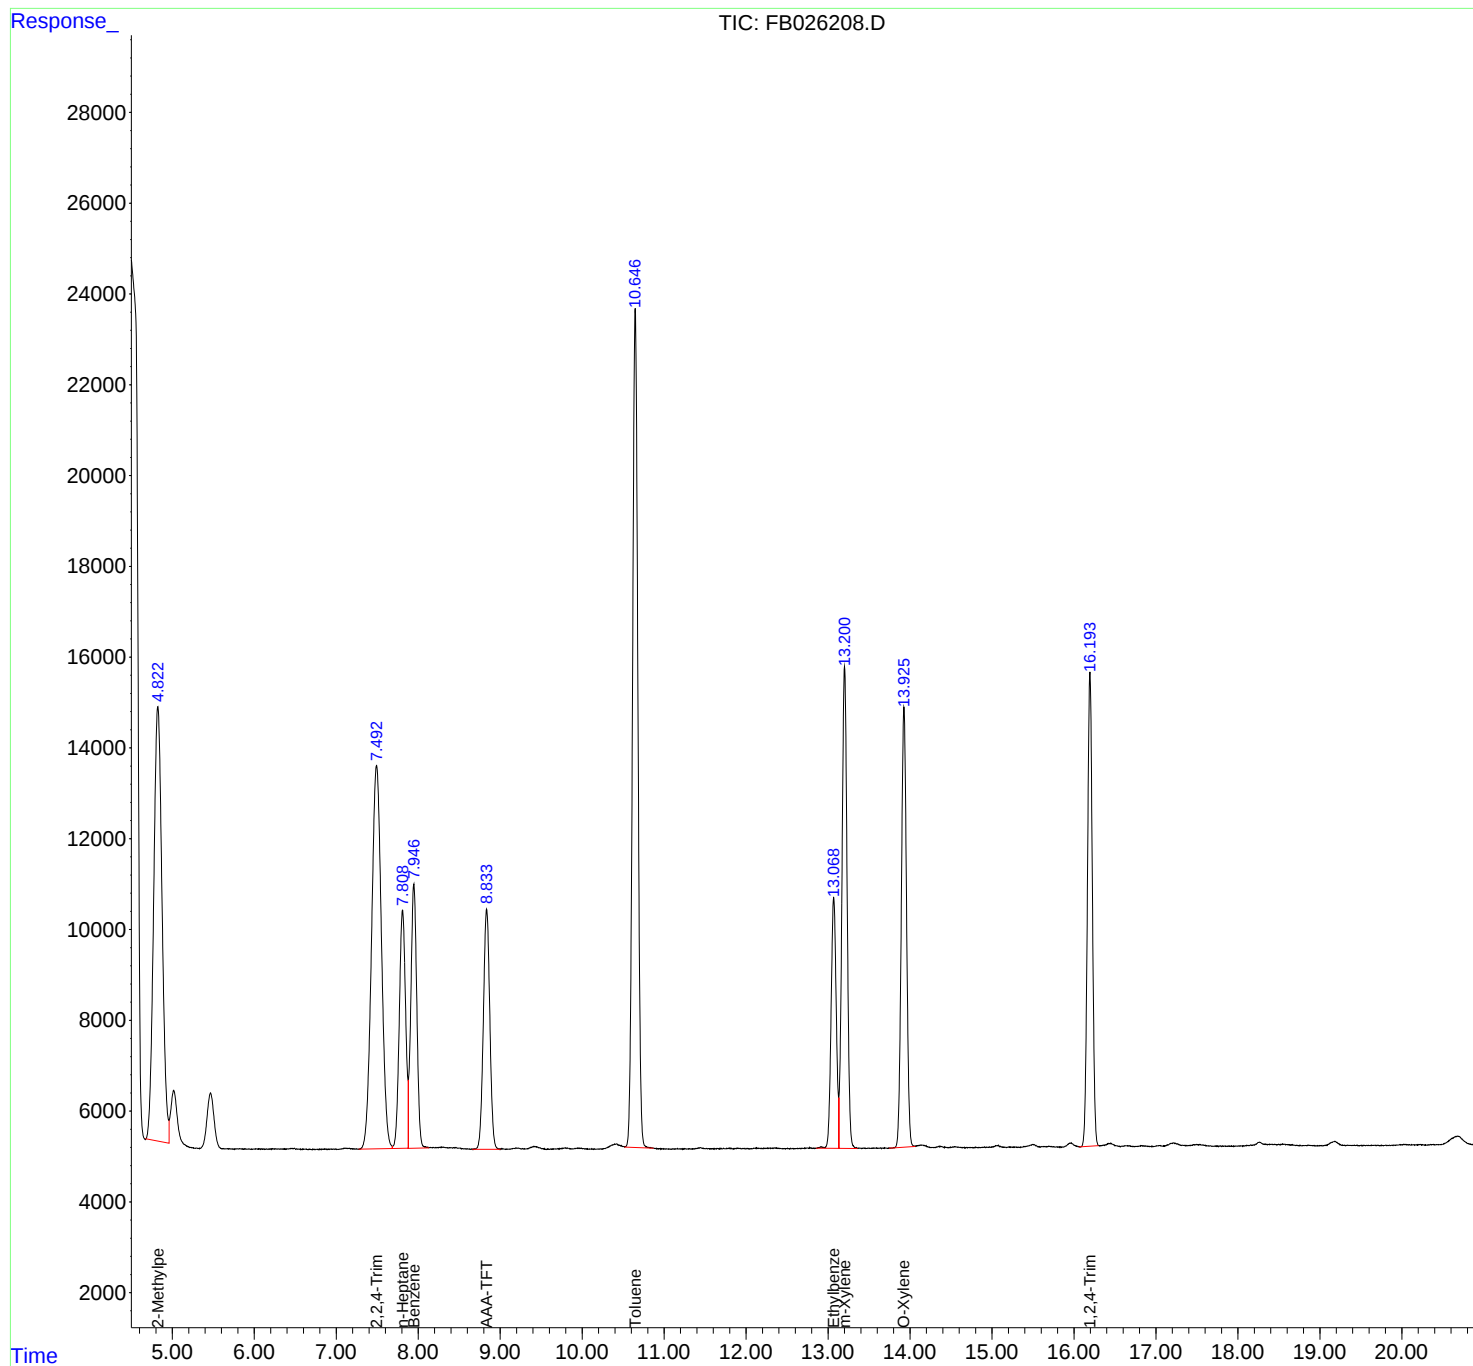


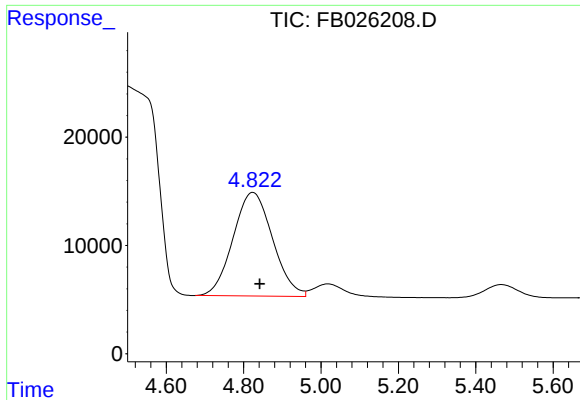

#1 2-Methylpentane


R.T.: 4.824 min
Delta R.T.: -0.018 min
Response: 678790
Conc: 30.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0817S1

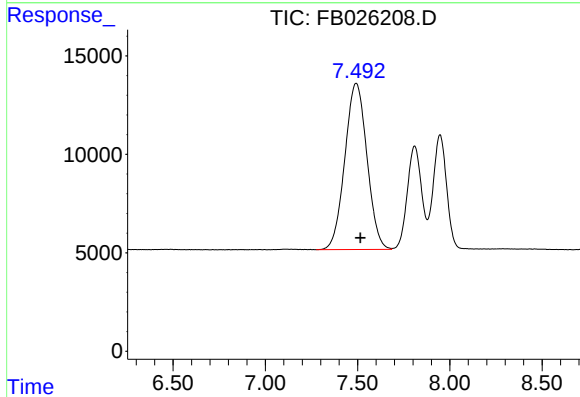


#2 2,2,4-Trimethylpentane

R.T.: 7.493 min
Delta R.T.: -0.022 min
Response: 704036
Conc: 32.03 ng/ml

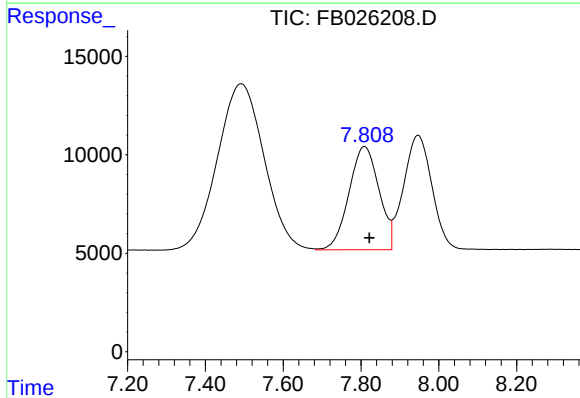


#3 n-Heptane

R.T.: 7.809 min
Delta R.T.: -0.012 min
Response: 281551
Conc: 9.35 ng/ml

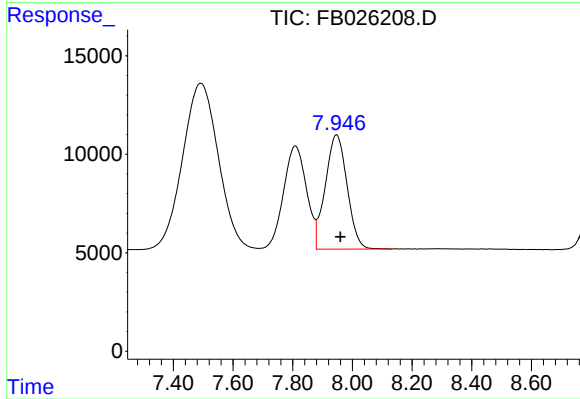

#4 Benzene


R.T.: 7.947 min
Delta R.T.: -0.013 min
Response: 294914
Conc: 9.33 ng/ml

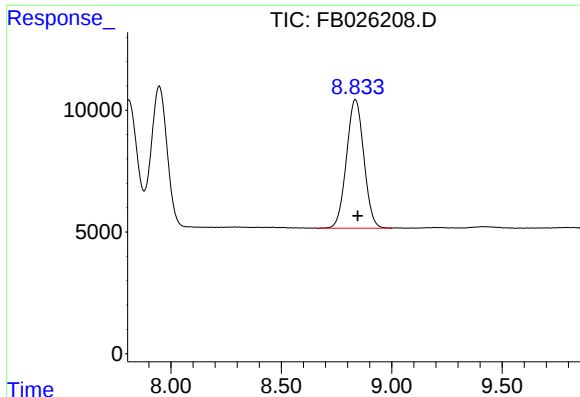

#5 AAA-TFT


R.T.: 8.835 min
Delta R.T.: -0.012 min
Response: 288917
Conc: 19.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0817S1

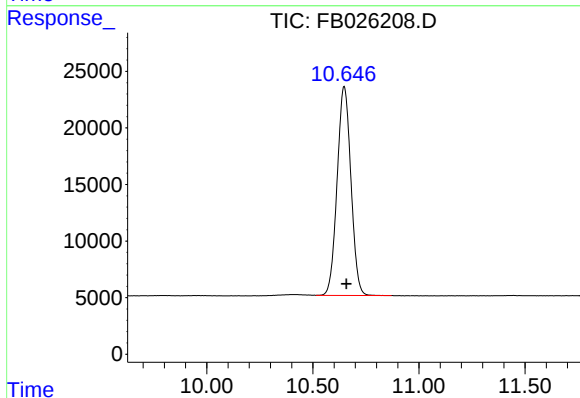


#6 Toluene

R.T.: 10.648 min
Delta R.T.: -0.010 min
Response: 834674
Conc: 29.00 ng/ml

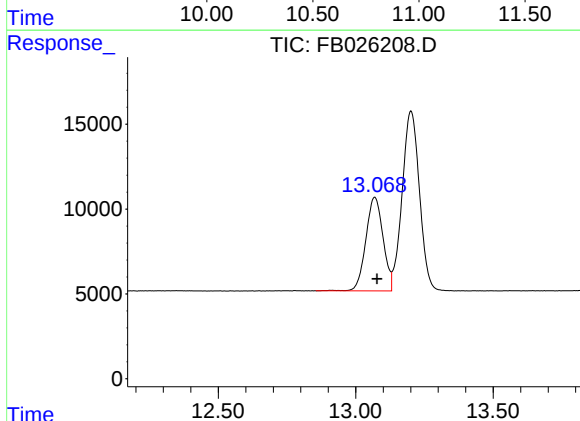


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.007 min
Response: 239819
Conc: 9.93 ng/ml

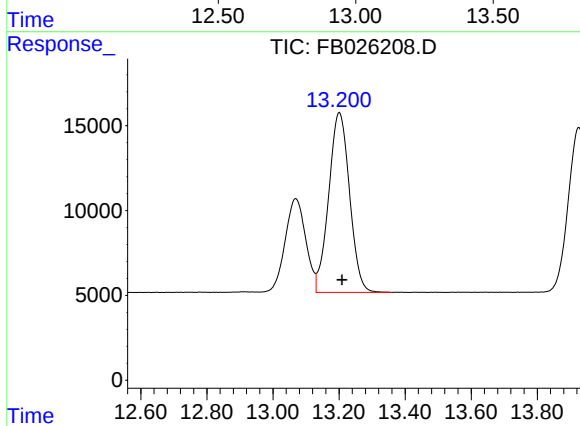

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.008 min
Response: 464782
Conc: 19.89 ng/ml

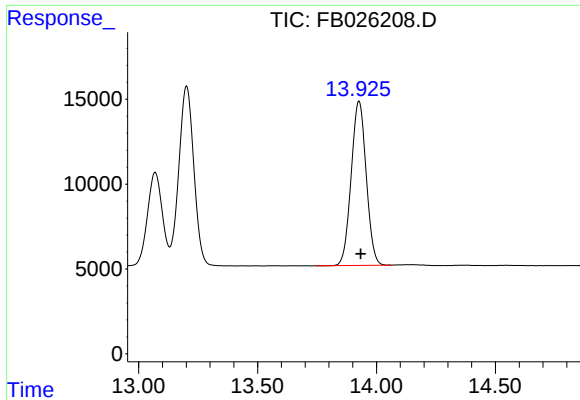

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.007 min
Response: 425169
Conc: 20.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0817S1

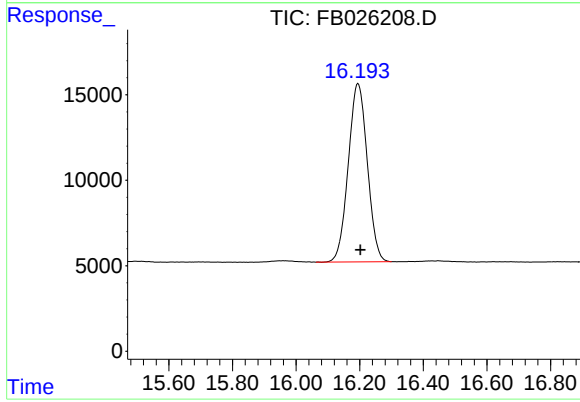

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.007 min
Response: 433981
Conc: 21.51 ng/ml