

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081722\
 Data File : FB027984.D
 Signal(s) : FID2B.CH
 Acq On : 17 Aug 2022 14:56
 Operator : AJ/MA
 Sample : BSF0817S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0817S1

Integration File: Calibration.e
 Quant Time: Aug 17 23:21:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	220615	19.036 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	599471	33.137 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	619456	31.589 ng/ml
3) t n-Heptane	7.753	200916	10.429 ng/ml
4) t Benzene	7.889	228601	9.832 ng/ml
6) t Toluene	10.623	665345	30.342 ng/ml
7) t Ethylbenzene	13.060	203689	9.884 ng/ml
8) t m-Xylene	13.193	405987	19.840 ng/ml
9) t O-Xylene	13.919	393670	19.873 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	395221	20.267 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081722\
Data File : FB027984.D
Signal(s) : FID2B.CH
Acq On : 17 Aug 2022 14:56
Operator : AJ/MA
Sample : BSF0817S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0817S1

Integration File: Calibration.e
Quant Time: Aug 17 23:21:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

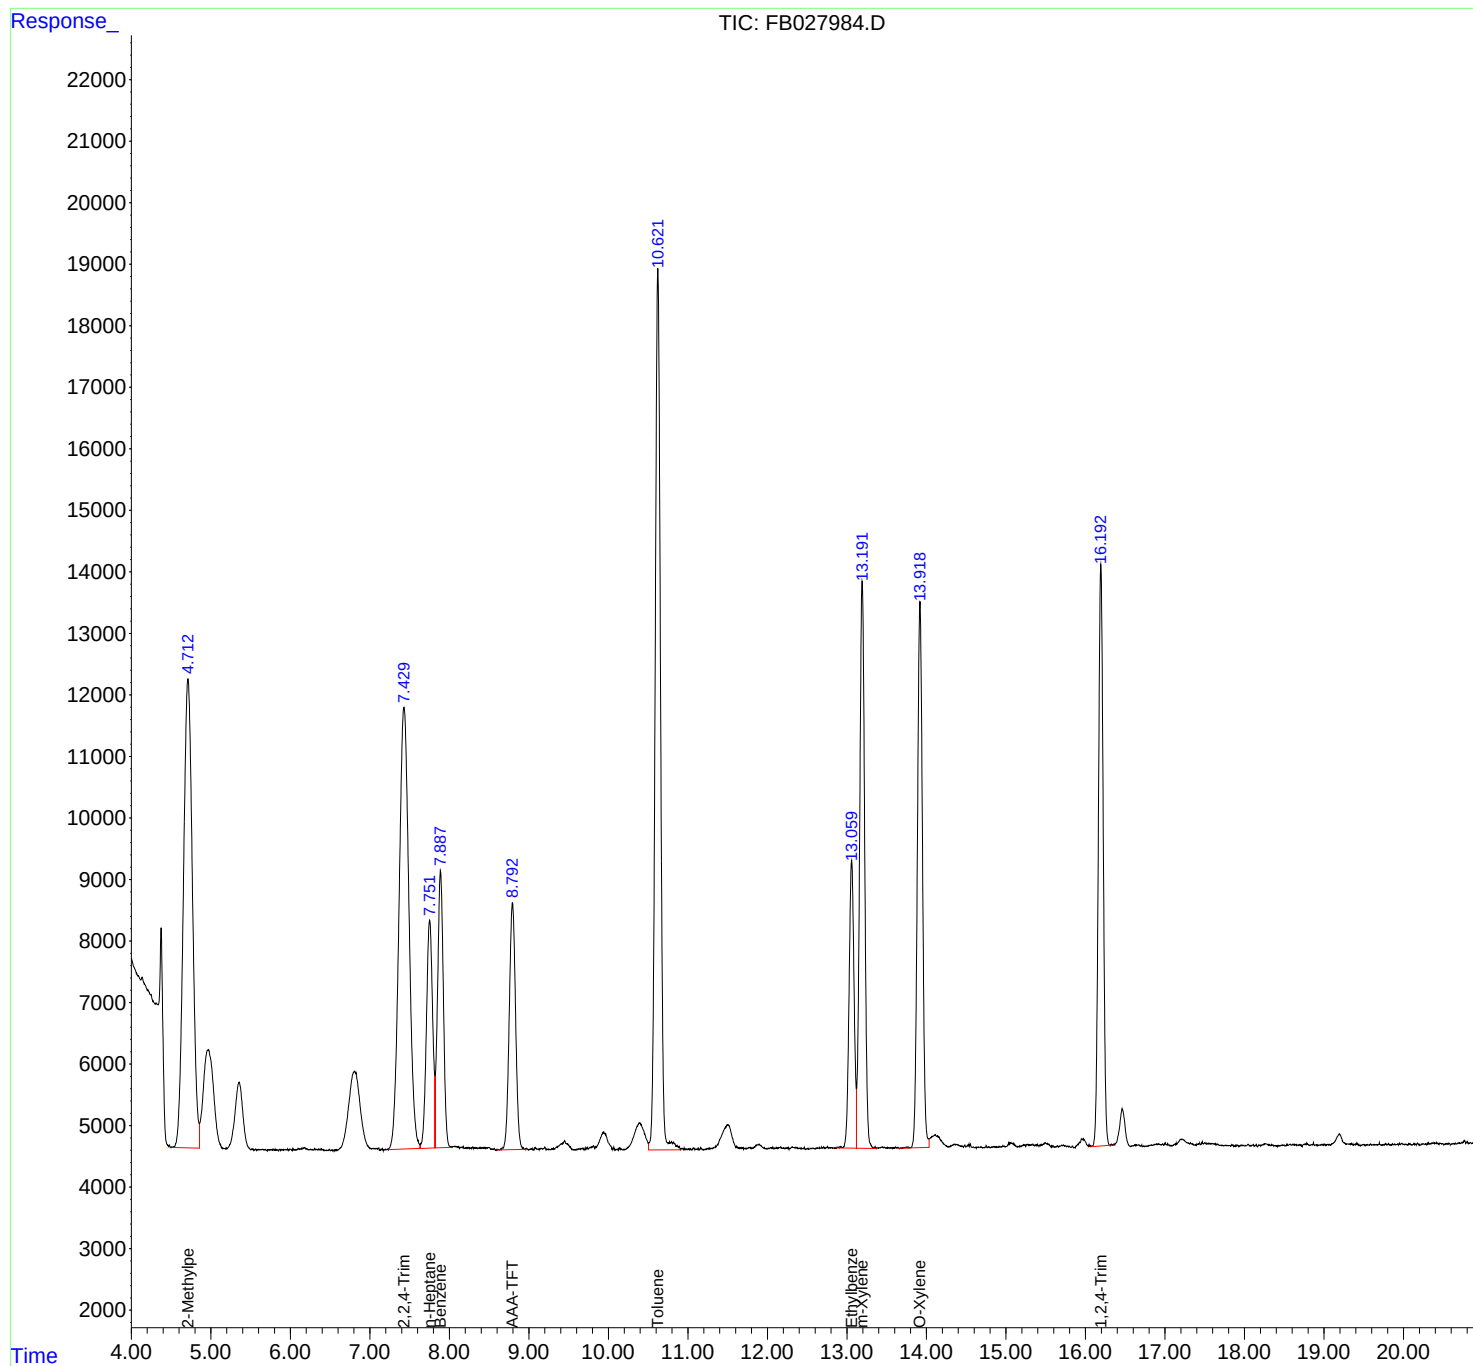


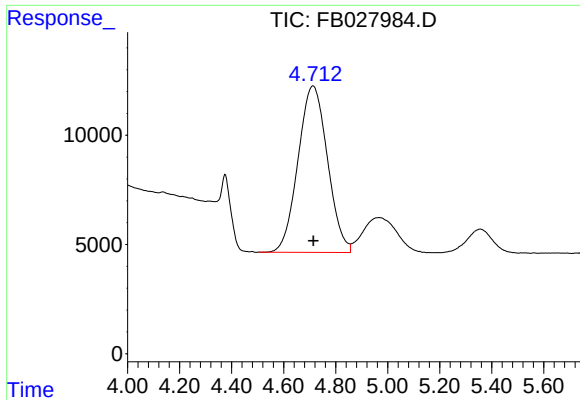

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: -0.002 min
Response: 599471
Conc: 33.14 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0817S1

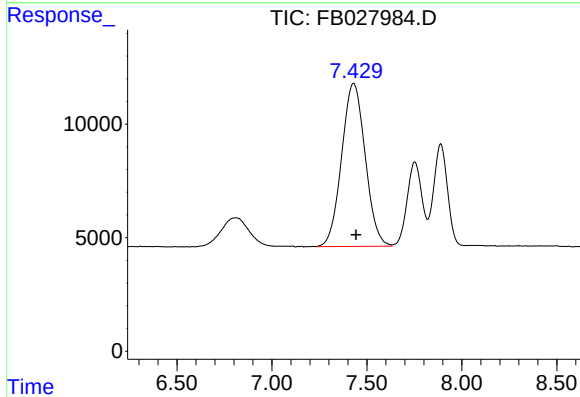


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: -0.013 min
Response: 619456
Conc: 31.59 ng/ml

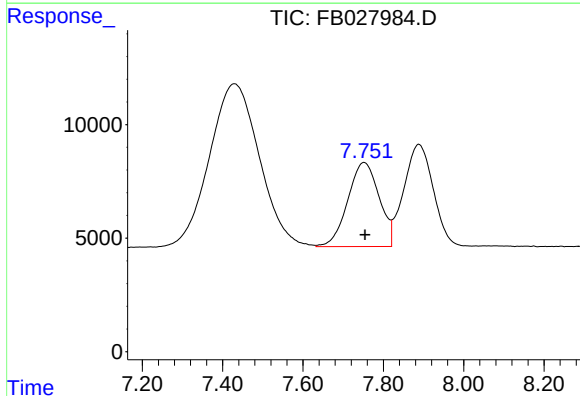


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.003 min
Response: 200916
Conc: 10.43 ng/ml

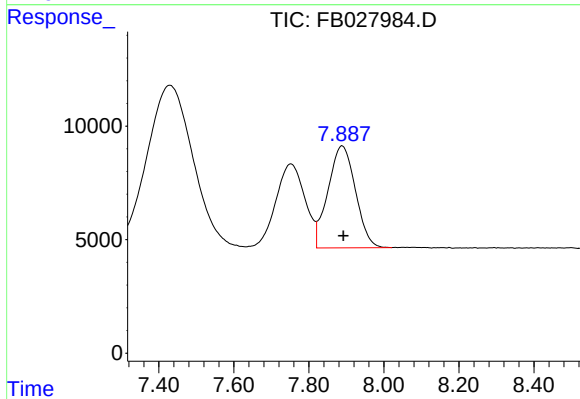

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 228601
Conc: 9.83 ng/ml

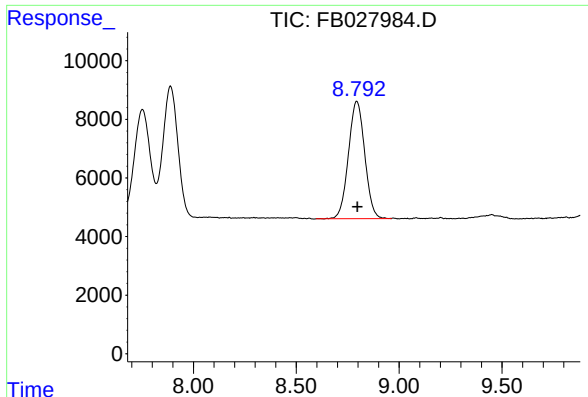

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.004 min
Response: 220615
Conc: 19.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0817S1

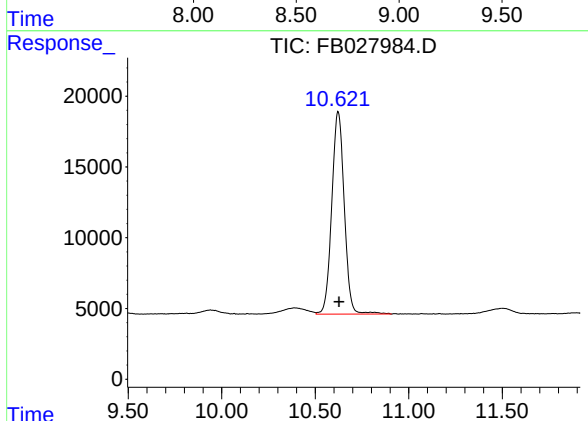


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.005 min
Response: 665345
Conc: 30.34 ng/ml

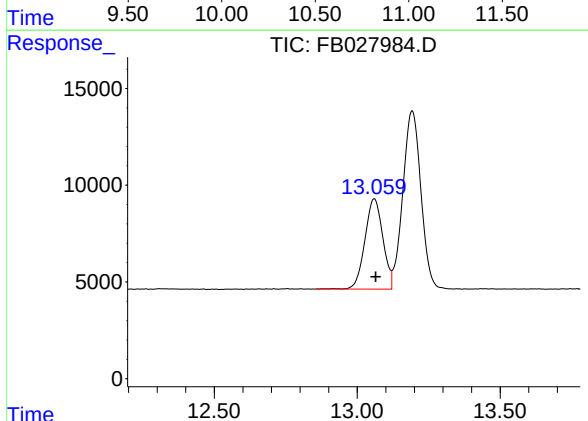


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.005 min
Response: 203689
Conc: 9.88 ng/ml

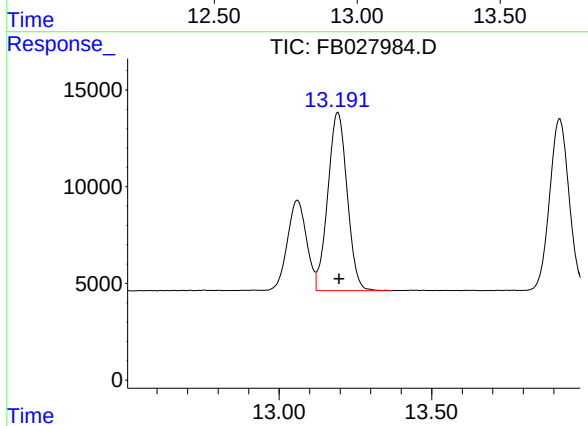

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.005 min
Response: 405987
Conc: 19.84 ng/ml

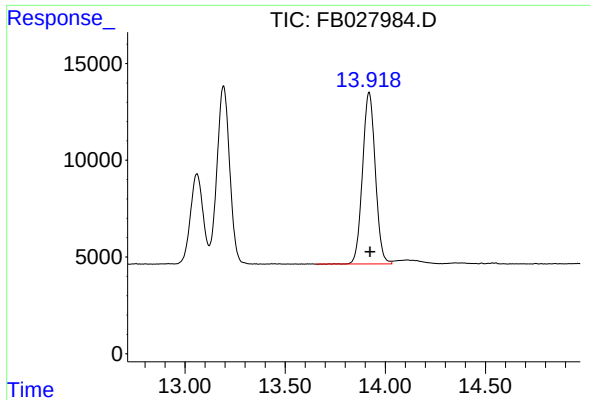

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.005 min
Response: 393670
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0817S1

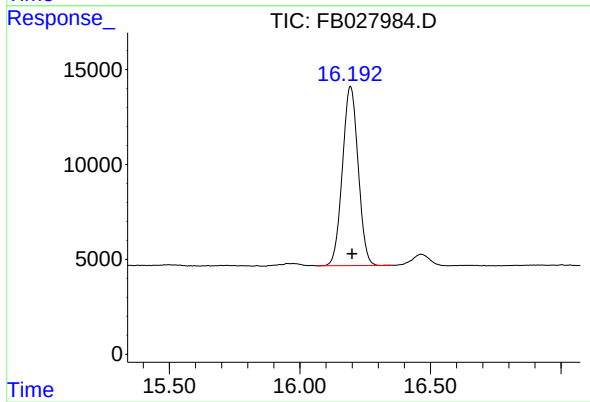

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.005 min
Response: 395221
Conc: 20.27 ng/ml