

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081722\
 Data File : FB027988.D
 Signal(s) : FID2B.CH
 Acq On : 17 Aug 2022 17:24
 Operator : AJ/MA
 Sample : N4226-01MS 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 B-1MS

Integration File: Calibration.e
 Quant Time: Aug 17 23:22:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	261380	22.553 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	529700	29.280 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	586349	29.900 ng/ml
3) t n-Heptane	7.752	188005	9.759 ng/ml
4) t Benzene	7.890	227534	9.786 ng/ml
6) t Toluene	10.624	620788	28.310 ng/ml
7) t Ethylbenzene	13.062	194648	9.446 ng/ml
8) t m-Xylene	13.195	386059	18.866 ng/ml
9) t O-Xylene	13.921	380559	19.211 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	371317	19.041 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081722\
Data File : FB027988.D
Signal(s) : FID2B.CH
Acq On : 17 Aug 2022 17:24
Operator : AJ/MA
Sample : N4226-01MS 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B-1MS

Integration File: Calibration.e
Quant Time: Aug 17 23:22:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

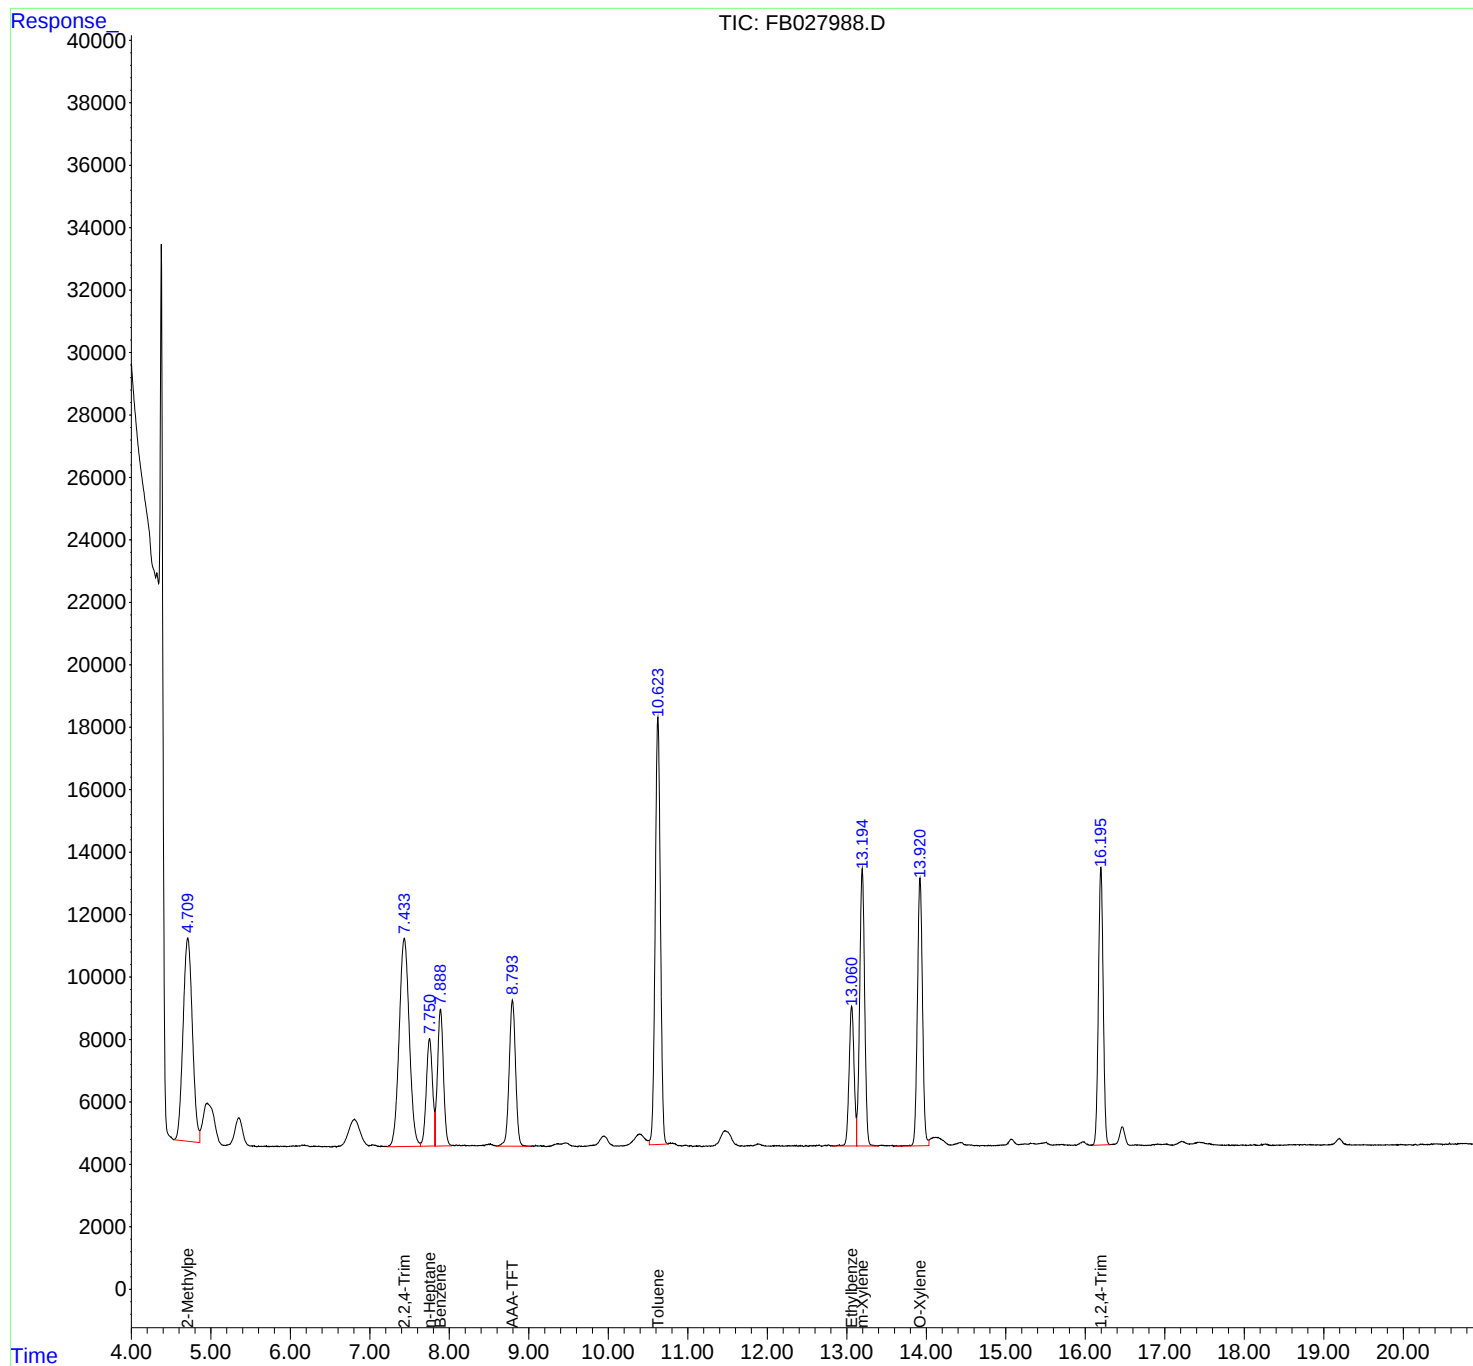


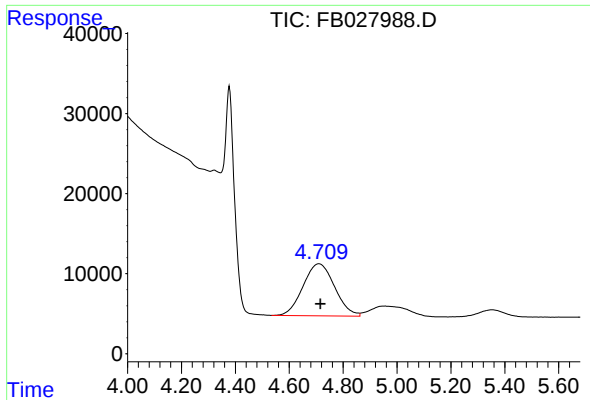

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: -0.004 min
Response: 529700
Conc: 29.28 ng/ml

Instrument :
FID_B
ClientSampleId :
B-1MS

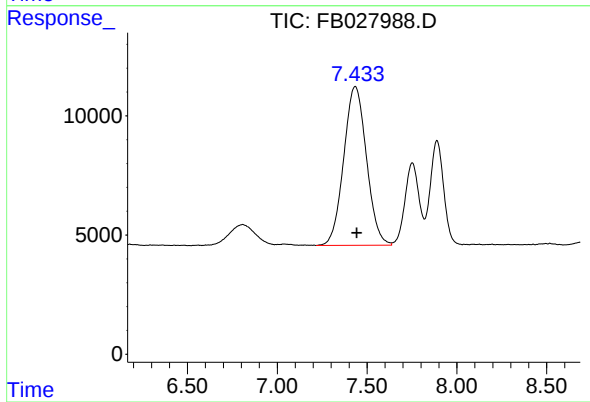


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: -0.008 min
Response: 586349
Conc: 29.90 ng/ml

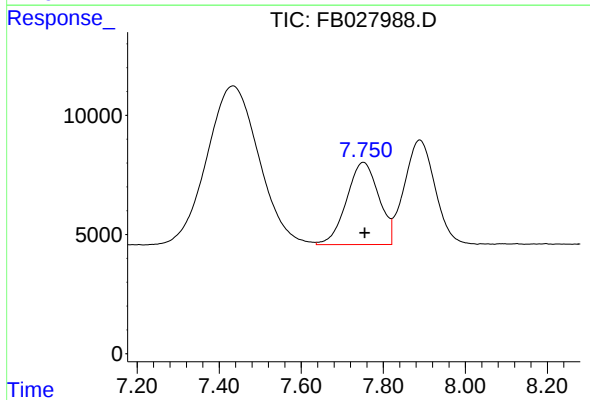


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 188005
Conc: 9.76 ng/ml

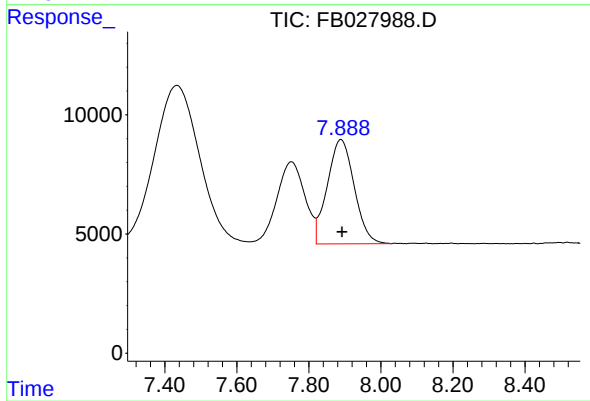

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 227534
Conc: 9.79 ng/ml

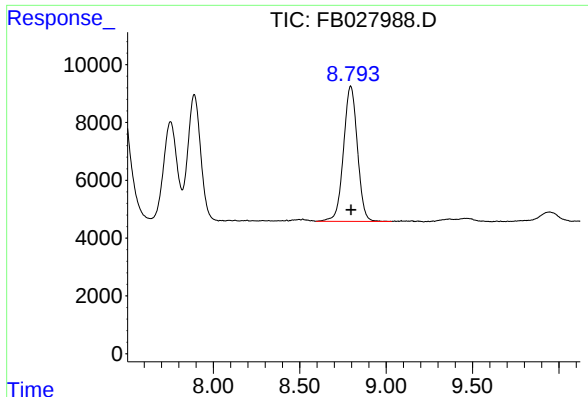

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 261380
Conc: 22.55 ng/ml

Instrument :
FID_B
ClientSampleId :
B-1MS

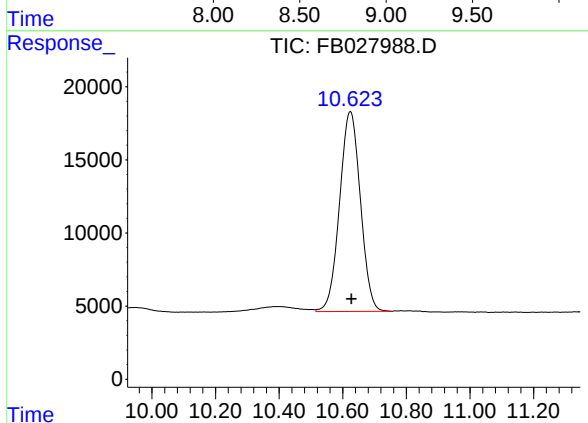


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 620788
Conc: 28.31 ng/ml

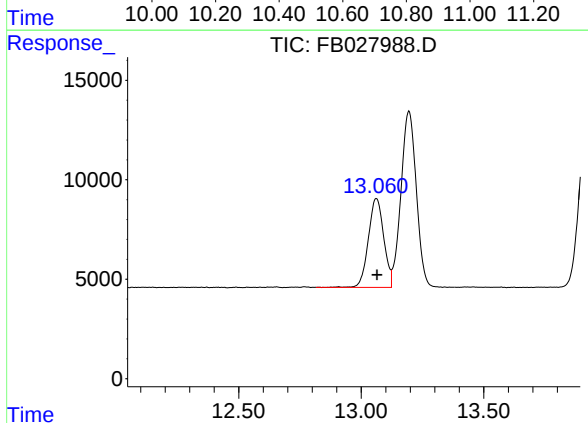


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.003 min
Response: 194648
Conc: 9.45 ng/ml

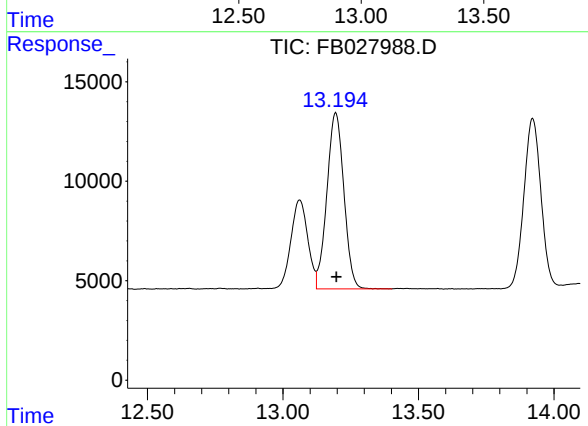

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 386059
Conc: 18.87 ng/ml

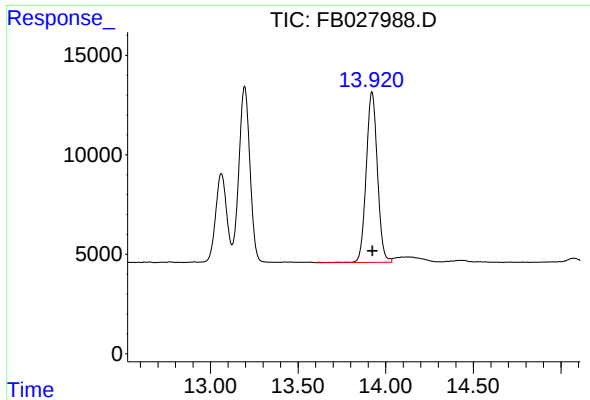

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.003 min
Response: 380559
Conc: 19.21 ng/ml

Instrument :
FID_B
ClientSampleId :
B-1MS

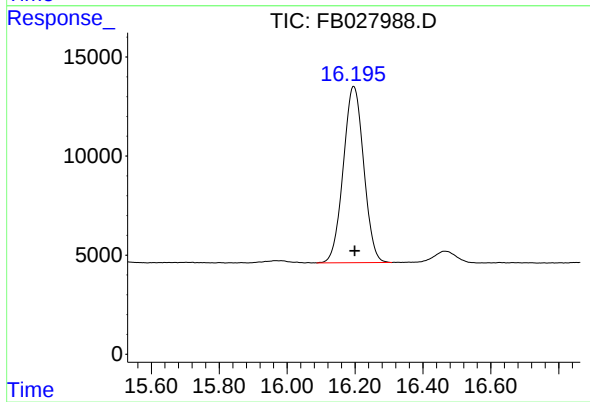

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.002 min
Response: 371317
Conc: 19.04 ng/ml