

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081722\
 Data File : FB027989.D
 Signal(s) : FID2B.CH
 Acq On : 17 Aug 2022 18:01
 Operator : AJ/MA
 Sample : N4226-01MSD 50X
 Misc : 5.04G/5.00 ML MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 B-1MSD

Integration File: Calibration.e
 Quant Time: Aug 17 23:22:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	214547	18.512 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	494260	27.321 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	586509	29.908 ng/ml
3) t n-Heptane	7.752	178523	9.267 ng/ml
4) t Benzene	7.889	222003	9.548 ng/ml
6) t Toluene	10.625	610509	27.841 ng/ml
7) t Ethylbenzene	13.062	192498	9.341 ng/ml
8) t m-Xylene	13.195	385994	18.863 ng/ml
9) t O-Xylene	13.922	380220	19.194 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	381394	19.558 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081722\
Data File : FB027989.D
Signal(s) : FID2B.CH
Acq On : 17 Aug 2022 18:01
Operator : AJ/MA
Sample : N4226-01MSD 50X
Misc : 5.04G/5.00 ML MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
B-1MSD

Integration File: Calibration.e
Quant Time: Aug 17 23:22:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

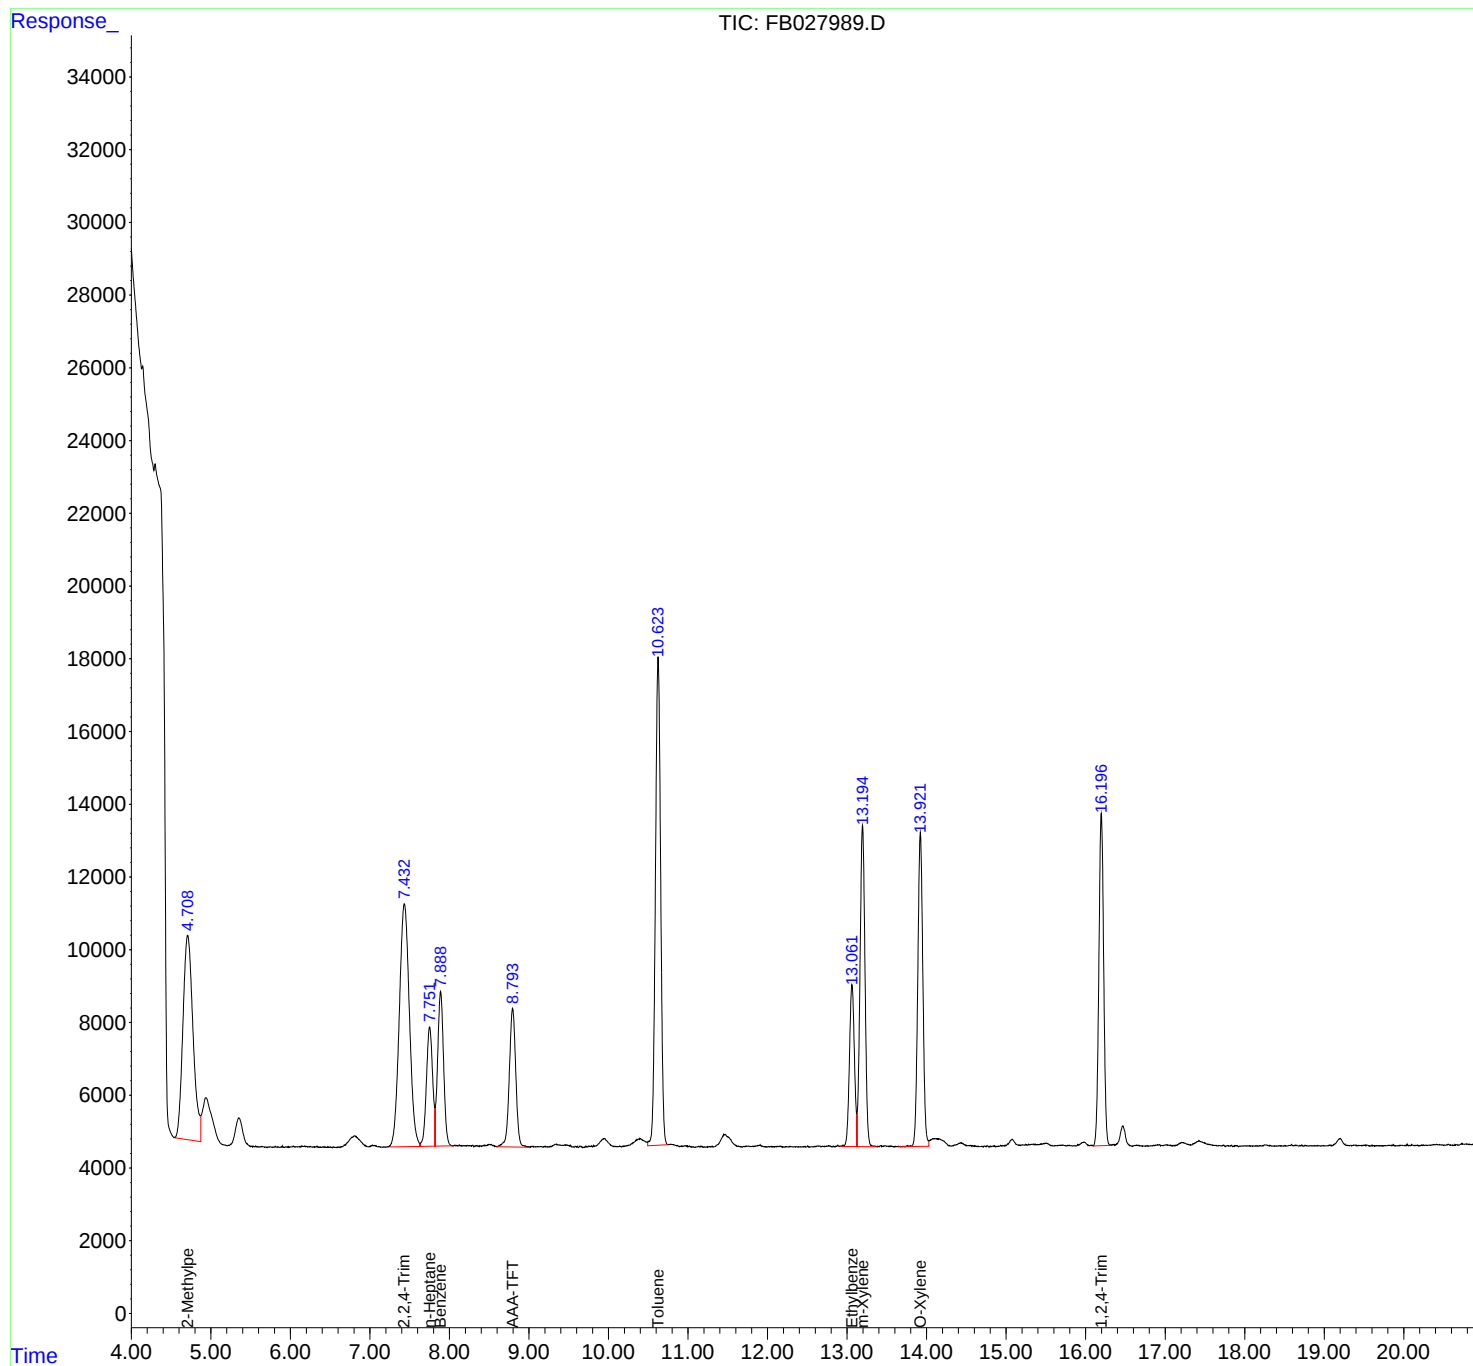


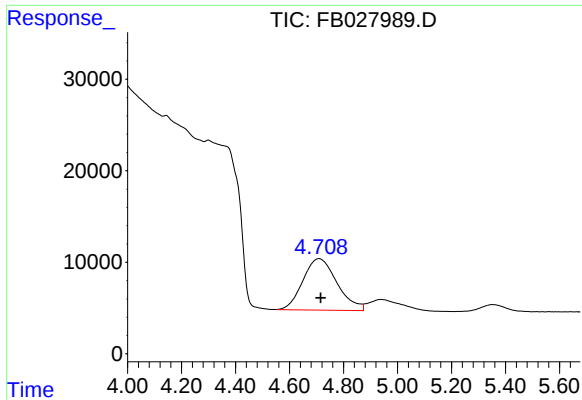

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: -0.005 min
Response: 494260
Conc: 27.32 ng/ml

Instrument :
FID_B
ClientSampleId :
B-1MSD

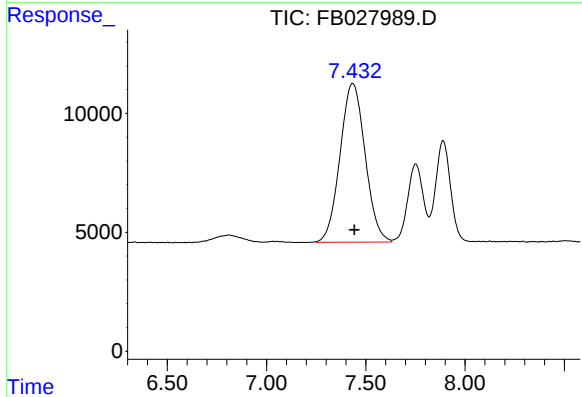


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: -0.010 min
Response: 586509
Conc: 29.91 ng/ml

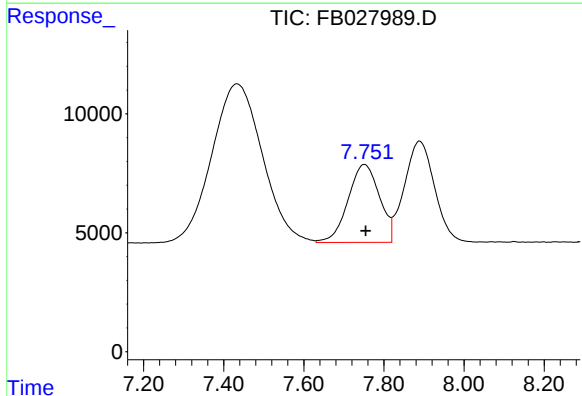


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 178523
Conc: 9.27 ng/ml

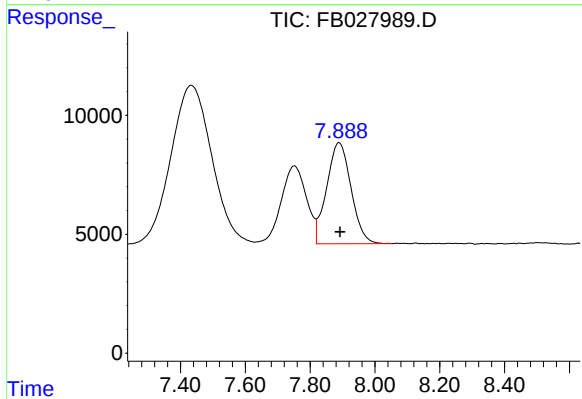

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.003 min
Response: 222003
Conc: 9.55 ng/ml

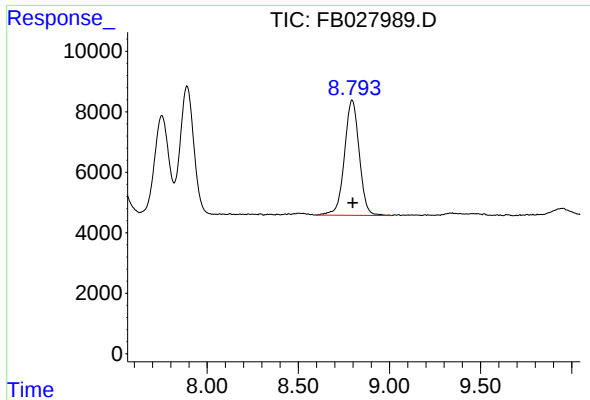

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 214547
Conc: 18.51 ng/ml

Instrument :
FID_B
ClientSampleId :
B-1MSD

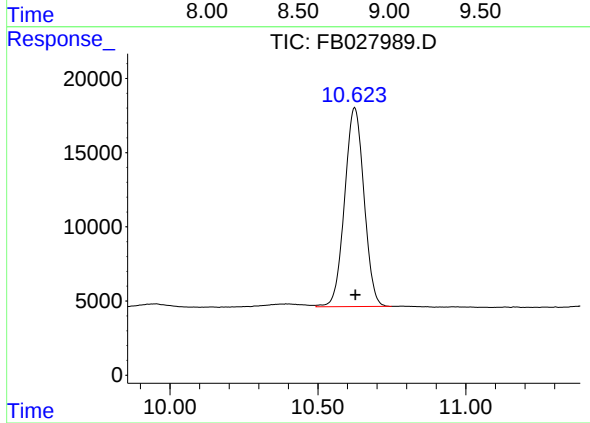


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.003 min
Response: 610509
Conc: 27.84 ng/ml

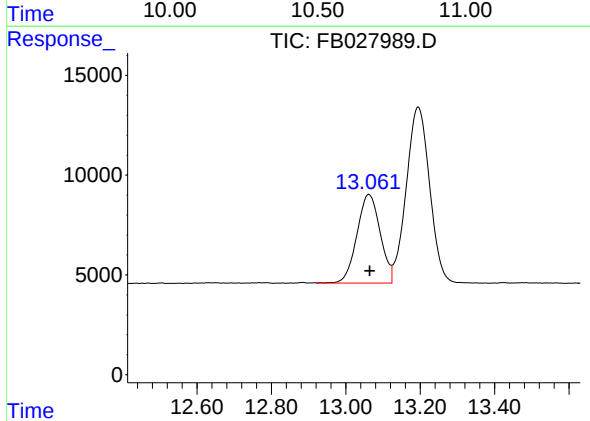


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.002 min
Response: 192498
Conc: 9.34 ng/ml

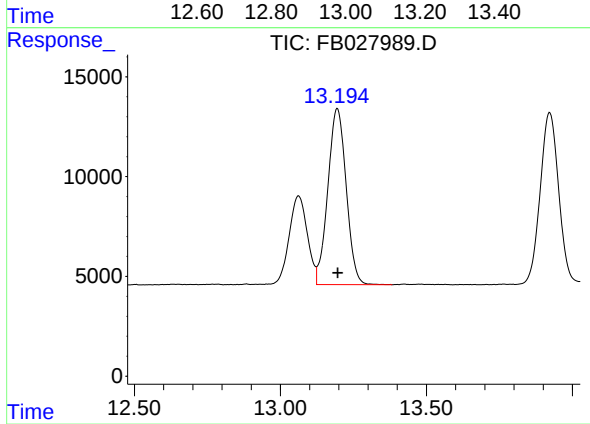

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 385994
Conc: 18.86 ng/ml

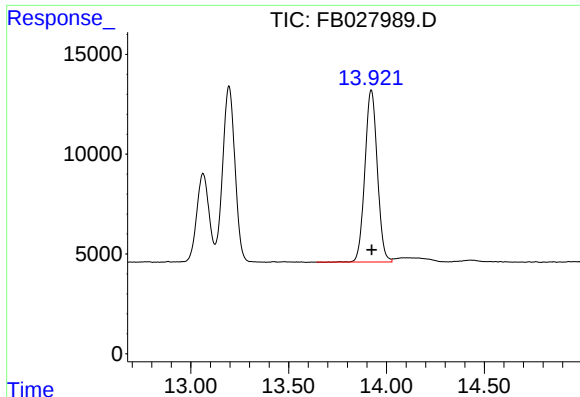

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 380220
Conc: 19.19 ng/ml

Instrument :
FID_B
ClientSampleId :
B-1MSD

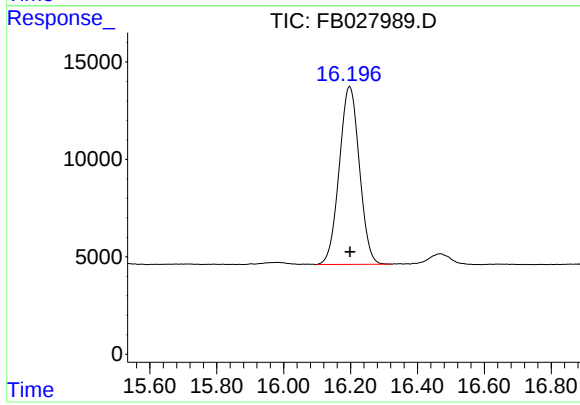

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.002 min
Response: 381394
Conc: 19.56 ng/ml