

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081822\
 Data File : FB027992.D
 Signal(s) : FID2B.CH
 Acq On : 18 Aug 2022 12:24
 Operator : AJ/MA
 Sample : VBF0818S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: SAMPLE.e
 Quant Time: Aug 18 16:17:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	260617	22.488 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.720	2053	0.113 ng/ml
2) t 2,2,4-Trimethylpentane	7.473	597	0.030 ng/ml
3) t n-Heptane	7.774	550	0.029 ng/ml
4) t Benzene	7.887	606	0.026 ng/ml
6) t Toluene	10.642	1027	0.047 ng/ml
7) t Ethylbenzene	13.069	1378	0.067 ng/ml
8) t m-Xylene	13.202	4069	0.199 ng/ml
9) t O-Xylene	13.940	1511	0.076 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	3918	0.201 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081822\
Data File : FB027992.D
Signal(s) : FID2B.CH
Acq On : 18 Aug 2022 12:24
Operator : AJ/MA
Sample : VBF0818S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: SAMPLE.e
Quant Time: Aug 18 16:17:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

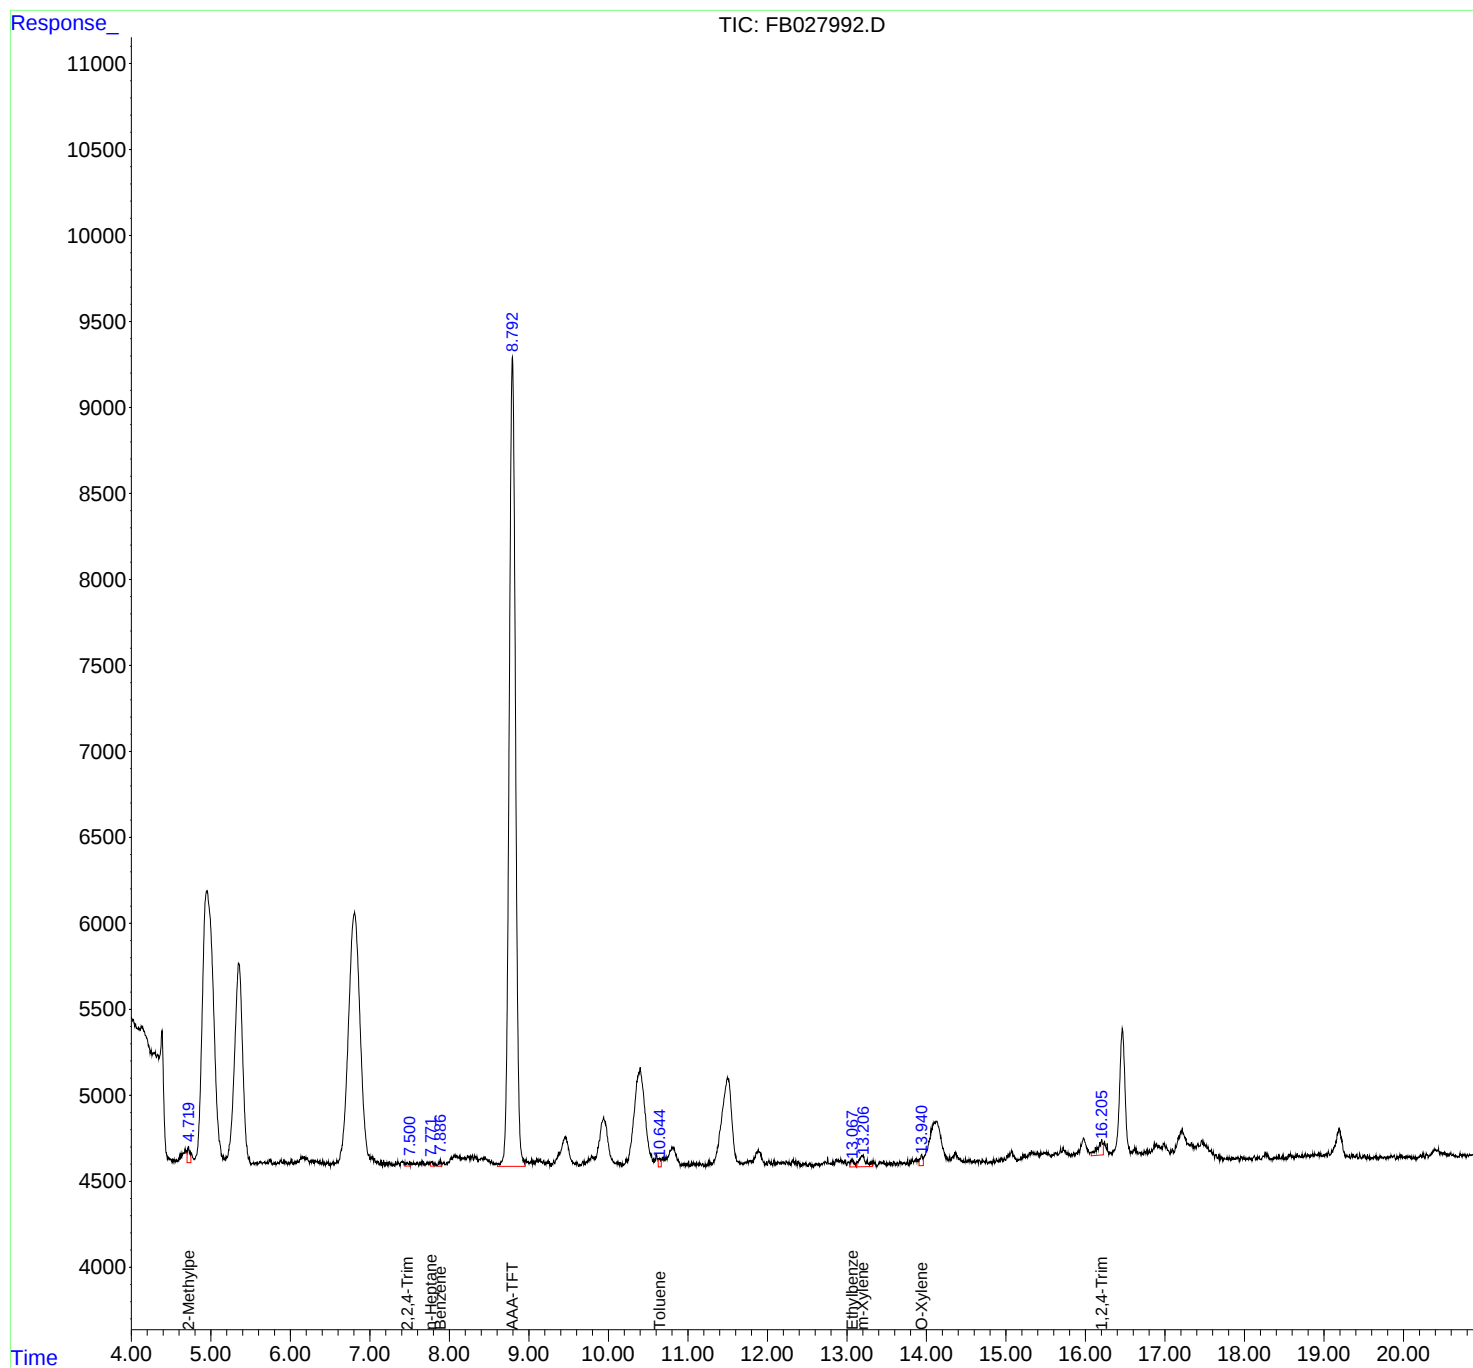


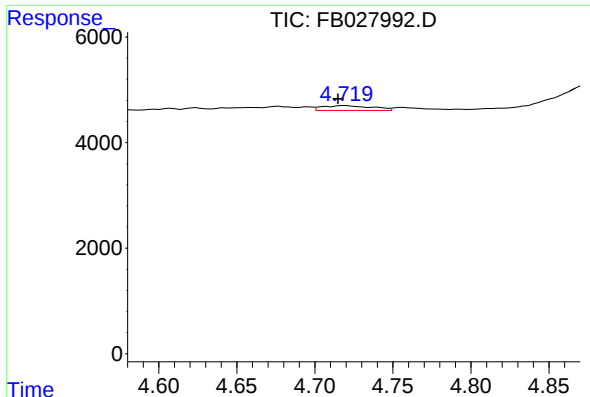

#1 2-Methylpentane


R.T.: 4.720 min
Delta R.T.: 0.005 min
Response: 2053
Conc: 0.11 ng/ml

Instrument :
FID_B
ClientSampleId :

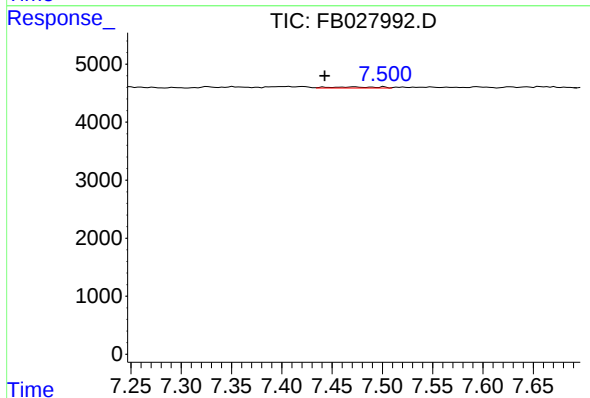


#2 2,2,4-Trimethylpentane

R.T.: 7.473 min
Delta R.T.: 0.030 min
Response: 597
Conc: 0.03 ng/ml

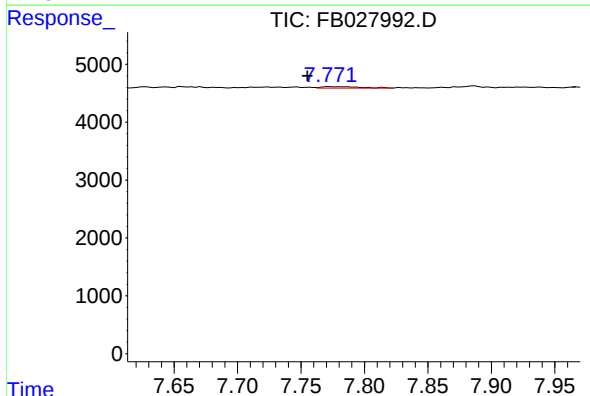


#3 n-Heptane

R.T.: 7.774 min
Delta R.T.: 0.019 min
Response: 550
Conc: 0.03 ng/ml

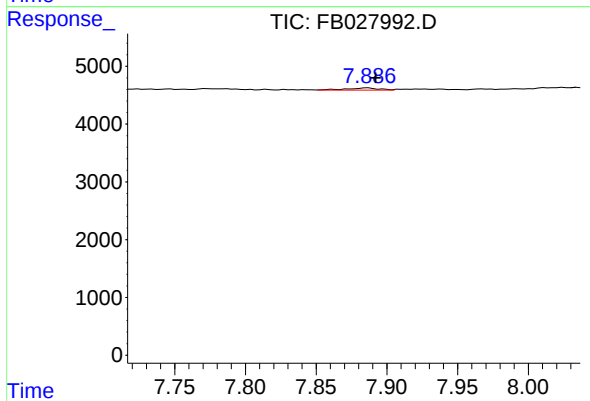

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.005 min
Response: 606
Conc: 0.03 ng/ml

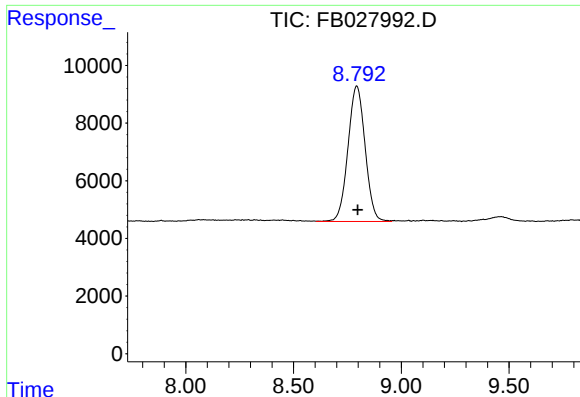

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: -0.004 min
Response: 260617
Conc: 22.49 ng/ml

Instrument :
FID_B
ClientSampleId :

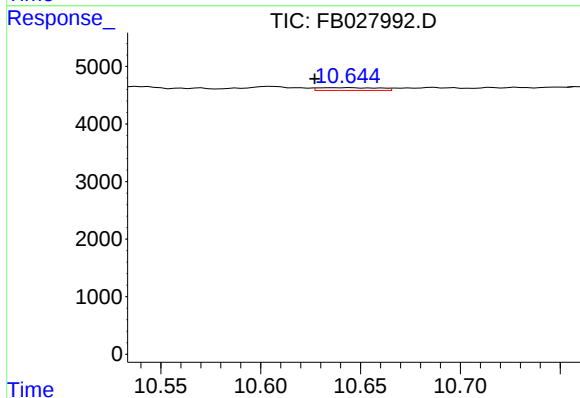


#6 Toluene

R.T.: 10.642 min
Delta R.T.: 0.014 min
Response: 1027
Conc: 0.05 ng/ml

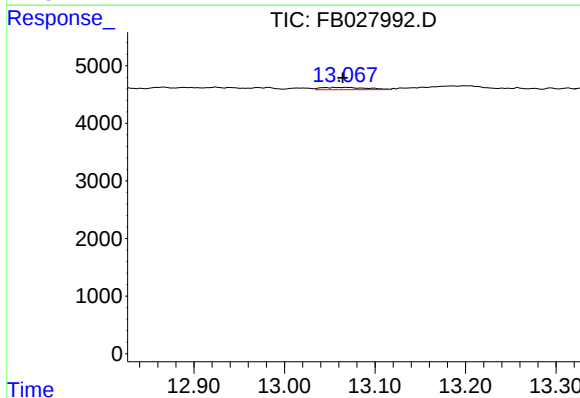


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.004 min
Response: 1378
Conc: 0.07 ng/ml

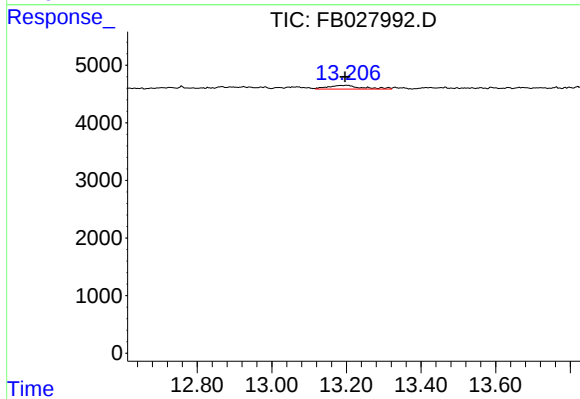

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: 0.005 min
Response: 4069
Conc: 0.20 ng/ml

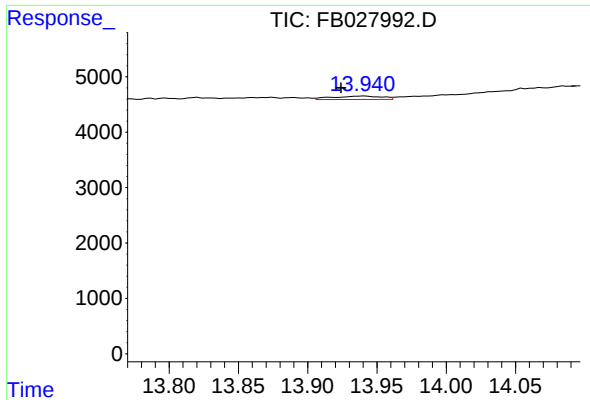

#9 O-Xylene

R.T.: 13.940 min
Delta R.T.: 0.016 min
Response: 1511
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :

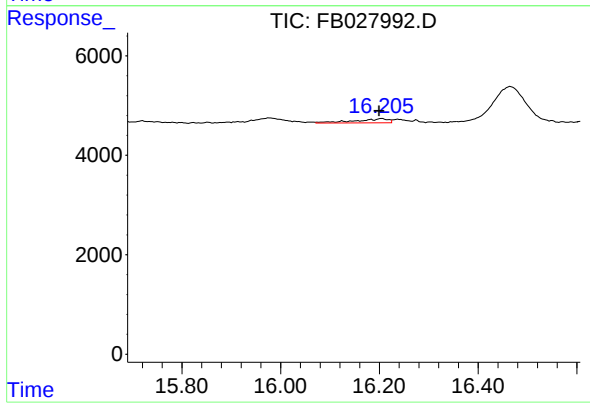

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.006 min
Response: 3918
Conc: 0.20 ng/ml