

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081822\
 Data File : FB027995.D
 Signal(s) : FID2B.CH
 Acq On : 18 Aug 2022 14:15
 Operator : AJ/MA
 Sample : N4243-01
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: SAMPLE.e
 Quant Time: Aug 18 16:17:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	223652	19.298 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	334	0.018 ng/ml
2) t 2,2,4-Trimethylpentane	7.454	509	0.026 ng/ml
3) t n-Heptane	7.747	319	0.017 ng/ml
4) t Benzene	7.883	818	0.035 ng/ml
6) t Toluene	10.620	5969	0.272 ng/ml
7) t Ethylbenzene	13.065	1108	0.054 ng/ml
8) t m-Xylene	13.194	4061	0.198 ng/ml
9) t O-Xylene	13.932	3364	0.170 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	4113	0.211 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081822\
Data File : FB027995.D
Signal(s) : FID2B.CH
Acq On : 18 Aug 2022 14:15
Operator : AJ/MA
Sample : N4243-01
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: SAMPLE.e
Quant Time: Aug 18 16:17:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

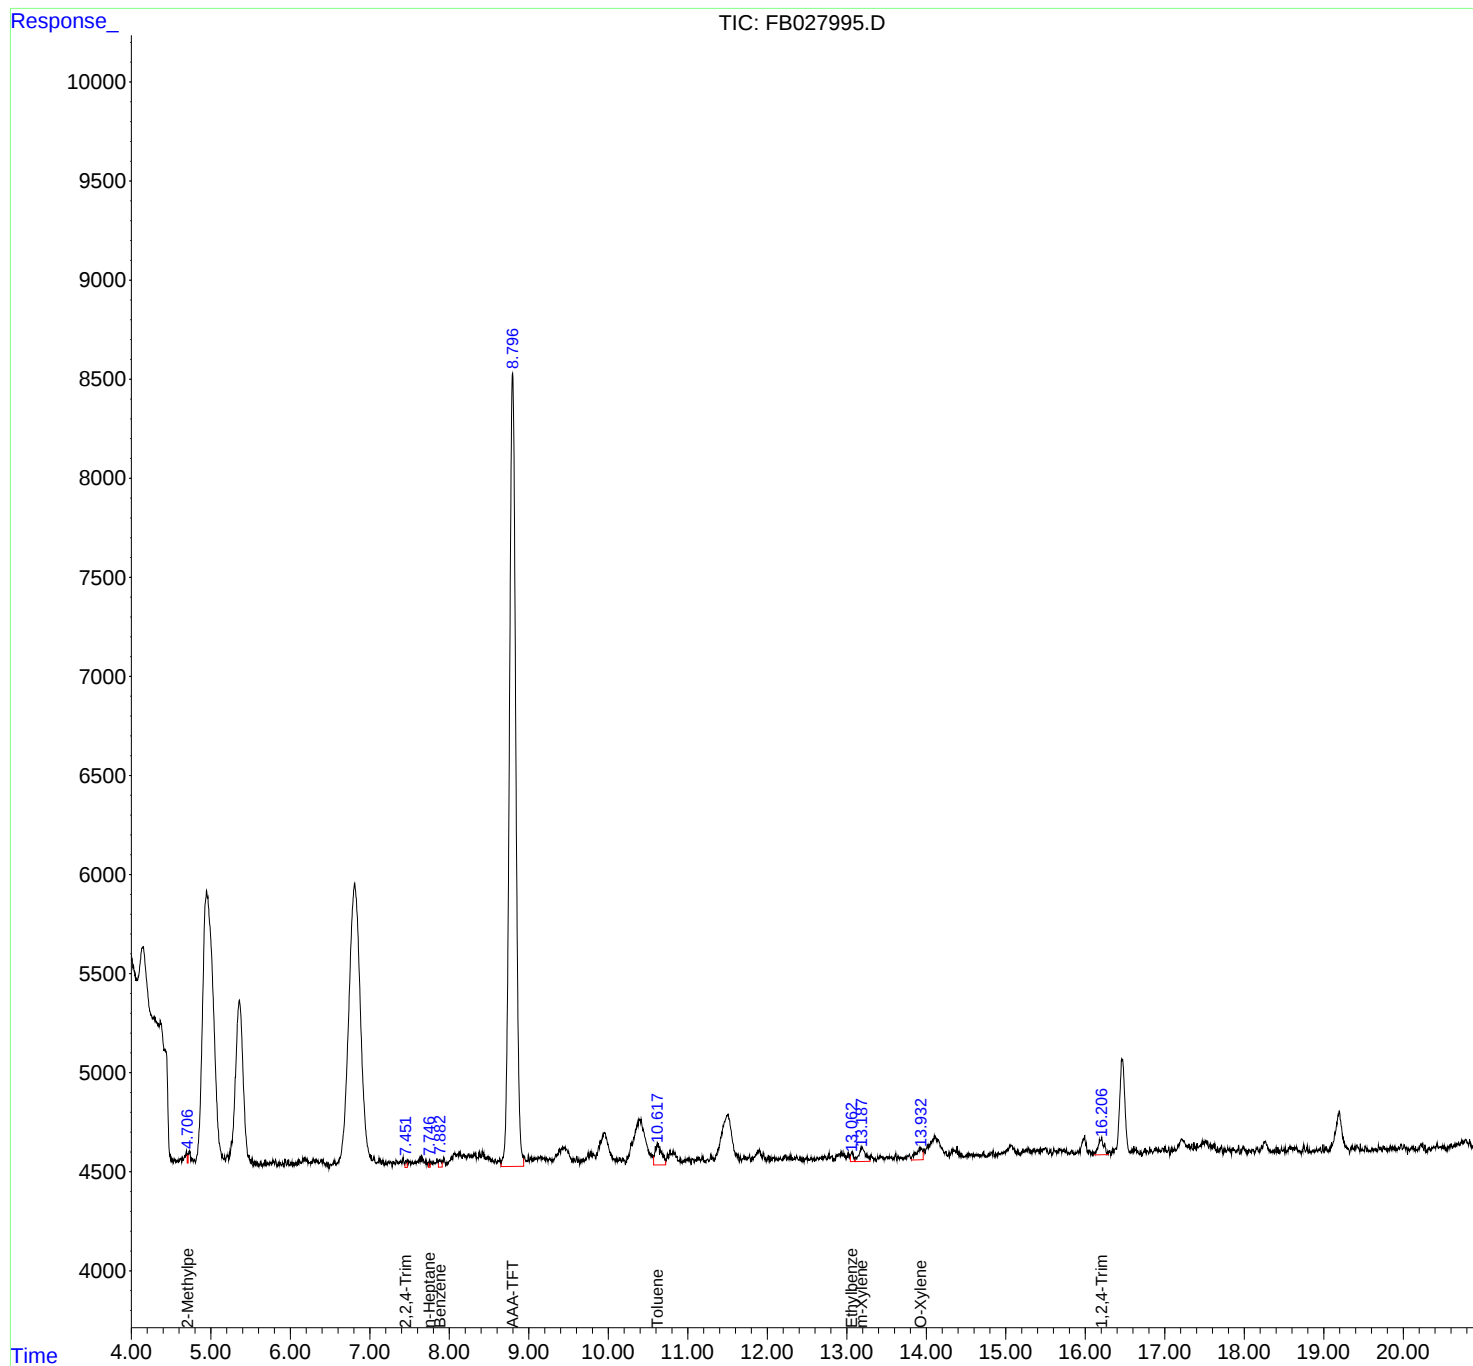


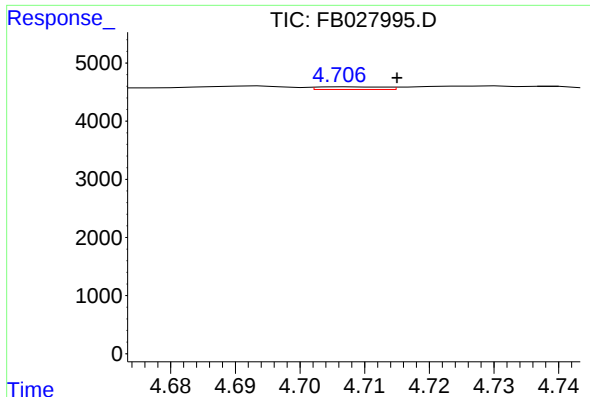

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.007 min
Response: 334
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :

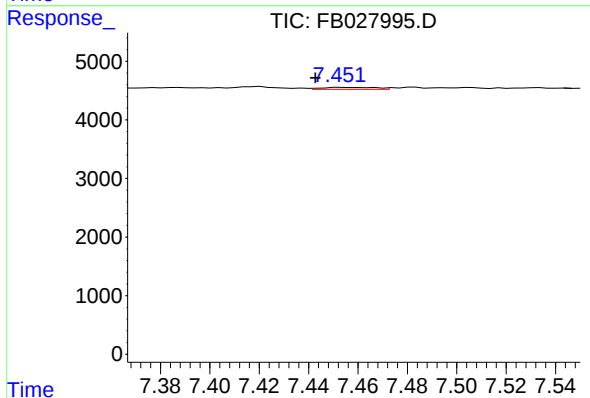


#2 2,2,4-Trimethylpentane

R.T.: 7.454 min
Delta R.T.: 0.012 min
Response: 509
Conc: 0.03 ng/ml

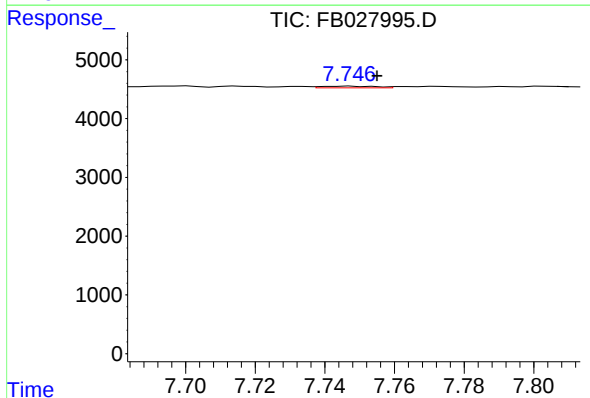


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.008 min
Response: 319
Conc: 0.02 ng/ml

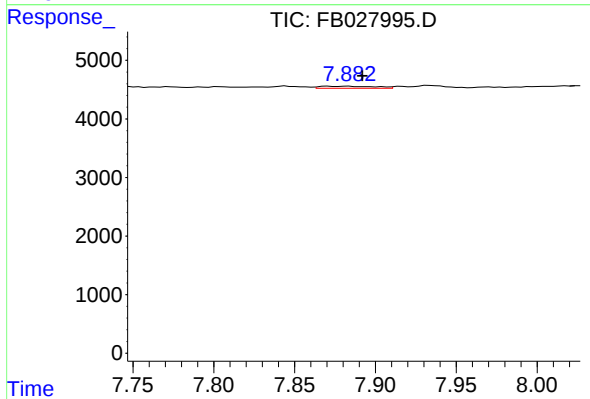

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.009 min
Response: 818
Conc: 0.04 ng/ml

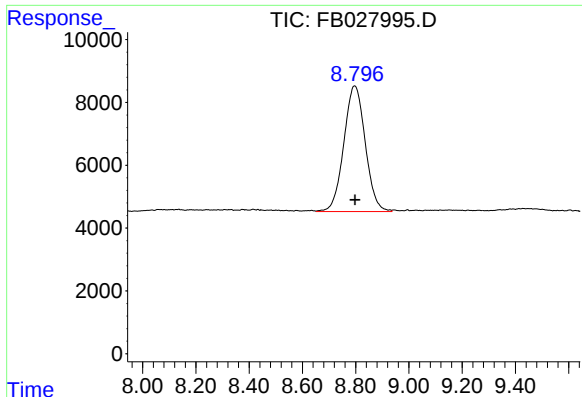

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 223652
Conc: 19.30 ng/ml

Instrument :
FID_B
ClientSampleId :

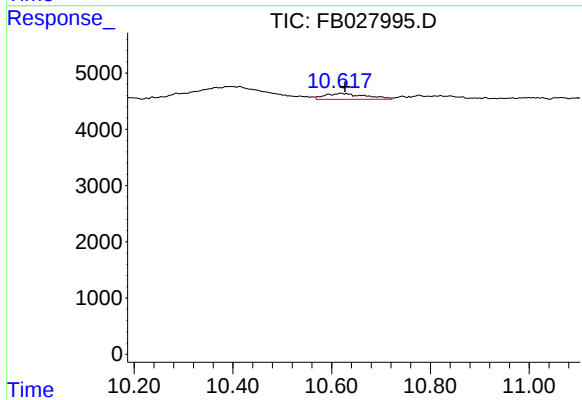


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.007 min
Response: 5969
Conc: 0.27 ng/ml

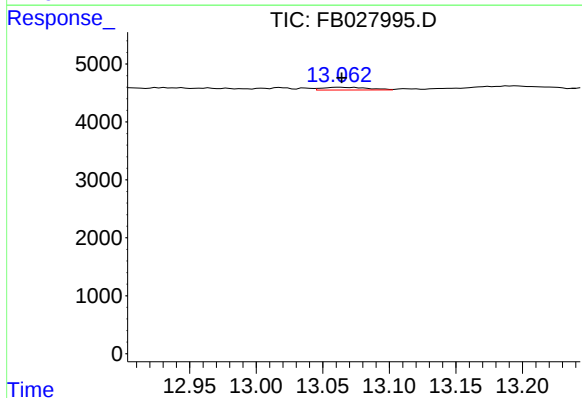


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.000 min
Response: 1108
Conc: 0.05 ng/ml

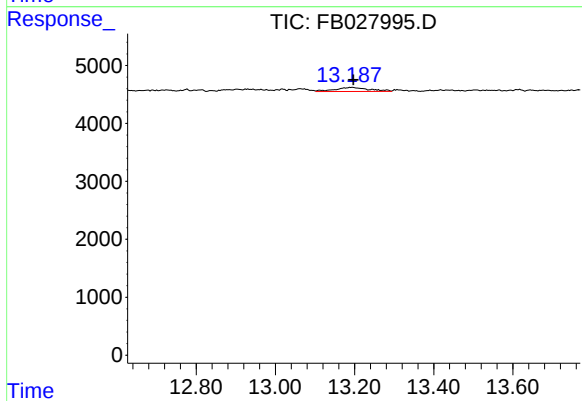

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.003 min
Response: 4061
Conc: 0.20 ng/ml

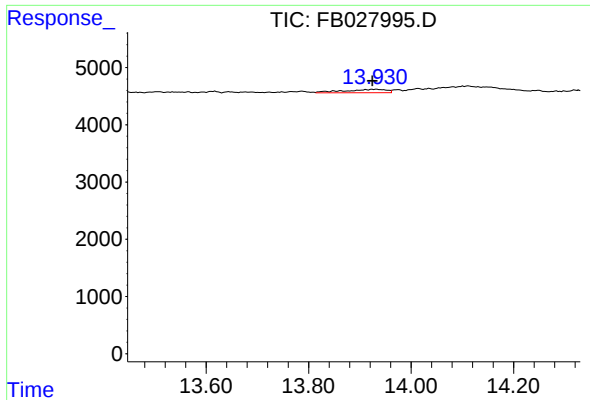

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.007 min
Response: 3364
Conc: 0.17 ng/ml

Instrument :
FID_B
ClientSampleId :

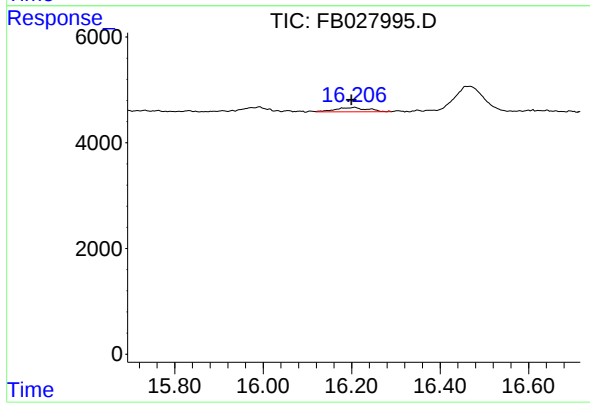

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.007 min
Response: 4113
Conc: 0.21 ng/ml