

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081822\
 Data File : FB027996.D
 Signal(s) : FID2B.CH
 Acq On : 18 Aug 2022 14:52
 Operator : AJ/MA
 Sample : N4243-01
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: SAMPLE.e
 Quant Time: Aug 18 16:17:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	108903	9.397 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	2540	0.140 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	784	0.040 ng/ml
3) t n-Heptane	7.778	1037	0.054 ng/ml
4) t Benzene	7.902	419	0.018 ng/ml
6) t Toluene	10.631	1221	0.056 ng/ml
7) t Ethylbenzene	13.062	1192	0.058 ng/ml
8) t m-Xylene	13.206	986	0.048 ng/ml
9) t O-Xylene	13.931	2004	0.101 ng/ml
10) t 1,2,4-Trimethylbenzene	16.240	3054	0.157 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081822\
Data File : FB027996.D
Signal(s) : FID2B.CH
Acq On : 18 Aug 2022 14:52
Operator : AJ/MA
Sample : N4243-01
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: SAMPLE.e
Quant Time: Aug 18 16:17:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

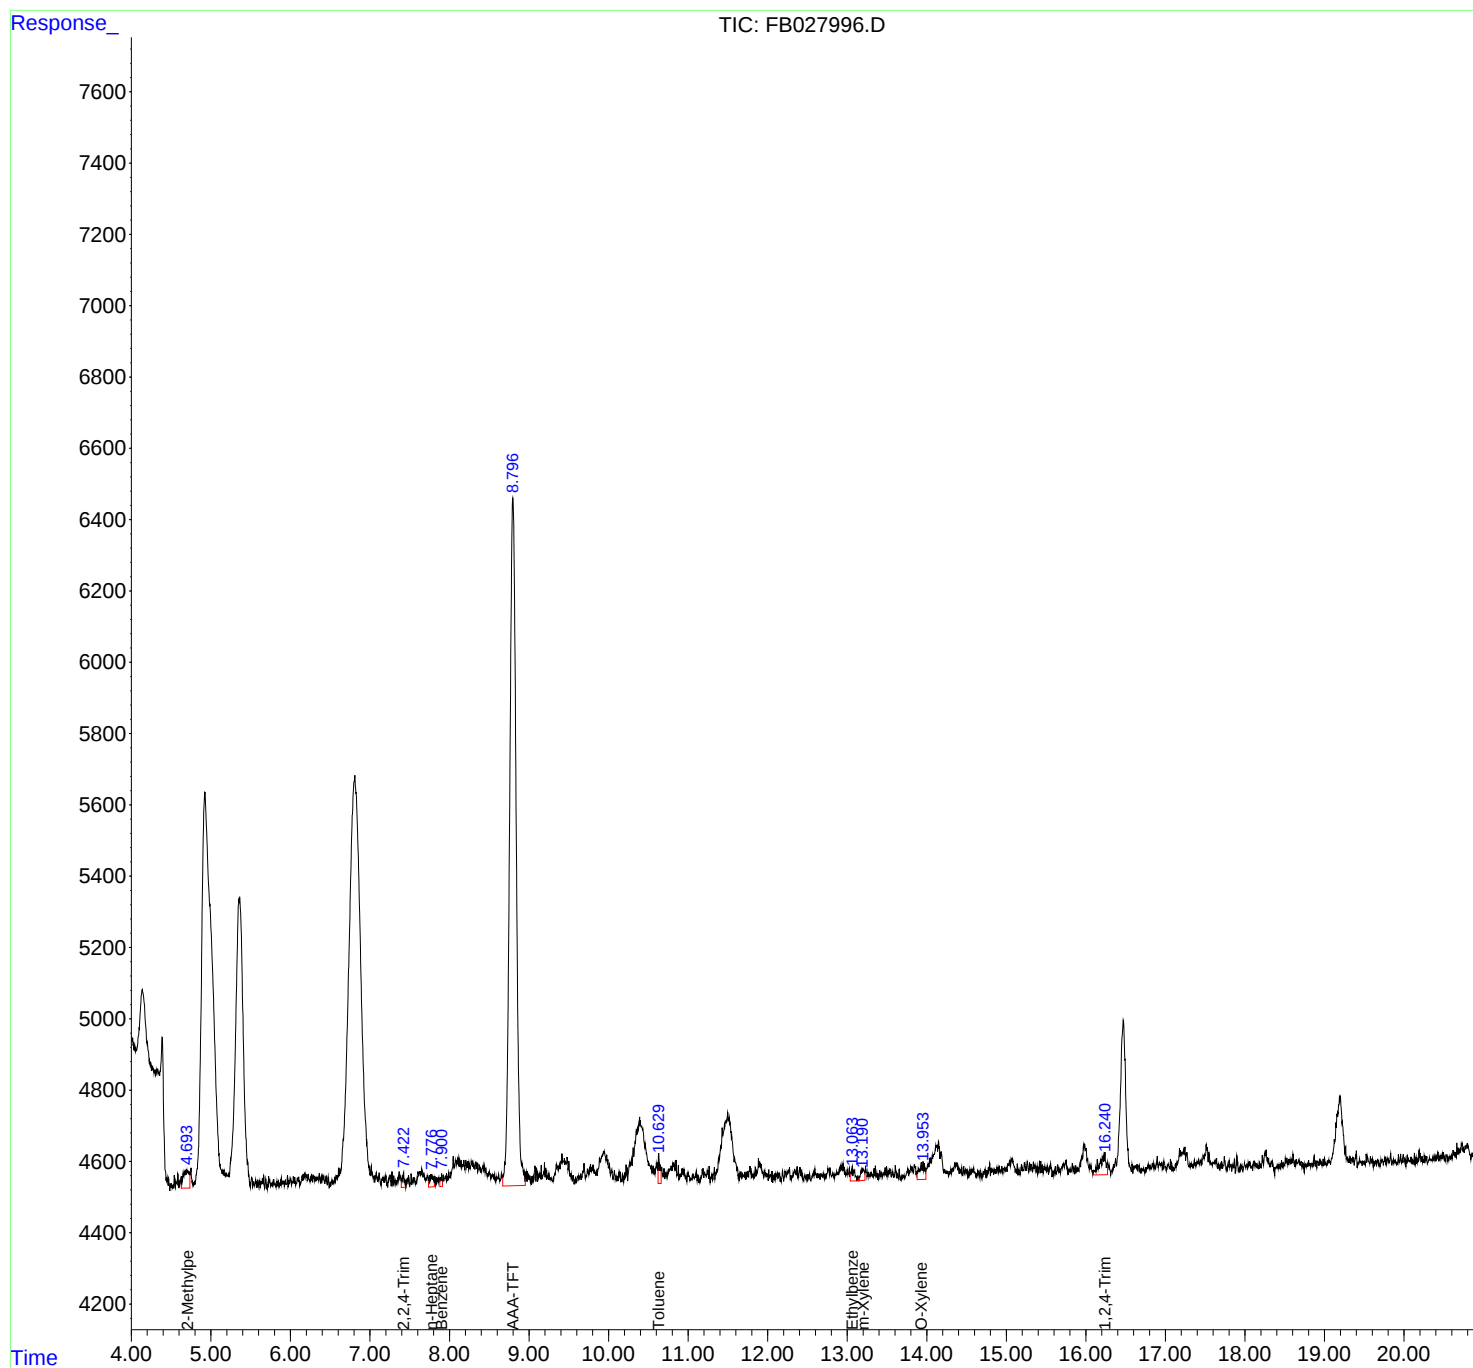


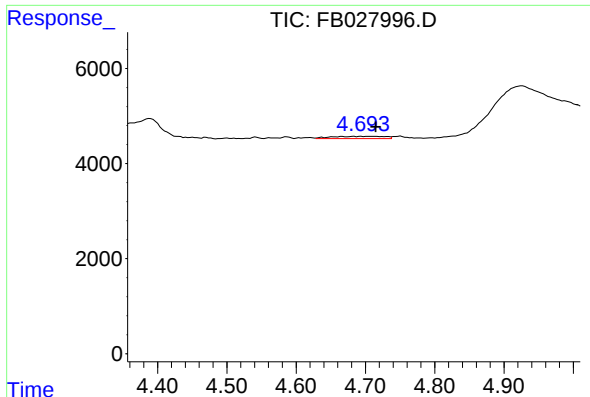

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: -0.003 min
Response: 2540
Conc: 0.14 ng/ml

Instrument :
FID_B
ClientSampleId :

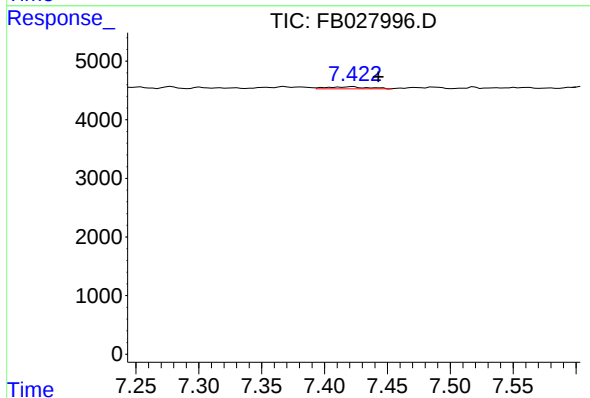


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.020 min
Response: 784
Conc: 0.04 ng/ml

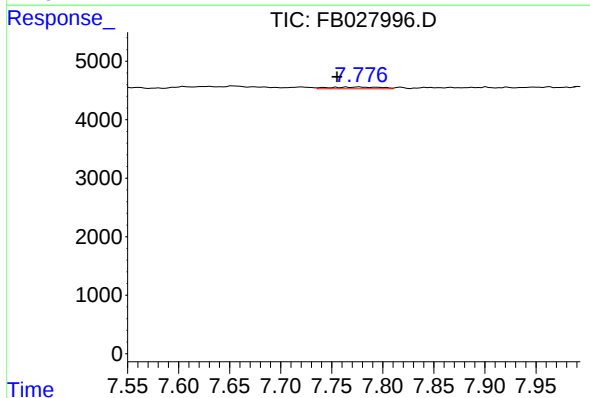


#3 n-Heptane

R.T.: 7.778 min
Delta R.T.: 0.023 min
Response: 1037
Conc: 0.05 ng/ml

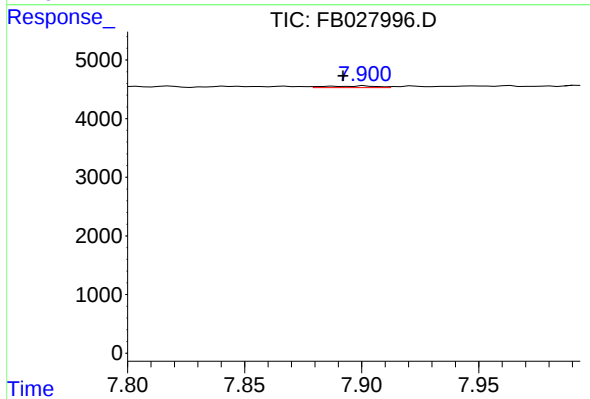

#4 Benzene


R.T.: 7.902 min
Delta R.T.: 0.010 min
Response: 419
Conc: 0.02 ng/ml

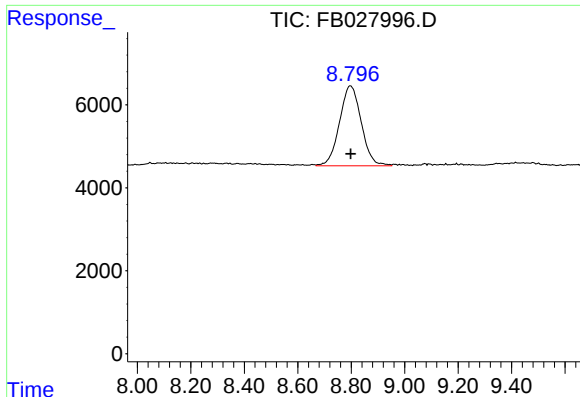

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 108903
Conc: 9.40 ng/ml

Instrument :
FID_B
ClientSampleId :

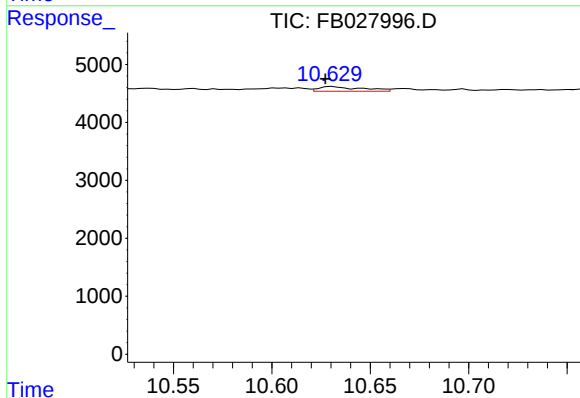


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.004 min
Response: 1221
Conc: 0.06 ng/ml

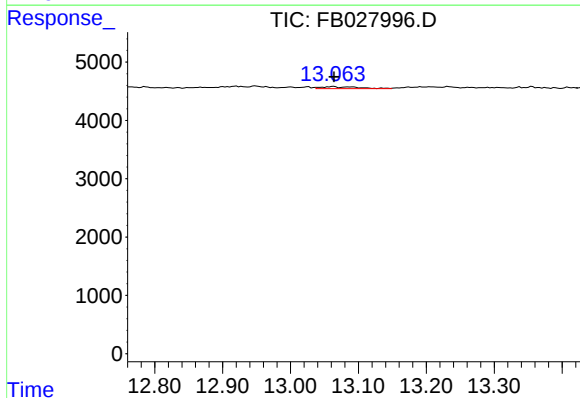


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.002 min
Response: 1192
Conc: 0.06 ng/ml

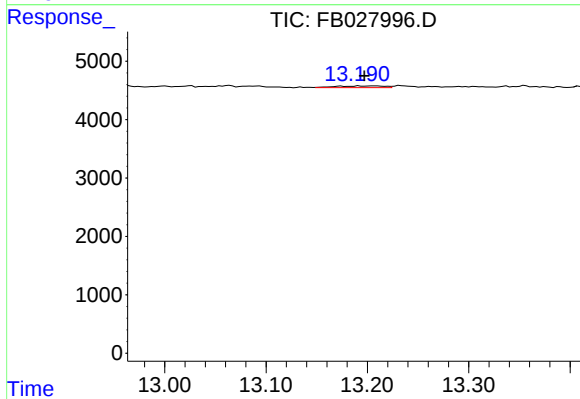

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.009 min
Response: 986
Conc: 0.05 ng/ml

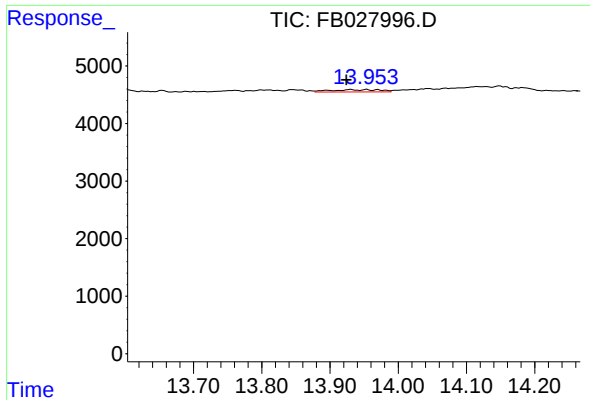

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.007 min
Response: 2004
Conc: 0.10 ng/ml

Instrument :
FID_B
ClientSampleId :

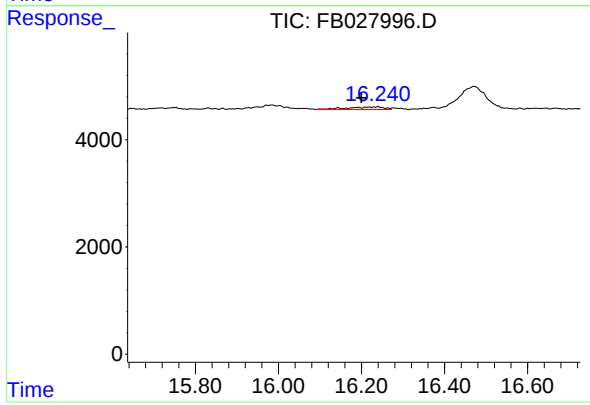

#10 1,2,4-Trimethylbenzene

R.T.: 16.240 min
Delta R.T.: 0.041 min
Response: 3054
Conc: 0.16 ng/ml