

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081922\
 Data File : FB028014.D
 Signal(s) : FID2B.CH
 Acq On : 19 Aug 2022 21:24
 Operator : AJ/MA
 Sample : N4260-01MS 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-T-4-(0-5)MS

Integration File: Calibration.e
 Quant Time: Aug 20 01:26:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	233477	20.146 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	548940	30.344 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	575047	29.324 ng/ml
3) t n-Heptane	7.753	198889	10.324 ng/ml
4) t Benzene	7.891	244388	10.511 ng/ml
6) t Toluene	10.625	677100	30.878 ng/ml
7) t Ethylbenzene	13.063	211277	10.253 ng/ml
8) t m-Xylene	13.196	414448	20.254 ng/ml
9) t O-Xylene	13.923	395093	19.945 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	360098	18.466 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081922\
Data File : FB028014.D
Signal(s) : FID2B.CH
Acq On : 19 Aug 2022 21:24
Operator : AJ/MA
Sample : N4260-01MS 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-T-4-(0-5)MS

Integration File: Calibration.e
Quant Time: Aug 20 01:26:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

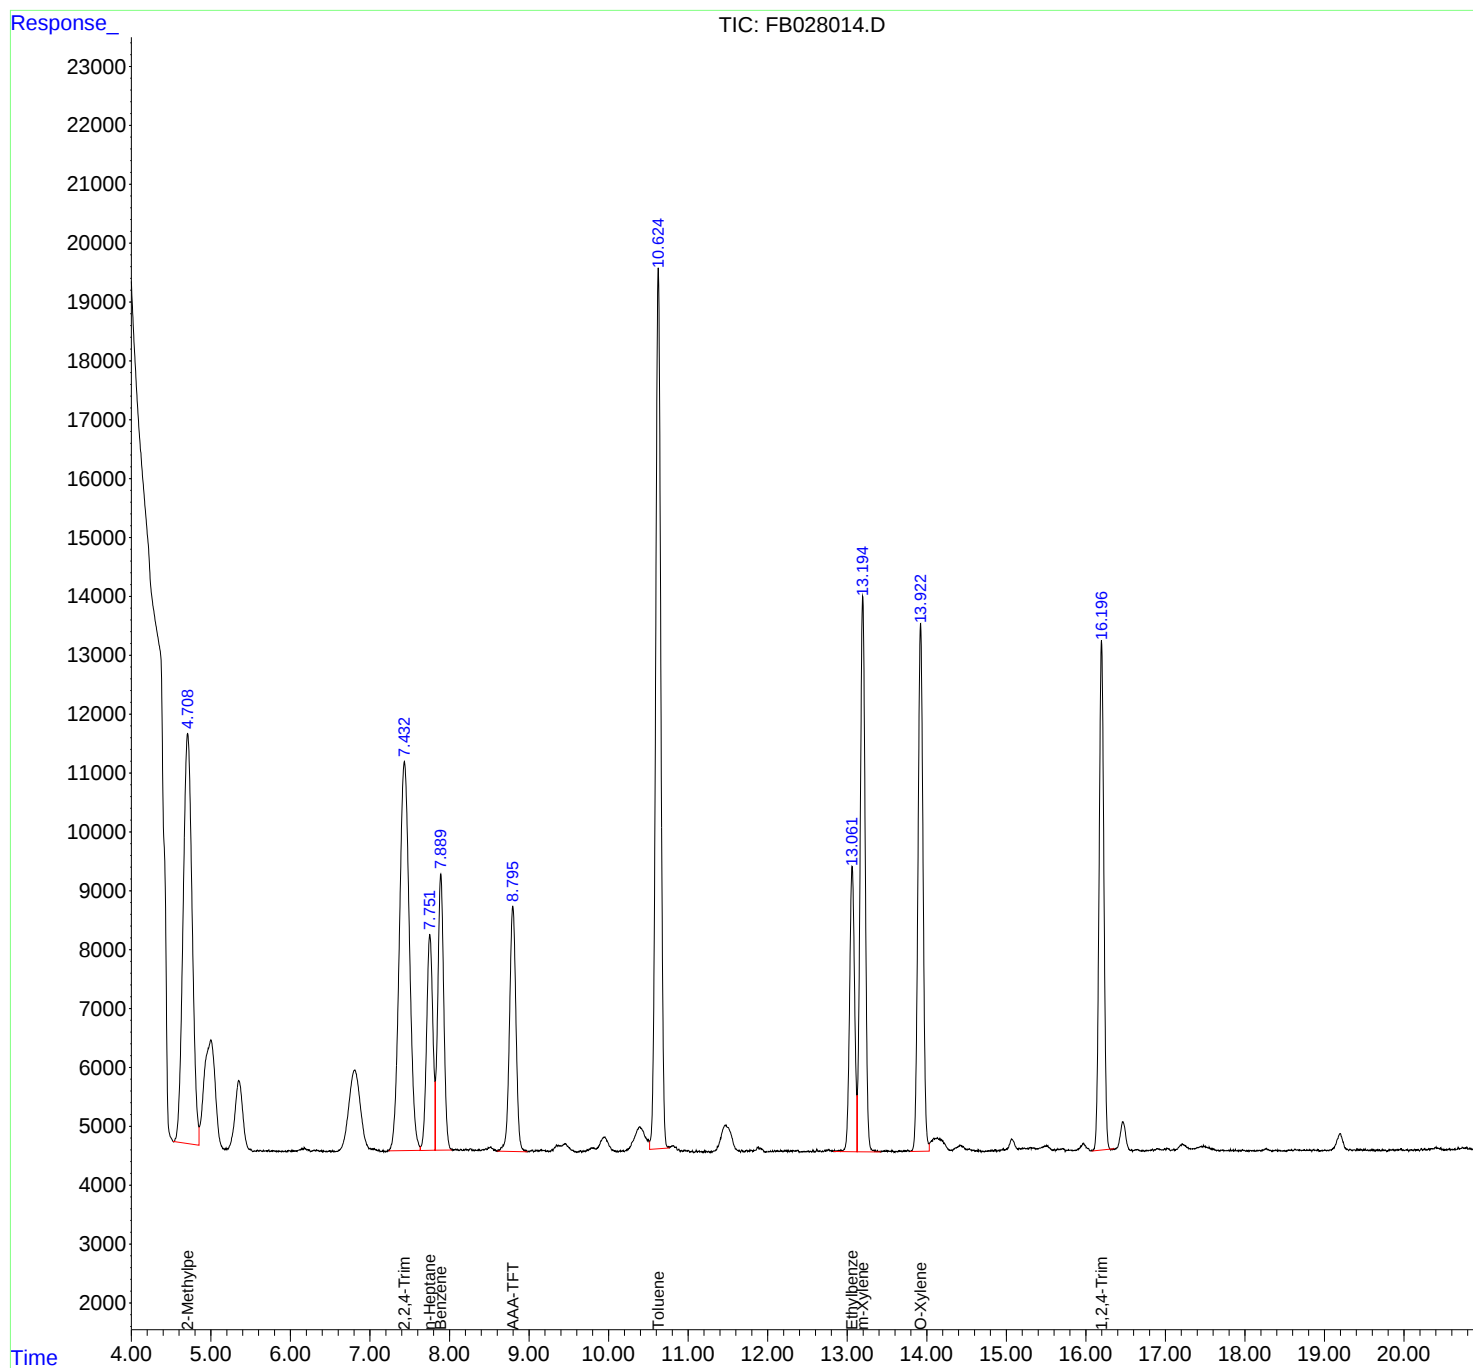


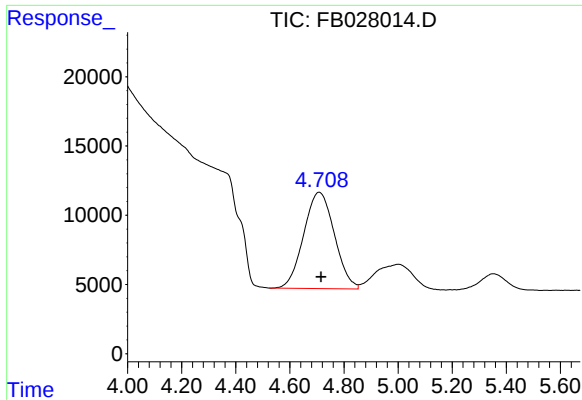

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: -0.006 min
Response: 548940
Conc: 30.34 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-4-(0-5)MS

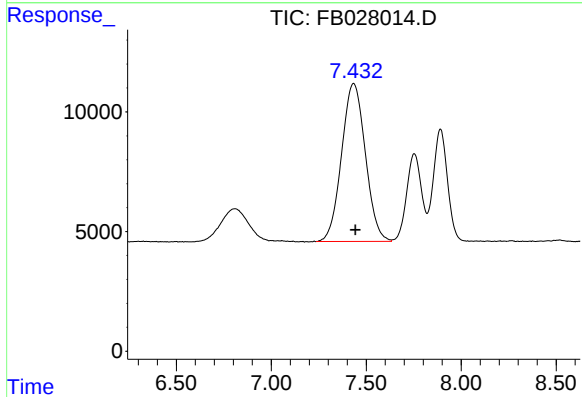


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: -0.009 min
Response: 575047
Conc: 29.32 ng/ml

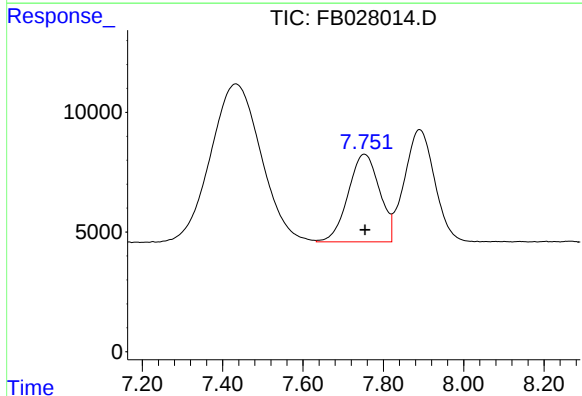


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 198889
Conc: 10.32 ng/ml

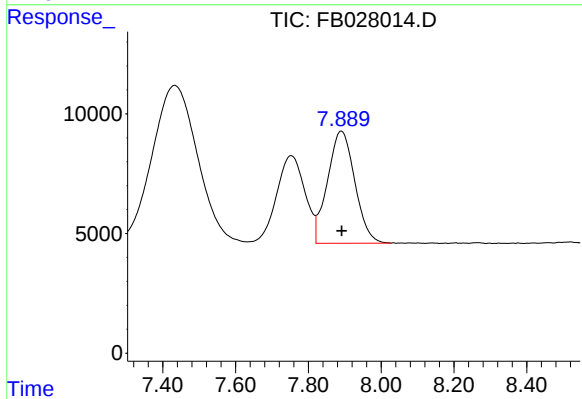

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 244388
Conc: 10.51 ng/ml

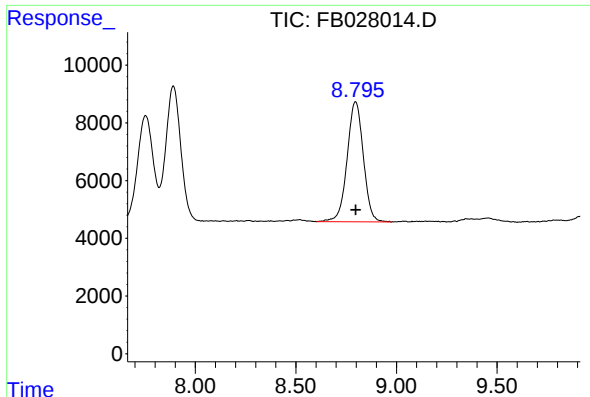

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 233477
Conc: 20.15 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-4-(0-5)MS

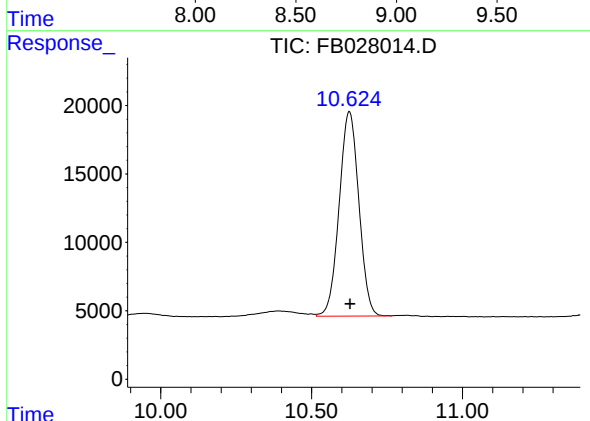


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.002 min
Response: 677100
Conc: 30.88 ng/ml

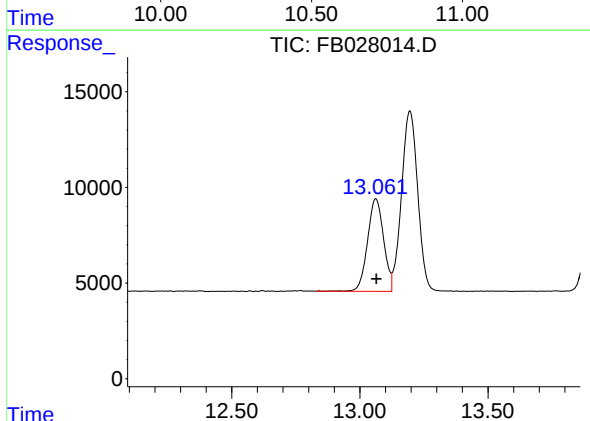


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.002 min
Response: 211277
Conc: 10.25 ng/ml

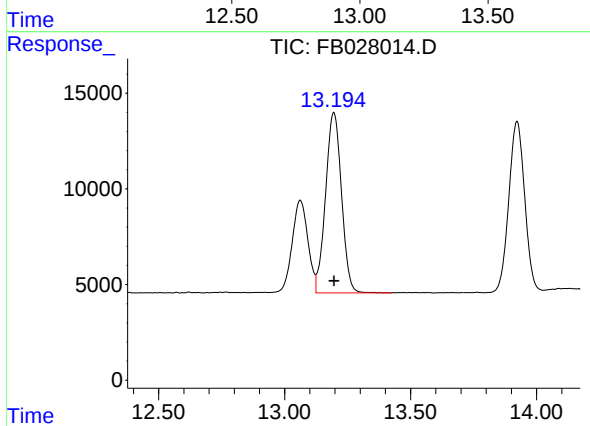

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.001 min
Response: 414448
Conc: 20.25 ng/ml

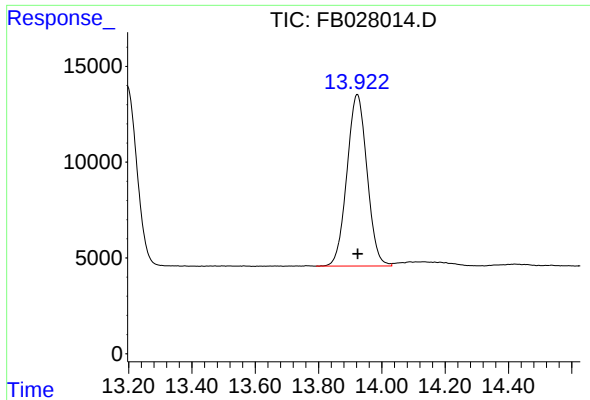

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.001 min
Response: 395093
Conc: 19.95 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-4-(0-5)MS

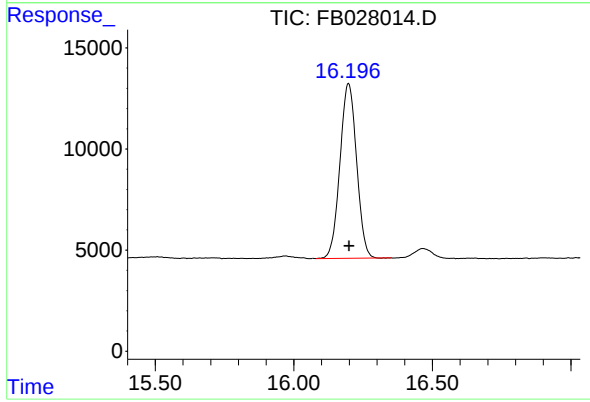

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.002 min
Response: 360098
Conc: 18.47 ng/ml