

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081922\
 Data File : FB028015.D
 Signal(s) : FID2B.CH
 Acq On : 19 Aug 2022 22:01
 Operator : AJ/MA
 Sample : N4260-01MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-T-4-(0-5)MSD

Integration File: Calibration.e
 Quant Time: Aug 20 01:26:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
 Quant Title :
 QLast Update : Tue Aug 09 12:12:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	248511	21.443 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	591642	32.704 ng/ml
2) t 2,2,4-Trimethylpentane	7.438	682392	34.798 ng/ml
3) t n-Heptane	7.753	225410	11.700 ng/ml
4) t Benzene	7.891	273780	11.775 ng/ml
6) t Toluene	10.625	748780	34.147 ng/ml
7) t Ethylbenzene	13.063	233436	11.328 ng/ml
8) t m-Xylene	13.196	458261	22.395 ng/ml
9) t O-Xylene	13.922	442975	22.362 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	412622	21.159 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB081922\
Data File : FB028015.D
Signal(s) : FID2B.CH
Acq On : 19 Aug 2022 22:01
Operator : AJ/MA
Sample : N4260-01MSD 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-T-4-(0-5)MSD

Integration File: Calibration.e
Quant Time: Aug 20 01:26:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB080922.M
Quant Title :
QLast Update : Tue Aug 09 12:12:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

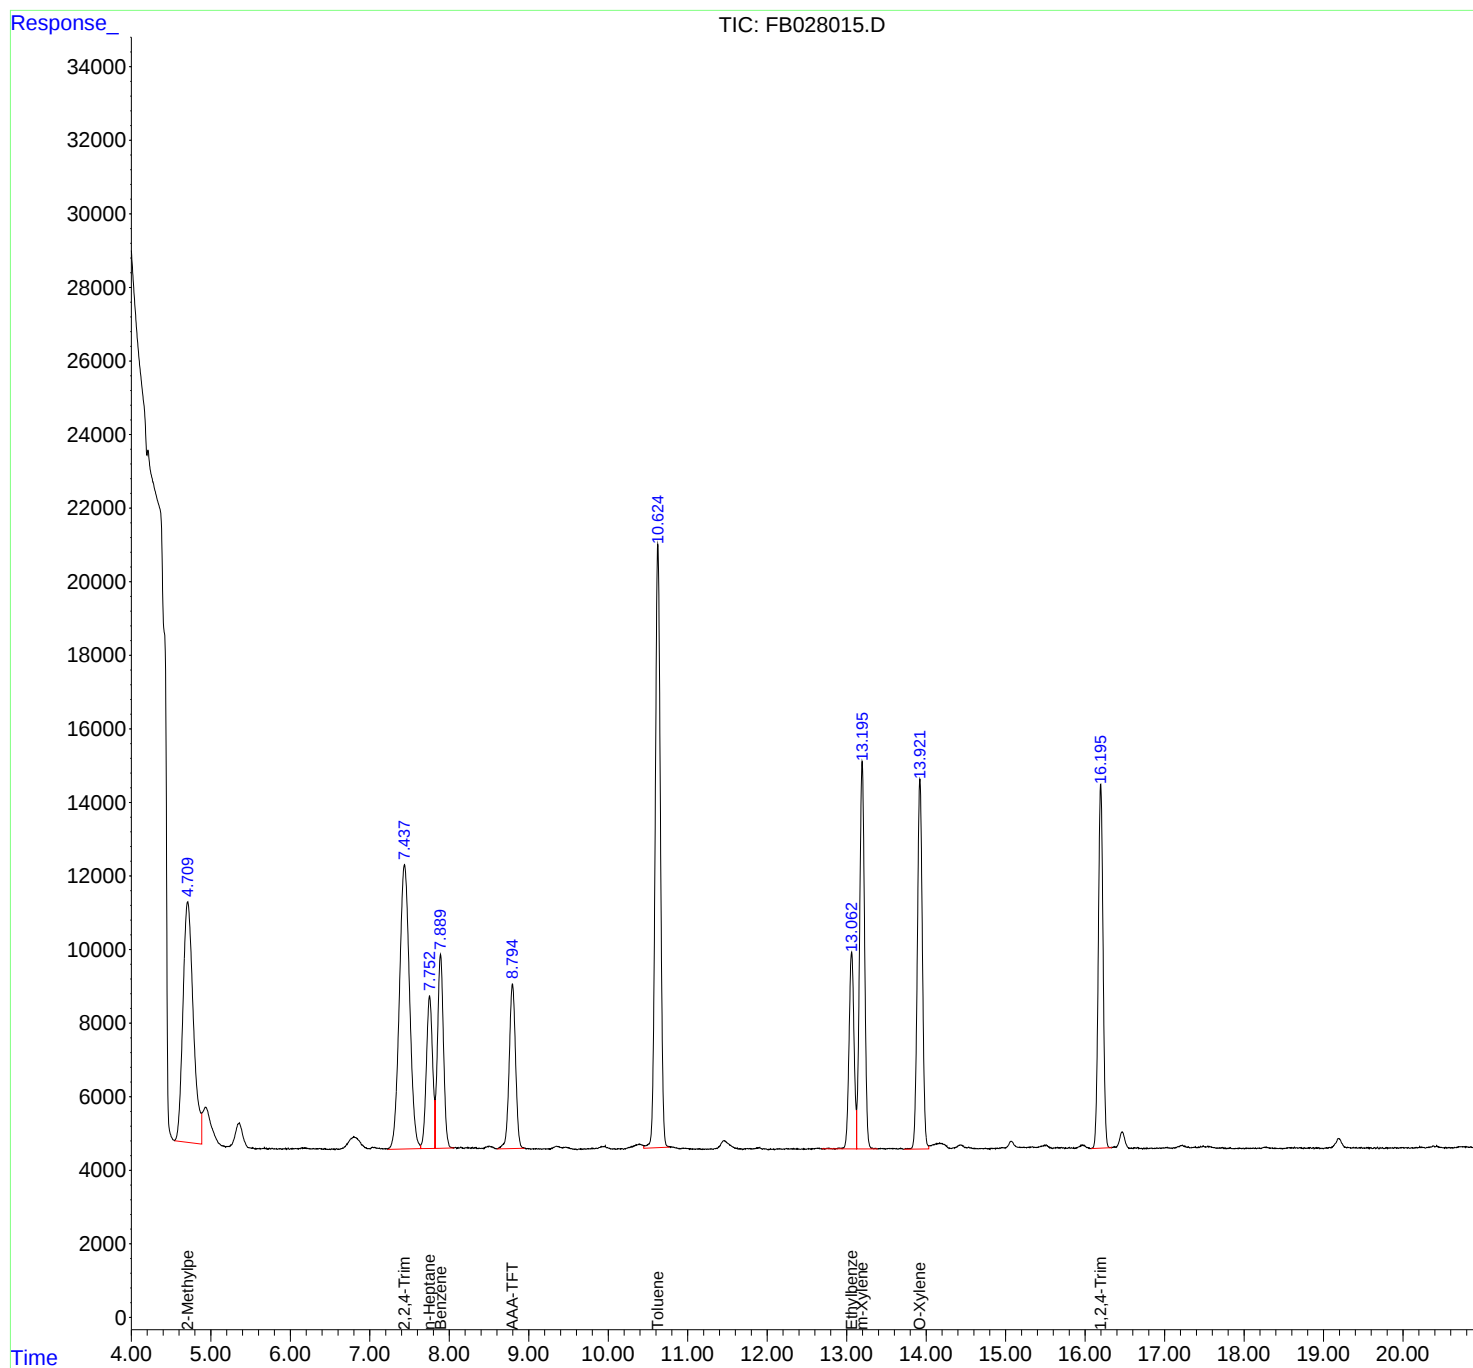


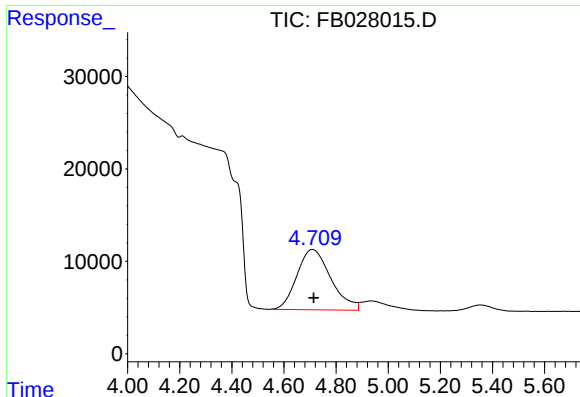

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: -0.005 min
Response: 591642
Conc: 32.70 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-4-(0-5)MSD

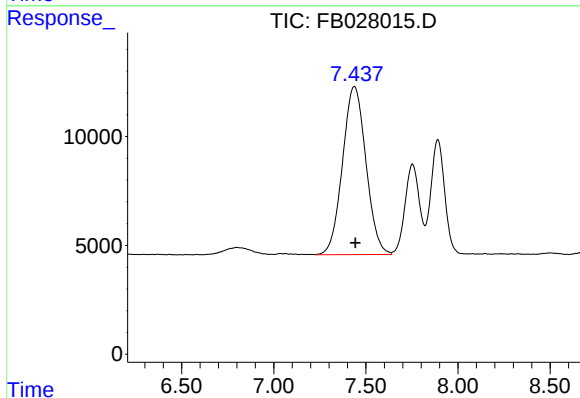


#2 2,2,4-Trimethylpentane

R.T.: 7.438 min
Delta R.T.: -0.005 min
Response: 682392
Conc: 34.80 ng/ml

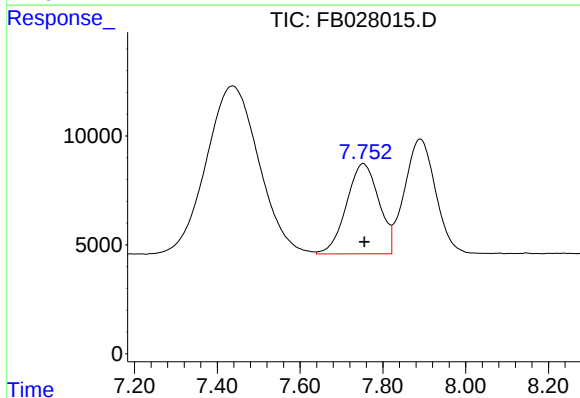


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 225410
Conc: 11.70 ng/ml

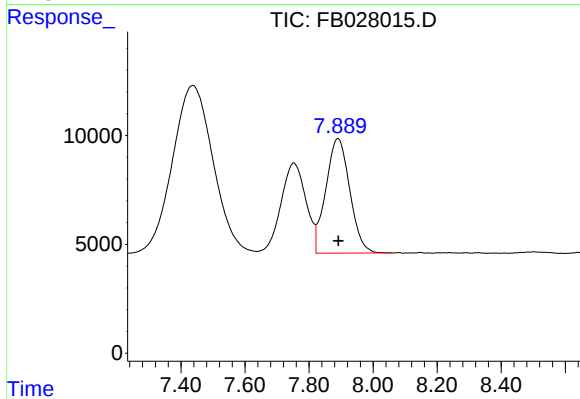

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 273780
Conc: 11.77 ng/ml

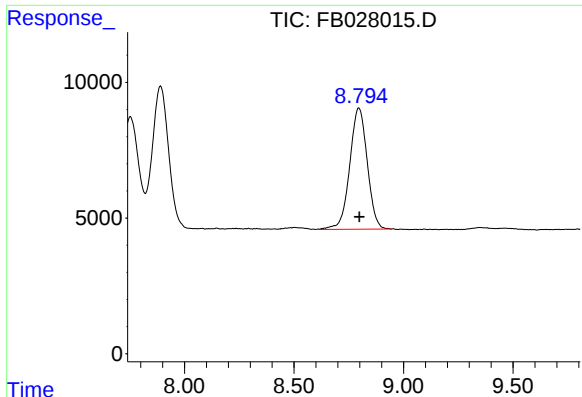

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.002 min
Response: 248511
Conc: 21.44 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-4-(0-5)MSD

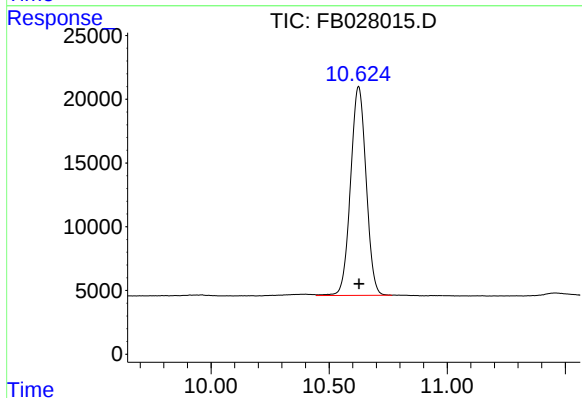


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.002 min
Response: 748780
Conc: 34.15 ng/ml

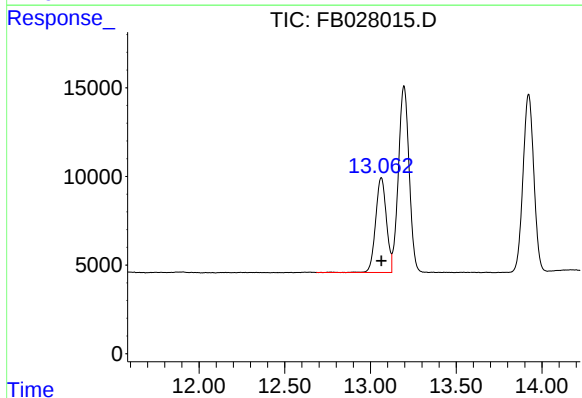


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.001 min
Response: 233436
Conc: 11.33 ng/ml

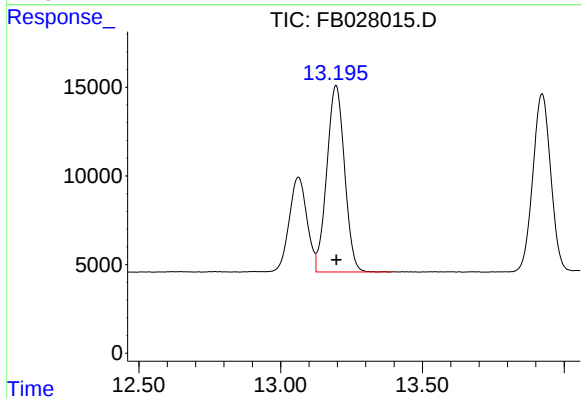

#8 m-Xylene


R.T.: 13.196 min
Delta R.T.: -0.001 min
Response: 458261
Conc: 22.40 ng/ml

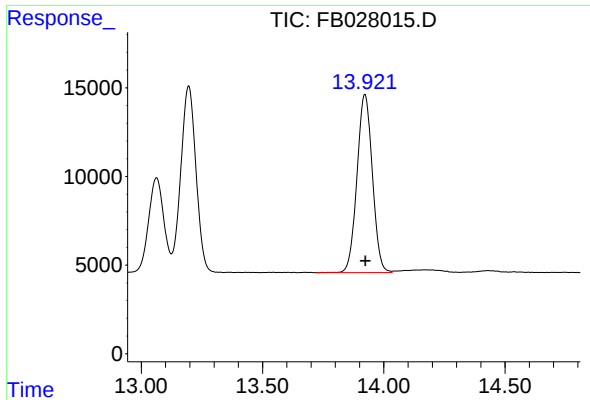

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.002 min
Response: 442975
Conc: 22.36 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-T-4-(0-5)MSD

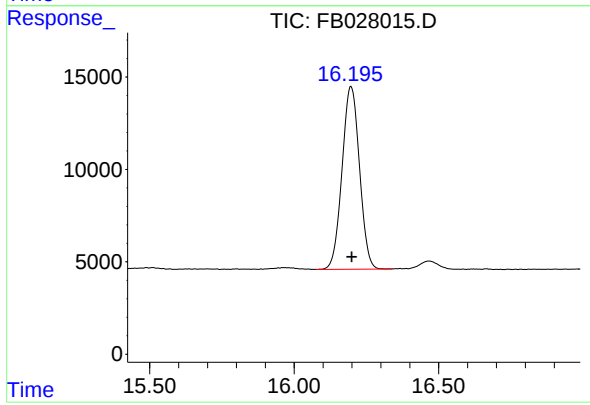

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: -0.002 min
Response: 412622
Conc: 21.16 ng/ml