

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082019\
 Data File : FB022045.D
 Signal(s) : FID2B.CH
 Acq On : 20 Aug 2019 16:39
 Operator : DD/AJ
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Aug 21 07:57:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:54:48 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.980	108034	5.161 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	281648	6.999 ng/ml
2) t 2,2,4-Trimethylpentane	7.599	280400	6.987 ng/ml
3) t n-Heptane	7.933	90408	2.376 ng/ml
4) t Benzene	8.073	106241	2.317 ng/ml
6) t Toluene	10.820	222784	6.999 ng/ml
7) t Ethylbenzene	13.267	52972	2.569 ng/ml
8) t m-Xylene	13.401	111141	5.304 ng/ml
9) t O-Xylene	14.129	120588	5.472 ng/ml
10) t 1,2,4-Trimethylbenzene	16.407	150945	6.225 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082019\
Data File : FB022045.D
Signal(s) : FID2B.CH
Acq On : 20 Aug 2019 16:39
Operator : DD/AJ
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Aug 21 07:57:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:54:48 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

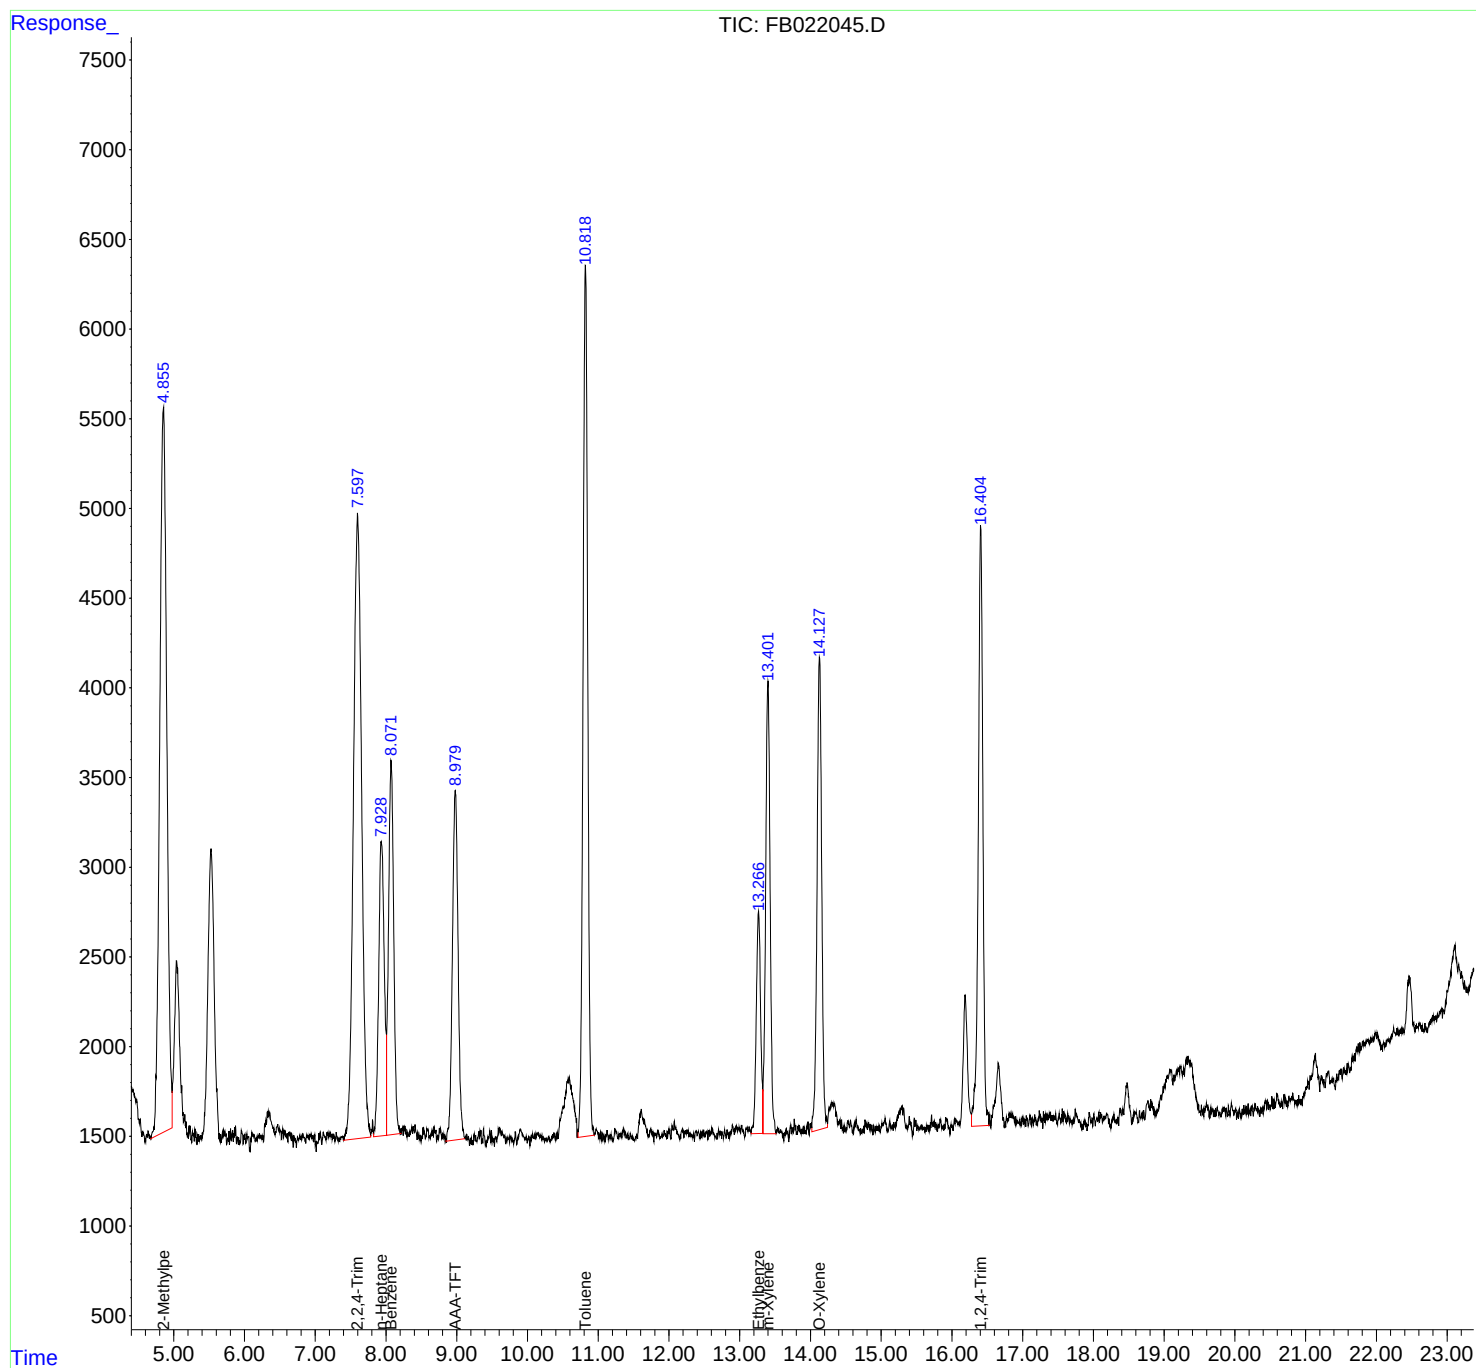


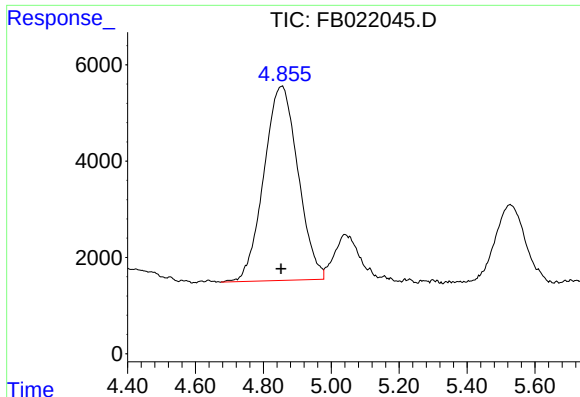

#1 2-Methylpentane


R.T.: 4.855 min
Delta R.T.: 0.003 min
Response: 281648
Conc: 7.00 ng/ml

Instrument :
FID_B
ClientSampleId :

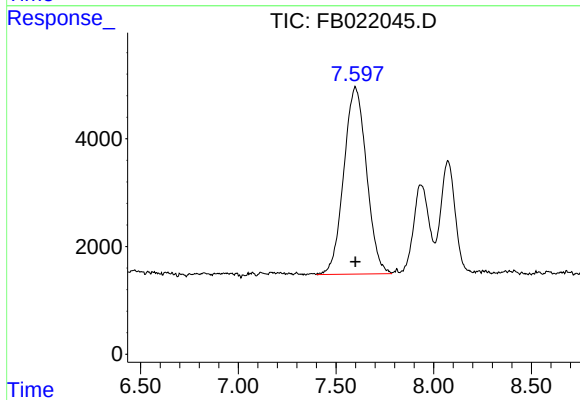


#2 2,2,4-Trimethylpentane

R.T.: 7.599 min
Delta R.T.: -0.001 min
Response: 280400
Conc: 6.99 ng/ml

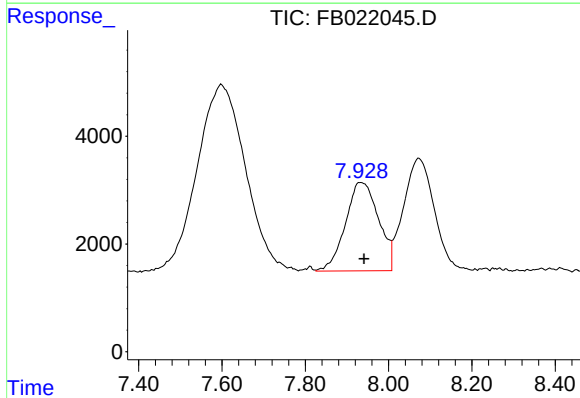


#3 n-Heptane

R.T.: 7.933 min
Delta R.T.: -0.008 min
Response: 90408
Conc: 2.38 ng/ml

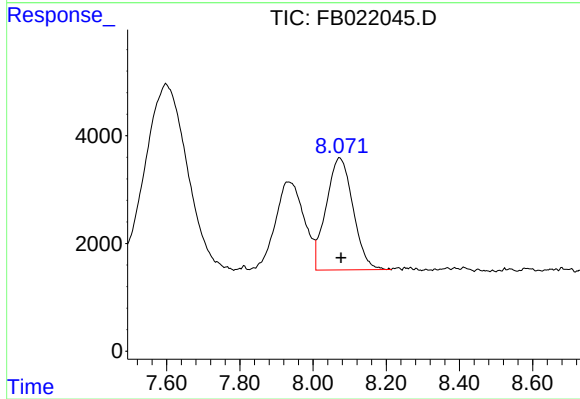

#4 Benzene


R.T.: 8.073 min
Delta R.T.: -0.003 min
Response: 106241
Conc: 2.32 ng/ml

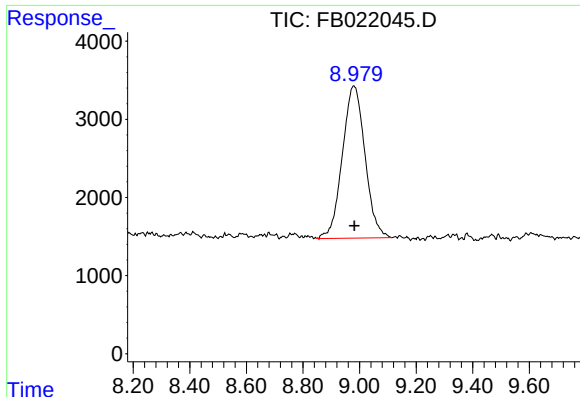

#5 AAA-TFT


R.T.: 8.980 min
Delta R.T.: -0.002 min
Response: 108034
Conc: 5.16 ng/ml

Instrument :
FID_B
ClientSampleId :

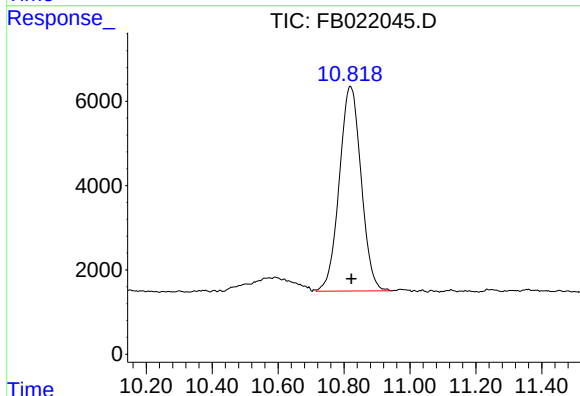


#6 Toluene

R.T.: 10.820 min
Delta R.T.: -0.003 min
Response: 222784
Conc: 7.00 ng/ml

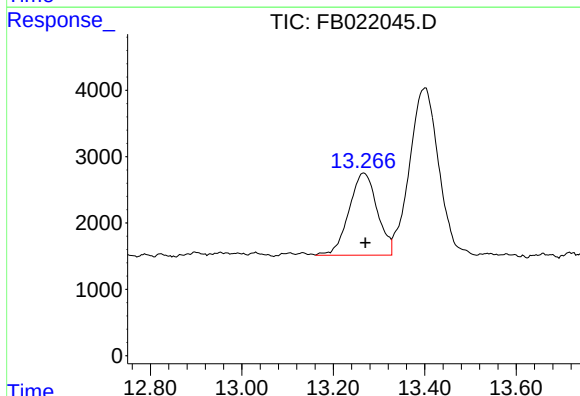


#7 Ethylbenzene

R.T.: 13.267 min
Delta R.T.: -0.003 min
Response: 52972
Conc: 2.57 ng/ml

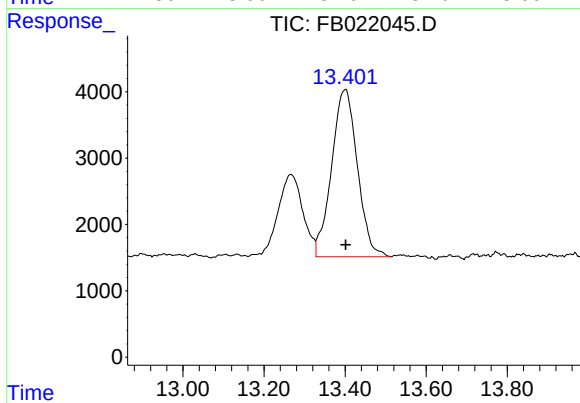

#8 m-Xylene


R.T.: 13.401 min
Delta R.T.: 0.000 min
Response: 111141
Conc: 5.30 ng/ml

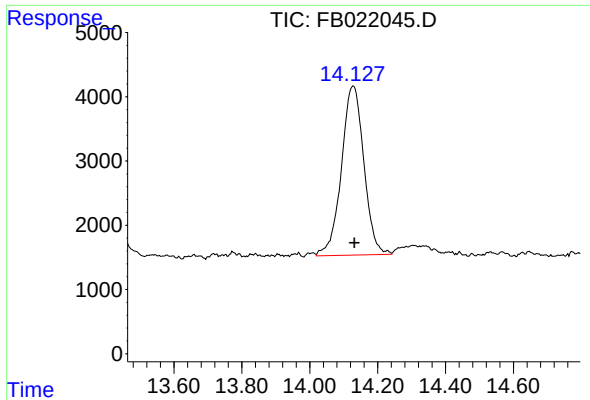

#9 O-Xylene

R.T.: 14.129 min
Delta R.T.: -0.003 min
Response: 120588
Conc: 5.47 ng/ml

Instrument :
FID_B
ClientSampleId :

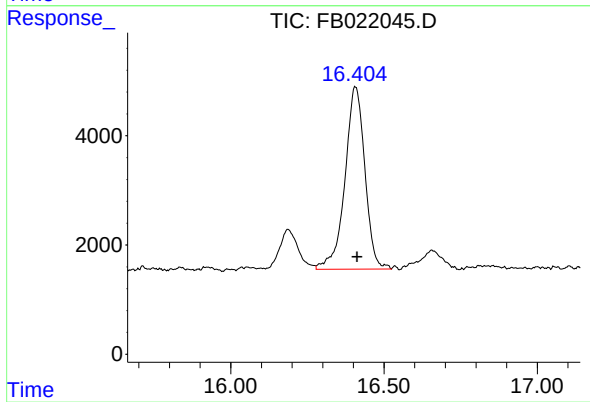

#10 1,2,4-Trimethylbenzene

R.T.: 16.407 min
Delta R.T.: -0.005 min
Response: 150945
Conc: 6.22 ng/ml