

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082020\
 Data File : FB024768.D
 Signal(s) : FID2B.CH
 Acq On : 20 Aug 2020 11:22
 Operator : DD/AJ
 Sample : L3496-02MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 21 01:34:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
 Quant Title :
 QLast Update : Mon Aug 10 12:11:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	442837	21.446 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	629690	26.166 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	693078	25.003 ng/ml
3) t n-Heptane	7.755	75597	2.780 ng/ml
4) t Benzene	7.891	349897	9.970 ng/ml
6) t Toluene	10.629	970868	28.185 ng/ml
7) t Ethylbenzene	13.068	267214	8.347 ng/ml
8) t m-Xylene	13.200	498967	15.990 ng/ml
9) t O-Xylene	13.928	510537	16.881 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	265937	10.828 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082020\
Data File : FB024768.D
Signal(s) : FID2B.CH
Acq On : 20 Aug 2020 11:22
Operator : DD/AJ
Sample : L3496-02MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 21 01:34:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB081020.M
Quant Title :
QLast Update : Mon Aug 10 12:11:06 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

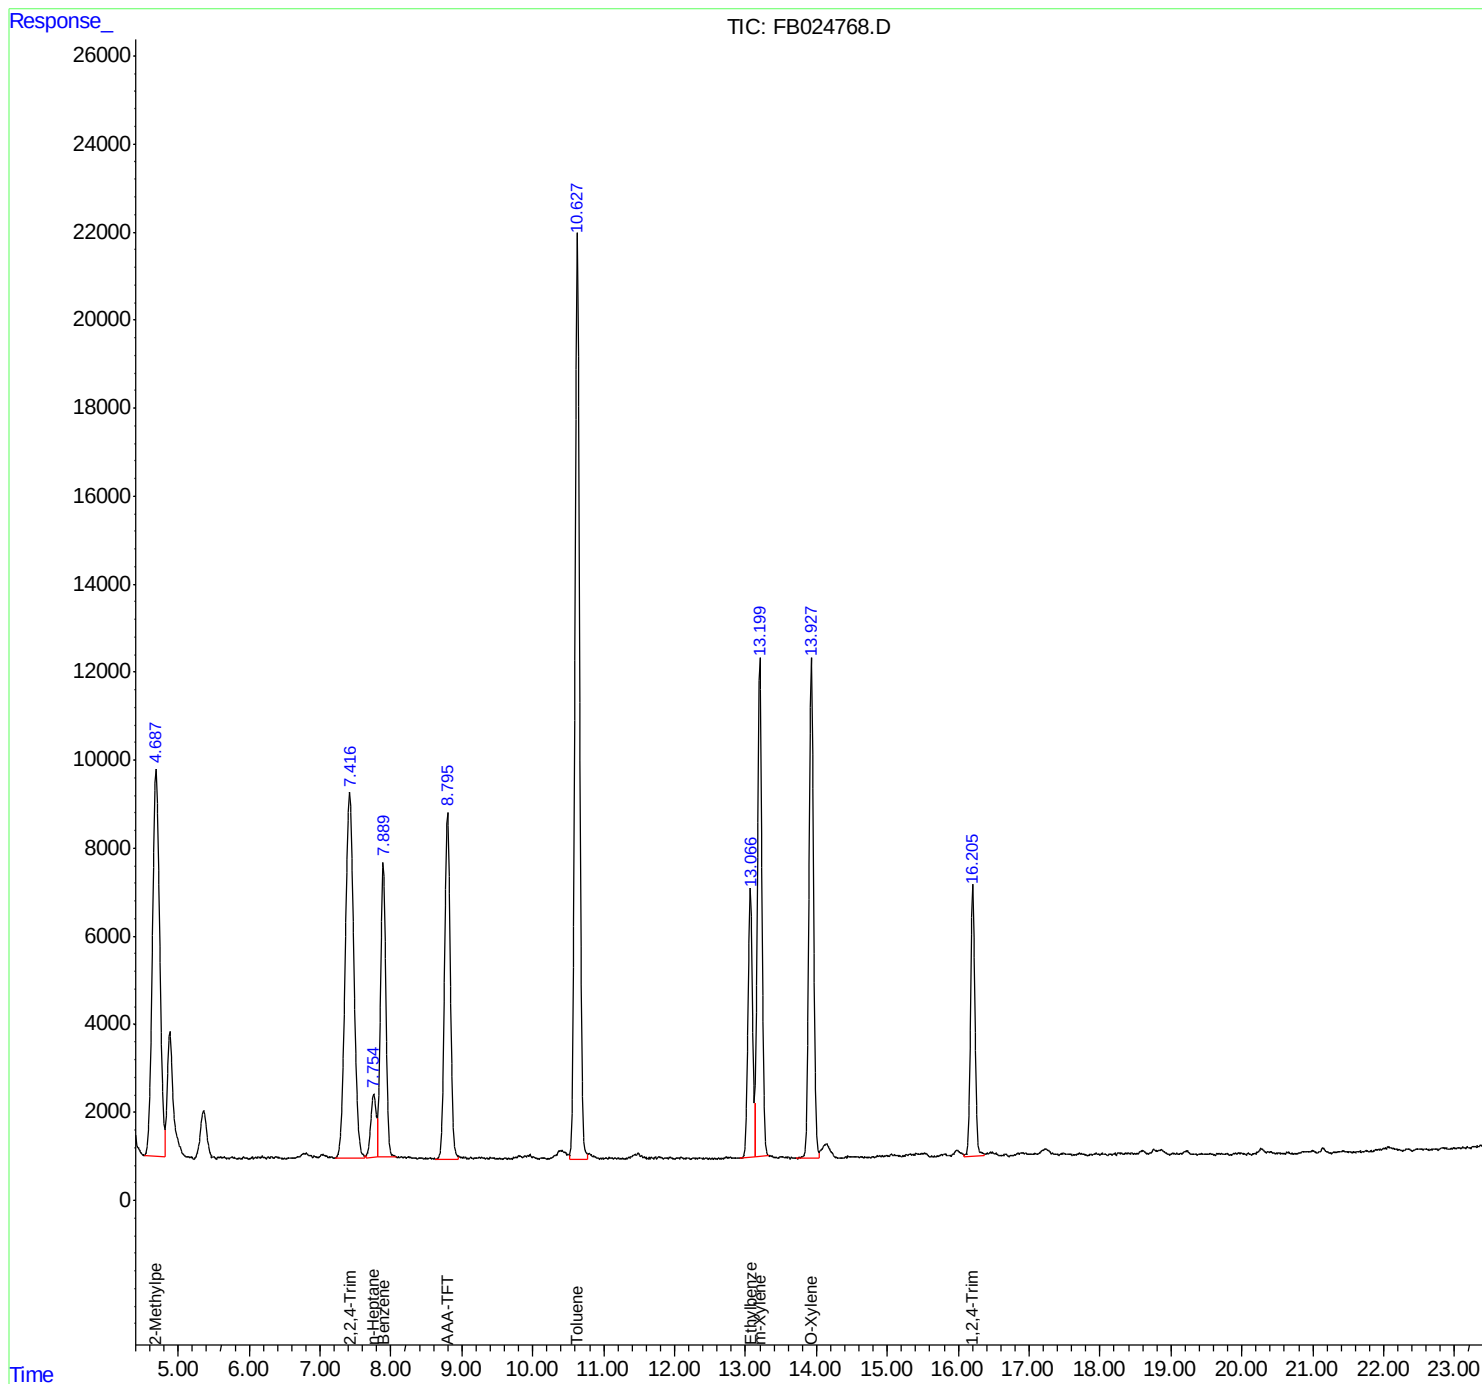

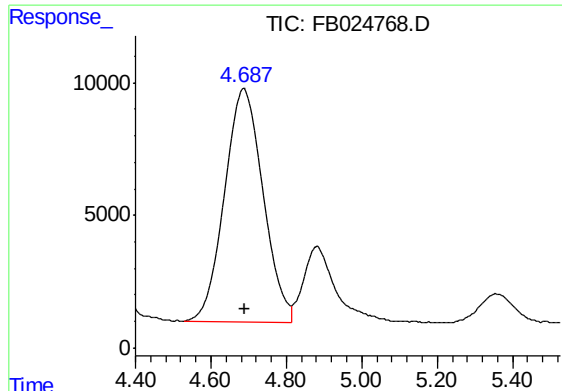


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 629690
Conc: 26.17 ng/ml

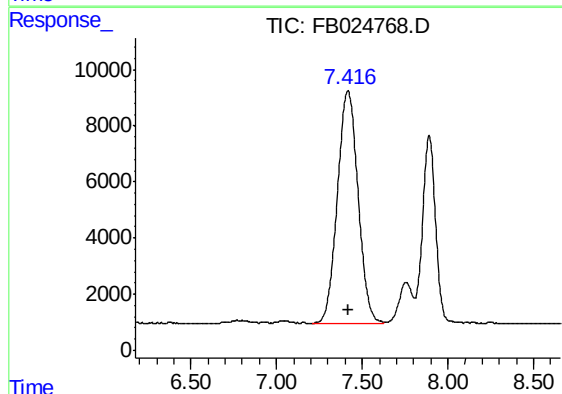


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 693078
Conc: 25.00 ng/ml

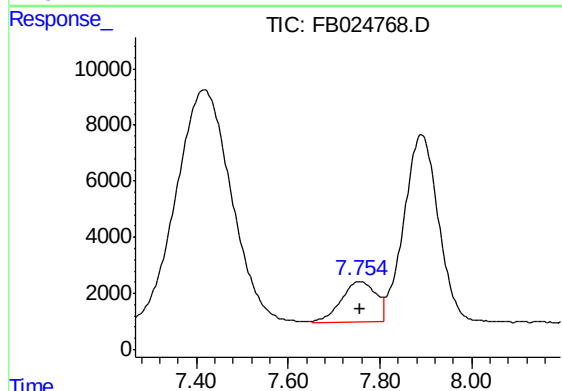


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.002 min
Response: 75597
Conc: 2.78 ng/ml

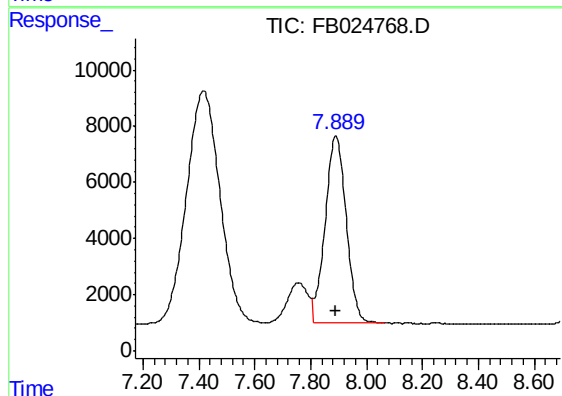


#4 Benzene

R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 349897
Conc: 9.97 ng/ml

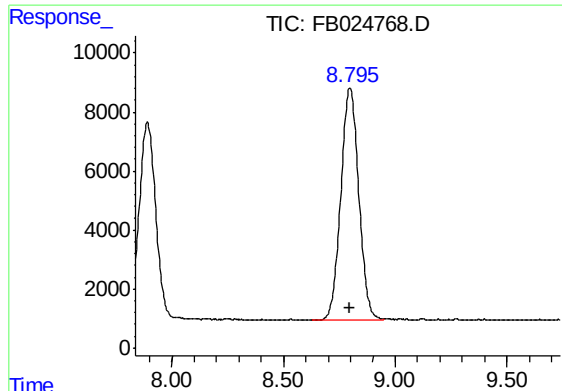


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 442837
Conc: 21.45 ng/ml

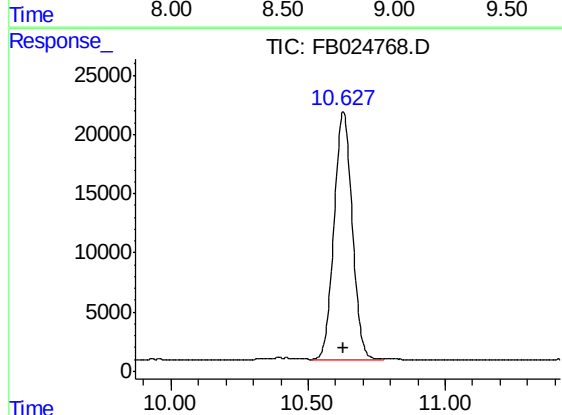


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 970868
Conc: 28.18 ng/ml

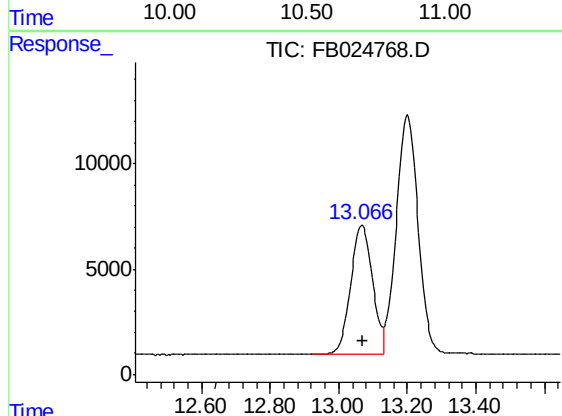


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.002 min
Response: 267214
Conc: 8.35 ng/ml

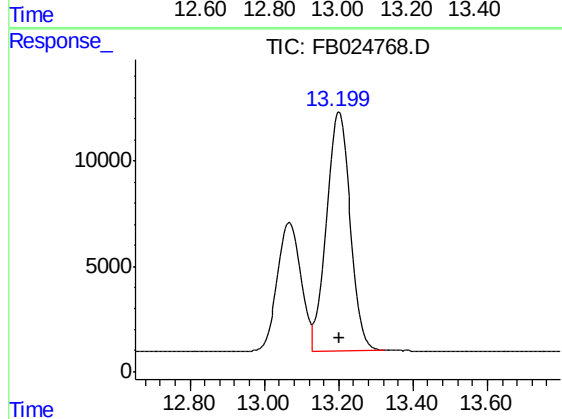


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.001 min
Response: 498967
Conc: 15.99 ng/ml

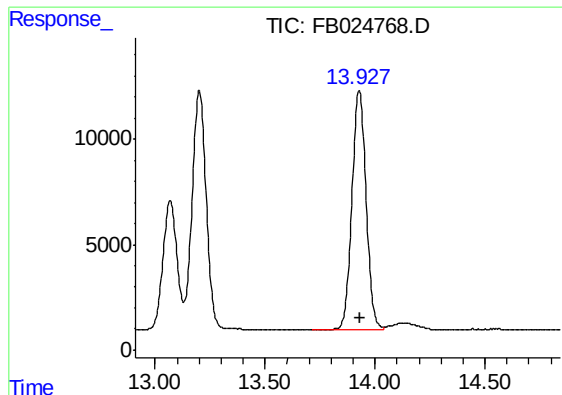

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.000 min
Response: 510537
Conc: 16.88 ng/ml

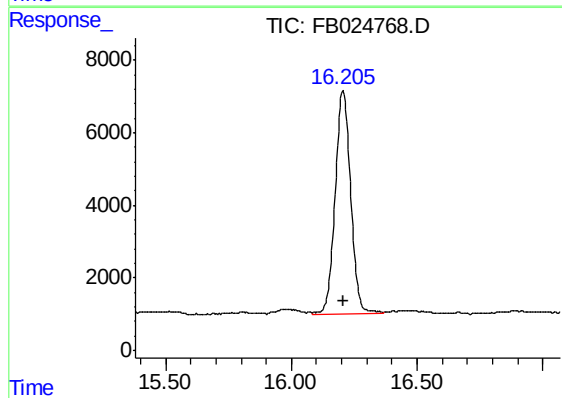

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.000 min
Response: 265937
Conc: 10.83 ng/ml