

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082020\  
Data File : FB024769.D  
Signal(s) : FID2B.CH  
Acq On : 20 Aug 2020 11:53  
Operator : DD/AJ  
Sample : L3502-12  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Aug 21 01:34:22 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB081020.M  
Quant Title :  
QLast Update : Mon Aug 10 12:11:06 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.797  | 489070   | 23.685 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.625 | 6475     | 0.188 ng/ml  |
| 7) t Ethylbenzene            | 13.051 | 5649     | 0.176 ng/ml  |
| 8) t m-Xylene                | 13.197 | 6475     | 0.207 ng/ml  |
| 9) t O-Xylene                | 13.914 | 1839     | 0.061 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.211 | 506      | 0.021 ng/ml  |
| -----                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082020\  
Data File : FB024769.D  
Signal(s) : FID2B.CH  
Acq On : 20 Aug 2020 11:53  
Operator : DD/AJ  
Sample : L3502-12  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Aug 21 01:34:22 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB081020.M  
Quant Title :  
QLast Update : Mon Aug 10 12:11:06 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

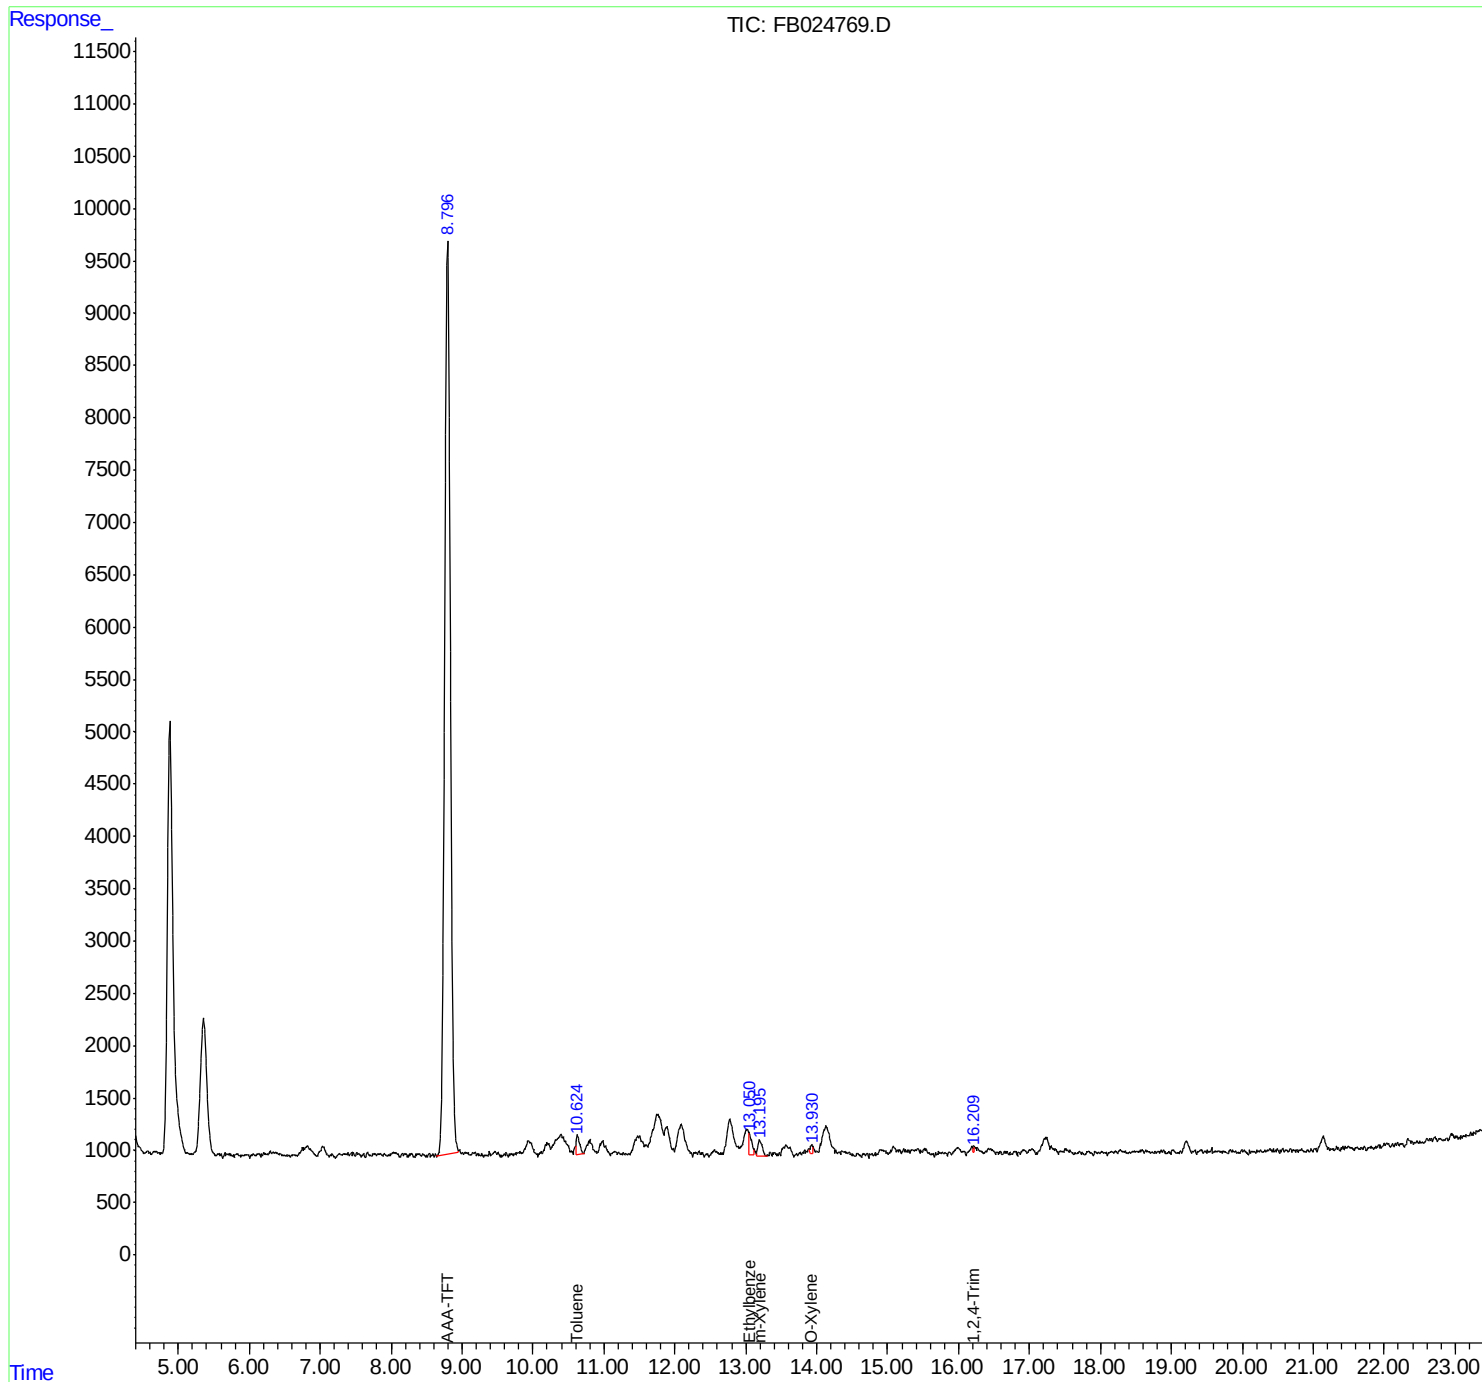

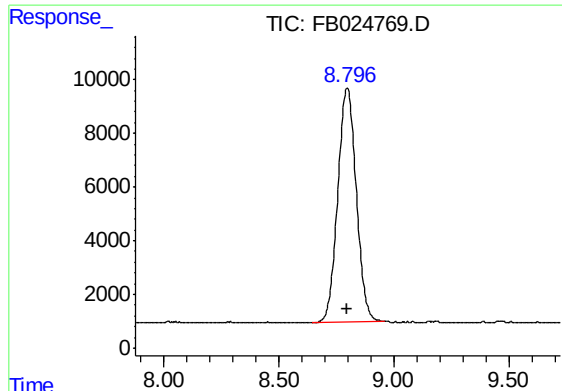


#5 AAA-TFT

R.T.: 8.797 min  
Delta R.T.: -0.002 min  
Response: 489070  
Conc: 23.68 ng/ml

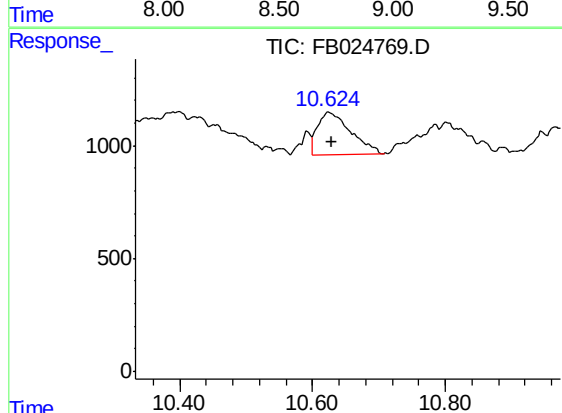


#6 Toluene

R.T.: 10.625 min  
Delta R.T.: -0.004 min  
Response: 6475  
Conc: 0.19 ng/ml

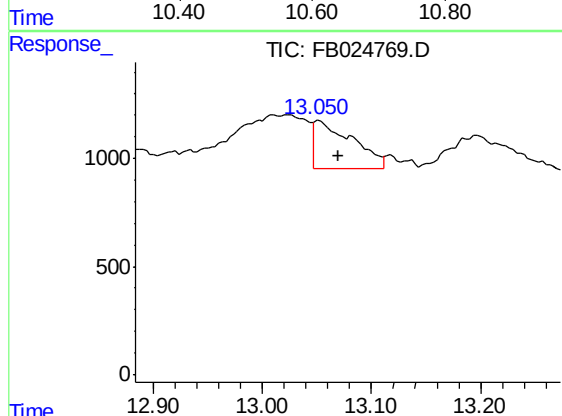


#7 Ethylbenzene

R.T.: 13.051 min  
Delta R.T.: -0.018 min  
Response: 5649  
Conc: 0.18 ng/ml

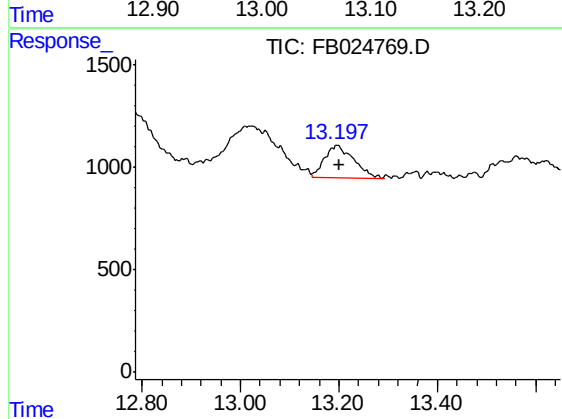


#8 m-Xylene

R.T.: 13.197 min  
Delta R.T.: -0.005 min  
Response: 6475  
Conc: 0.21 ng/ml

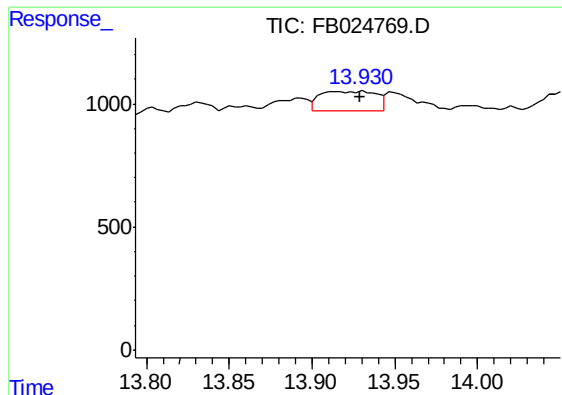

#9 O-Xylene

R.T.: 13.914 min  
Delta R.T.: -0.015 min  
Response: 1839  
Conc: 0.06 ng/ml

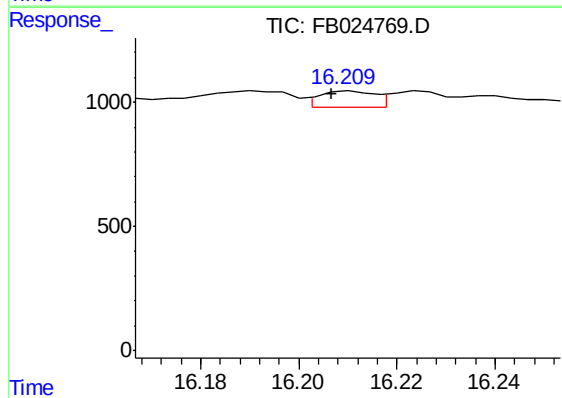

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min  
Delta R.T.: 0.004 min  
Response: 506  
Conc: 0.02 ng/ml