

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082118\
 Data File : FB017478.D
 Signal(s) : FID2B.CH
 Acq On : 21 Aug 2018 10:42
 Operator : MJ/SJ
 Sample : J4555-03MSD
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 21 11:06:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
 Quant Title :
 QLast Update : Mon Aug 20 13:42:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.111	167230	20.283 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	441925	31.538 ng/ml
2) t 2,2,4-Trimethylpentane	7.727	404089	28.675 ng/ml
3) t n-Heptane	8.067	128761	9.343 ng/ml
4) t Benzene	8.206	186457	10.576 ng/ml
6) t Toluene	10.960	449352	31.236 ng/ml
7) t Ethylbenzene	13.410	146933	9.963 ng/ml
8) t m-Xylene	13.542	308873	19.869 ng/ml
9) t O-Xylene	14.274	328106	19.988 ng/ml
10) t 1,2,4-Trimethylbenzene	16.557	383697	19.700 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082118\
Data File : FB017478.D
Signal(s) : FID2B.CH
Acq On : 21 Aug 2018 10:42
Operator : MJ/SJ
Sample : J4555-03MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 21 11:06:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082018.M
Quant Title :
QLast Update : Mon Aug 20 13:42:39 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

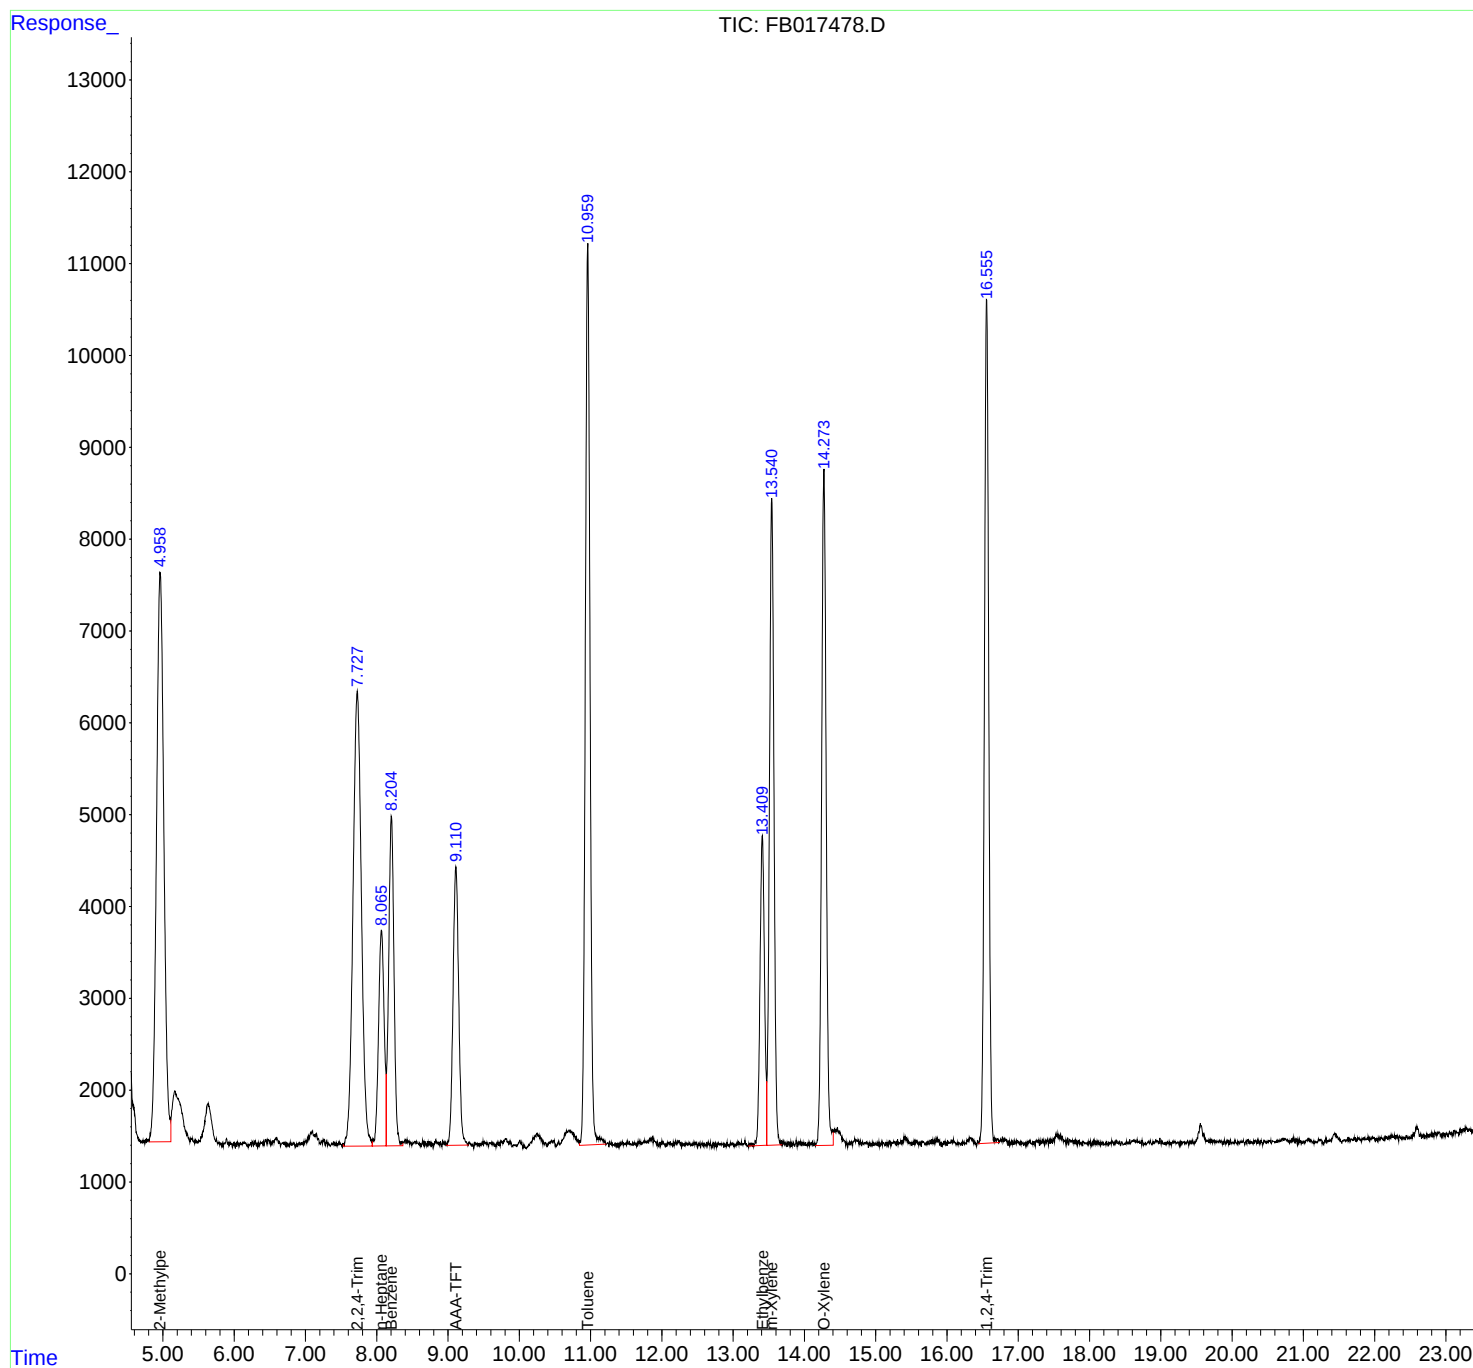

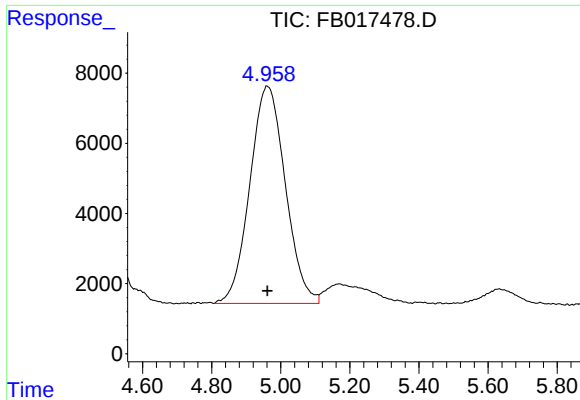


#1 2-Methylpentane

R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 441925
Conc: 31.54 ng/ml

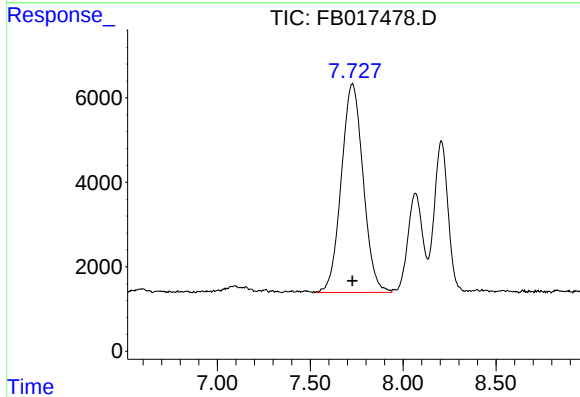


#2 2,2,4-Trimethylpentane

R.T.: 7.727 min
Delta R.T.: 0.000 min
Response: 404089
Conc: 28.68 ng/ml

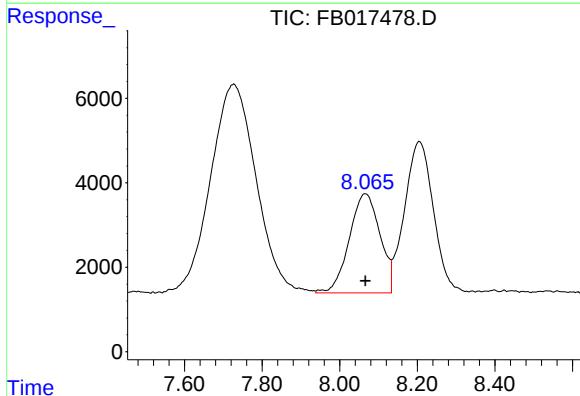


#3 n-Heptane

R.T.: 8.067 min
Delta R.T.: 0.001 min
Response: 128761
Conc: 9.34 ng/ml

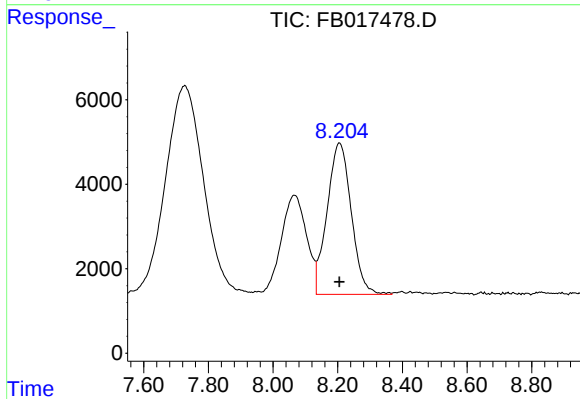


#4 Benzene

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 186457
Conc: 10.58 ng/ml

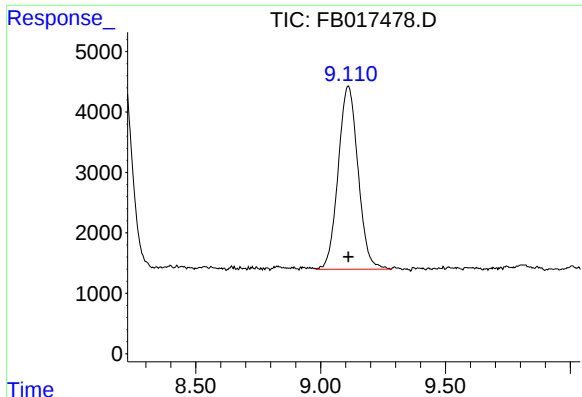


#5 AAA-TFT

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 167230
Conc: 20.28 ng/ml

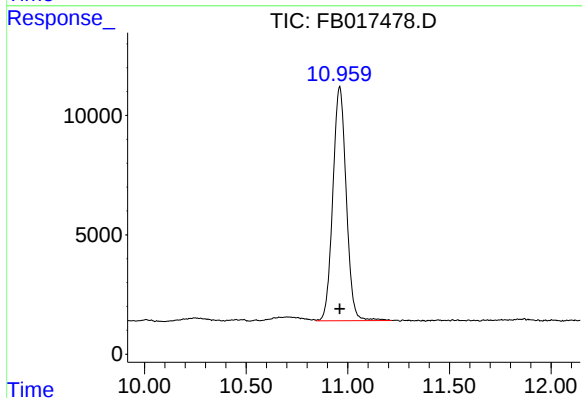


#6 Toluene

R.T.: 10.960 min
Delta R.T.: 0.000 min
Response: 449352
Conc: 31.24 ng/ml

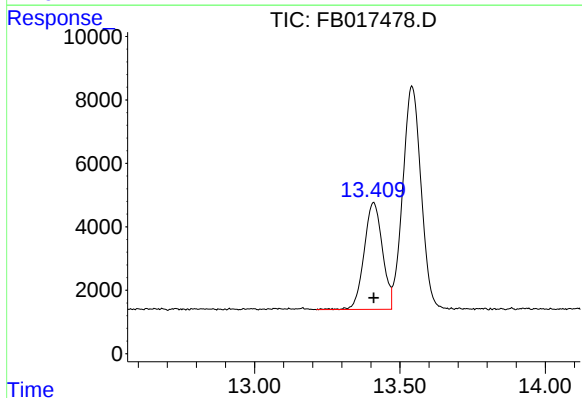


#7 Ethylbenzene

R.T.: 13.410 min
Delta R.T.: -0.001 min
Response: 146933
Conc: 9.96 ng/ml

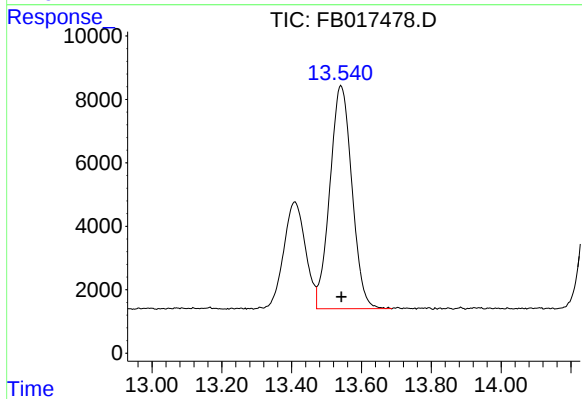


#8 m-Xylene

R.T.: 13.542 min
Delta R.T.: 0.000 min
Response: 308873
Conc: 19.87 ng/ml

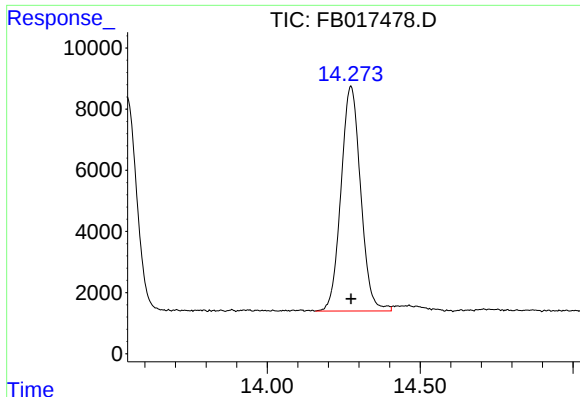

#9 O-Xylene

R.T.: 14.274 min
Delta R.T.: 0.000 min
Response: 328106
Conc: 19.99 ng/ml

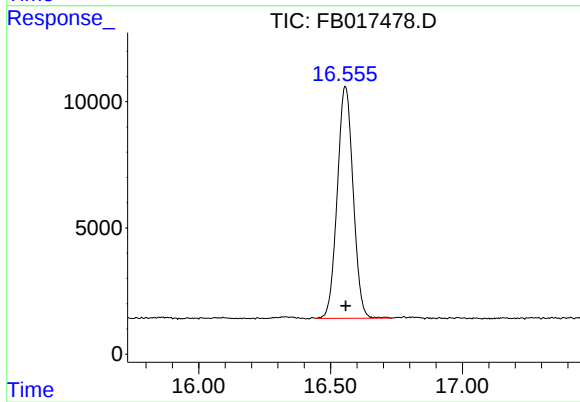

#10 1,2,4-Trimethylbenzene

R.T.: 16.557 min
Delta R.T.: 0.000 min
Response: 383697
Conc: 19.70 ng/ml